

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100318\
 Data File : BM016978.D
 Acq On : 03 Oct 2018 15:37
 Operator : MJ/SJ
 Sample : J5115-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 04 01:53:19 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 04 01:52:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	200182	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	829540	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.34	164	422658	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	922706	20.00	ng/ul	0.00
78) Chrysene-d12	21.29	240	1031316	20.00	ng/ul	0.00
86) Perylene-d12	23.52	264	1106264	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	9927	2.12	ng/uL	0.00
5) Phenol-d5	6.88	99	199905	11.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	134318	12.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	178622	12.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	156226	11.96	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	80457	14.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	80407	16.23	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	156516	12.43	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	214879	14.13	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	455073	13.41	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	580285	13.24	ng/ul	0.00
52) 4-Nitrophenol-d4	14.55	143	34019	6.11	ng/ul	0.00
58) Fluorene-d10	15.34	176	407034	13.74	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.46	200	30104	7.95	ng/ul	0.00
71) Anthracene-d10	17.19	188	614619	13.81	ng/ul	0.00
79) Pyrene-d10	19.49	212	695072	13.89	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.37	264	813136	14.09	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.90	94	17380	1.031	ng/ul 99
45) Dimethylphthalate	13.81	163	124831	3.764	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100318\
Data File : BM016978.D
Acq On : 03 Oct 2018 15:37
Operator : MJ/SJ
Sample : J5115-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 04 01:53:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 04 01:52:46 2018
Response via : Initial Calibration

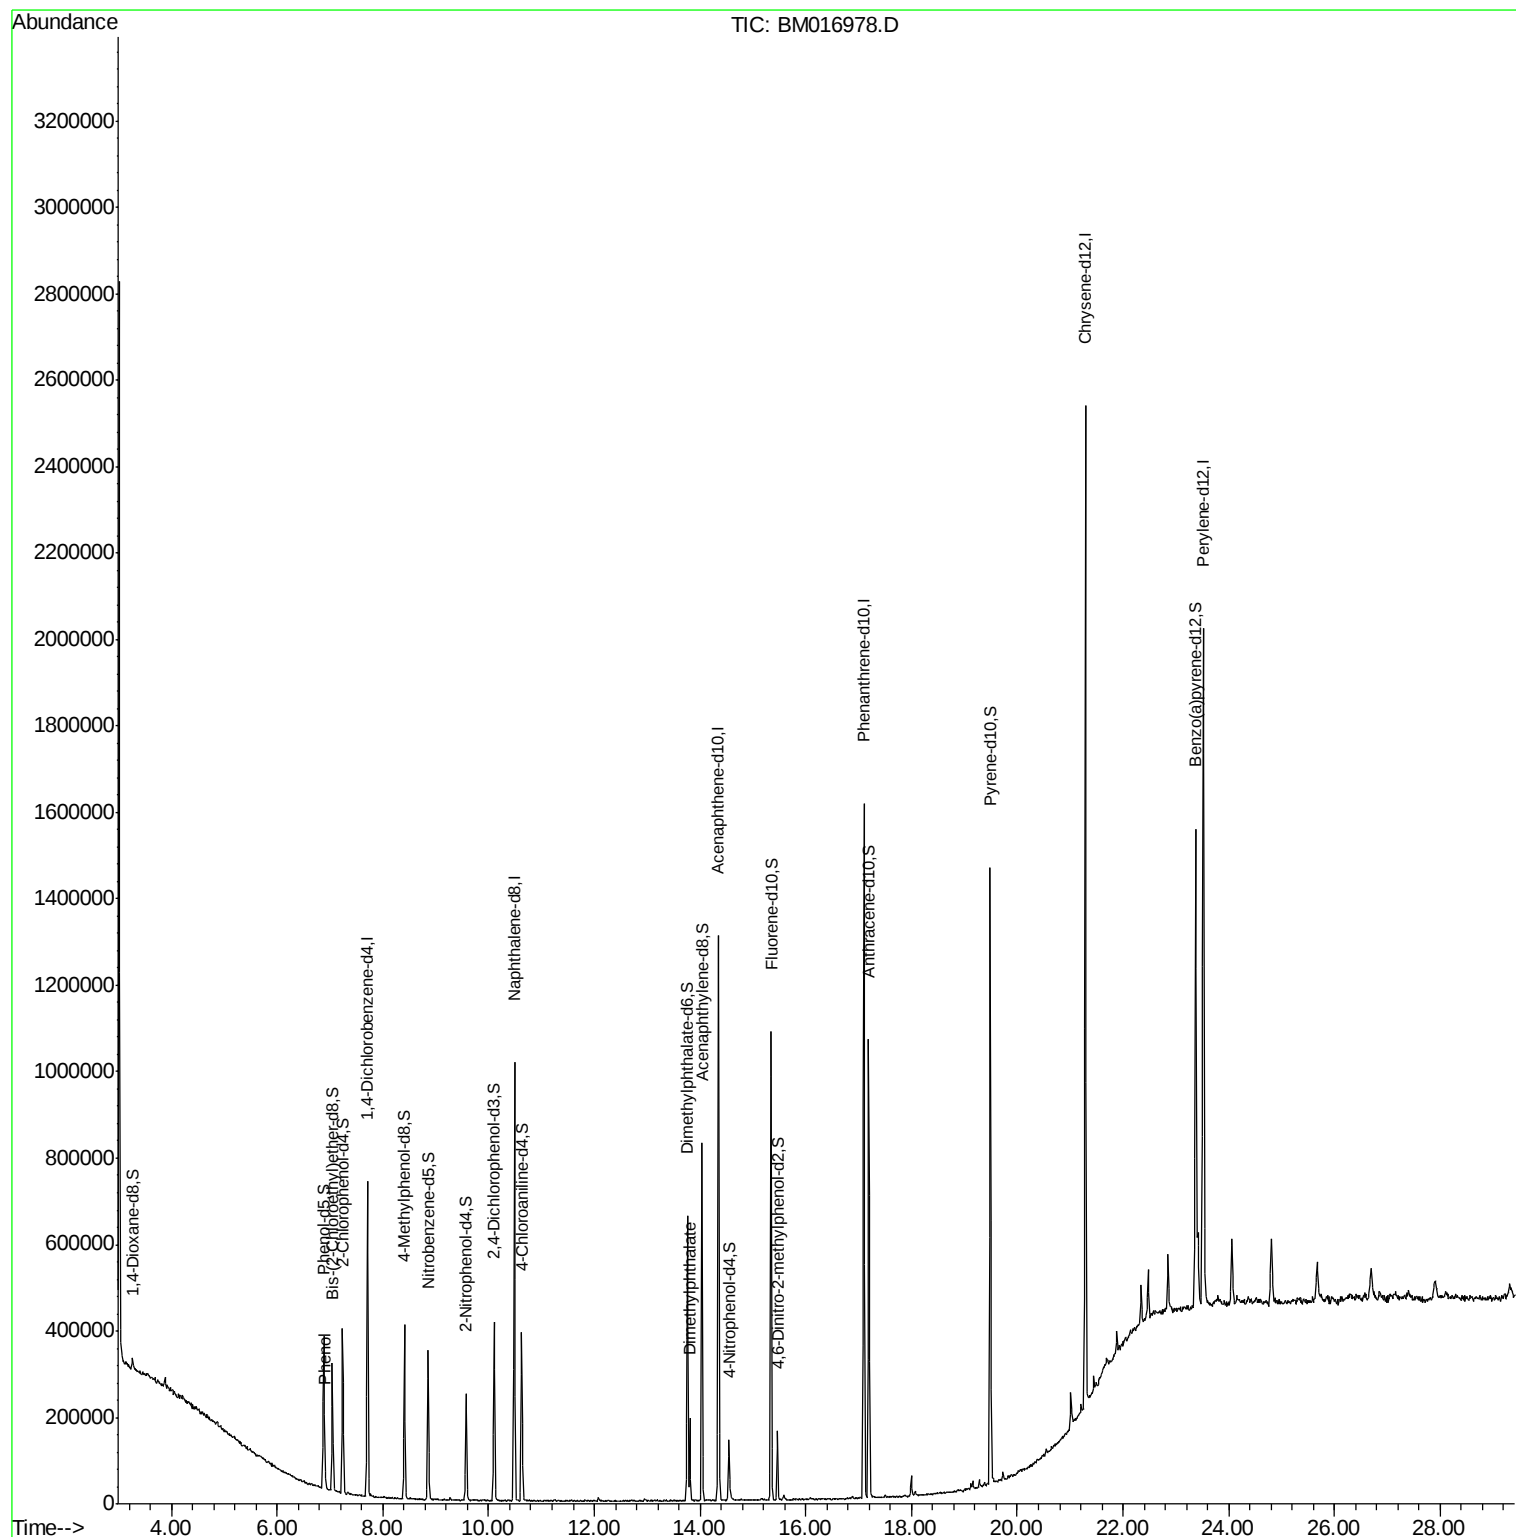

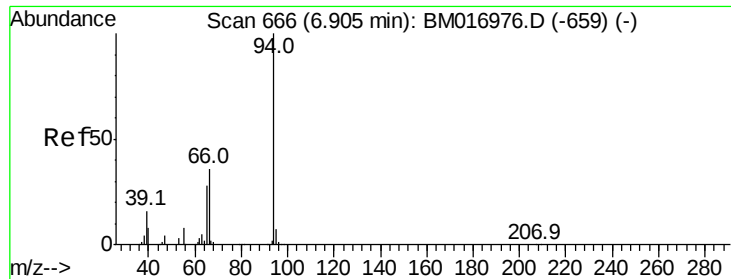

#6

Phenol

Concen: 1.031 ng/ul

RT: 6.90 min Scan# 666

Delta R.T. -0.00 min

Lab File: BM016978.D

Acq: 03 Oct 2018 15:37


Instrument :

BNA_M

ClientSampleId :

Tot Ion: 94 Resp: 17380

Ion	Ratio	Lower	Upper
94	100		
65	28.8	23.0	34.6
66	38.8	30.4	45.6



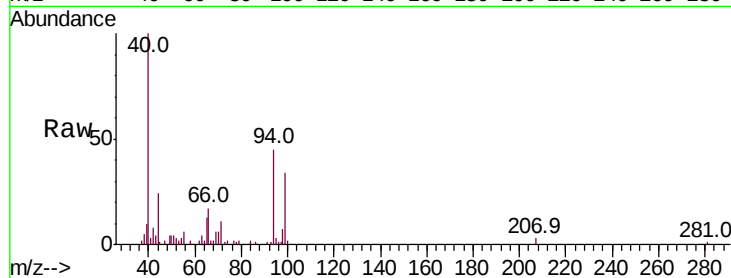


Abundance

Ion 94.00 (93.70 to 94.70): BM016976.D (-659) (-)

Ion 65.00 (64.70 to 65.70): BM016976.D (-659) (-)

Ion 66.00 (65.70 to 66.70): BM016976.D (-659) (-)

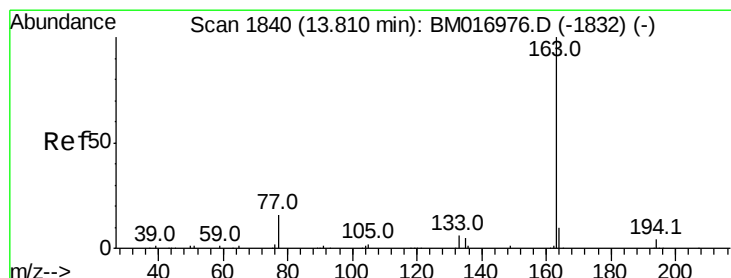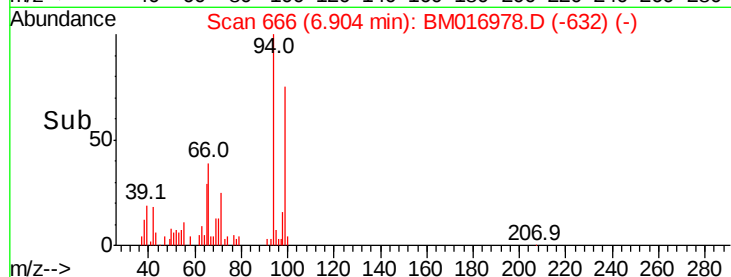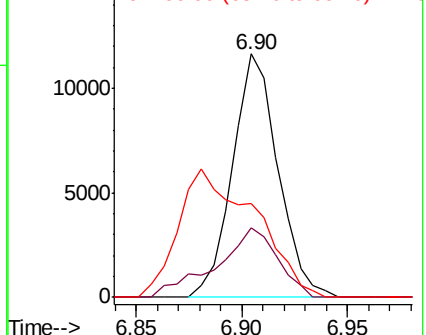

#45

Dimethylphthalate

Concen: 3.764 ng/ul

RT: 13.81 min Scan# 1840


Delta R.T. -0.00 min

Lab File: BM016978.D

Acq: 03 Oct 2018 15:37

Tgt Ion: 163 Resp: 124831

Ion	Ratio	Lower	Upper
163	100		
194	5.0	4.0	6.0
164	10.0	8.4	12.6

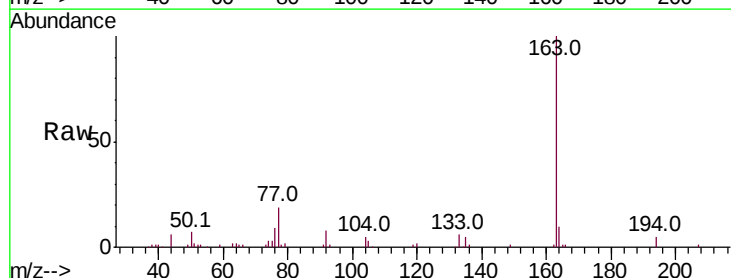

Abundance

Ion 163.00 (162.70 to 163.70): BM016976.D (-1832) (-)

Ion 194.00 (193.70 to 194.70): BM016976.D (-1832) (-)

Ion 164.00 (163.70 to 164.70): BM016976.D (-1832) (-)

