

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100318\
 Data File : BM016981.D
 Acq On : 03 Oct 2018 17:25
 Operator : MJ/SJ
 Sample : J5115-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 04 01:53:36 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 04 01:52:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	209988	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	863560	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.35	164	454285	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	1015184	20.00	ng/ul	0.00
78) Chrysene-d12	21.29	240	1130941	20.00	ng/ul	0.00
86) Perylene-d12	23.52	264	1209549	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.26	96	16375	3.33	ng/uL	0.00
5) Phenol-d5	6.88	99	361368	20.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	226380	20.64	ng/ul	0.00
9) 2-Chlorophenol-d4	7.24	132	309482	21.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	290769	21.22	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	146295	25.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	151270	29.33	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	287978	21.97	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	402564	25.44	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	880155	24.13	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	1124245	23.86	ng/ul	0.00
52) 4-Nitrophenol-d4	14.55	143	114762	19.17	ng/ul	0.00
58) Fluorene-d10	15.34	176	794286	24.95	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.46	200	85322	20.47	ng/ul	0.00
71) Anthracene-d10	17.19	188	1216893	24.84	ng/ul	0.00
79) Pyrene-d10	19.49	212	1376397	25.08	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.38	264	1591059	25.22	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.90	94	23778	1.345	ng/ul	95
45) Dimethylphthalate	13.80	163	273659	7.677	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100318\
Data File : BM016981.D
Acq On : 03 Oct 2018 17:25
Operator : MJ/SJ
Sample : J5115-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 04 01:53:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 04 01:52:46 2018
Response via : Initial Calibration

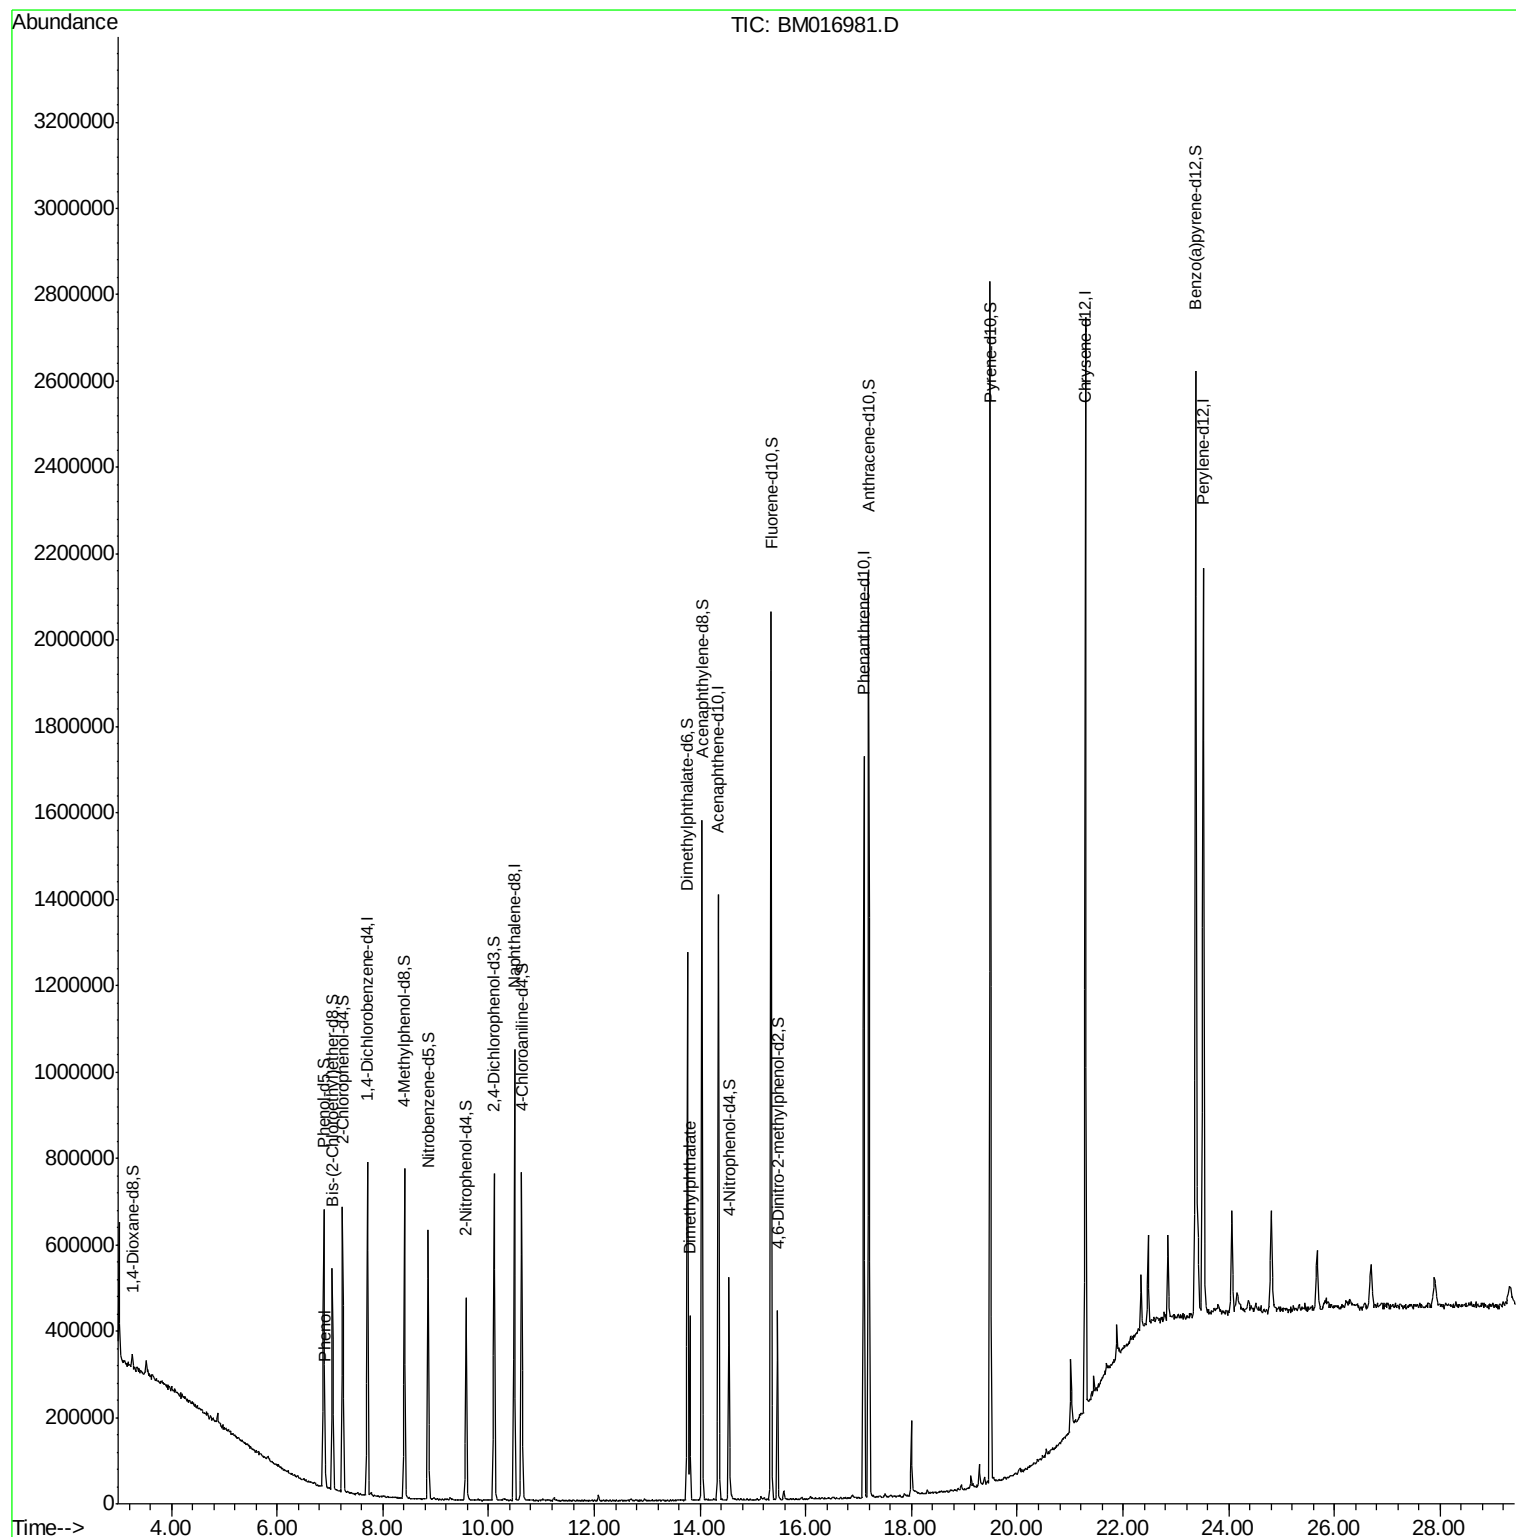

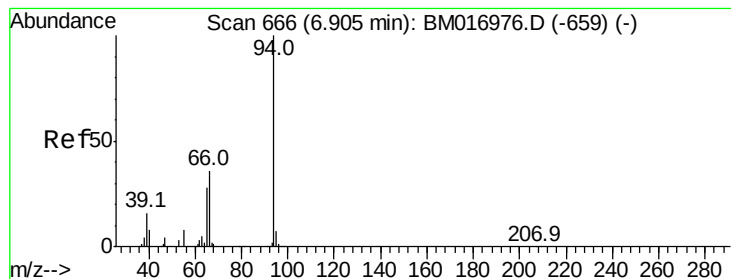

#6

Phenol

Concen: 1.345 ng/ul

RT: 6.90 min Scan# 666

Delta R.T. -0.00 min

Lab File: BM016981.D

Acq: 03 Oct 2018 17:25


Instrument :

BNA_M

ClientSampleId :

Tot Ion: 94 Resp: 23778

Ion	Ratio	Lower	Upper
94	100		
65	31.9	23.0	34.6
66	41.1	30.4	45.6



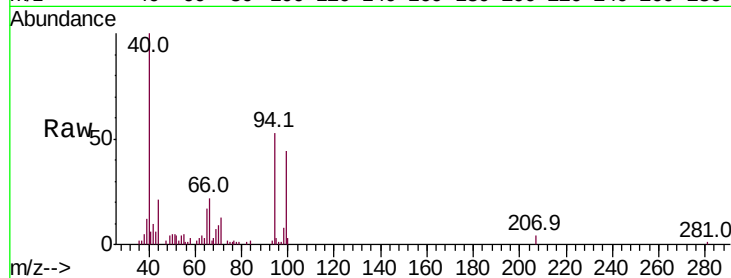


Abundance

Ion 94.00 (93.70 to 94.70): BM016976.D (-659) (-)

Ion 65.00 (64.70 to 65.70): BM016976.D (-659) (-)

Ion 66.00 (65.70 to 66.70): BM016976.D (-659) (-)

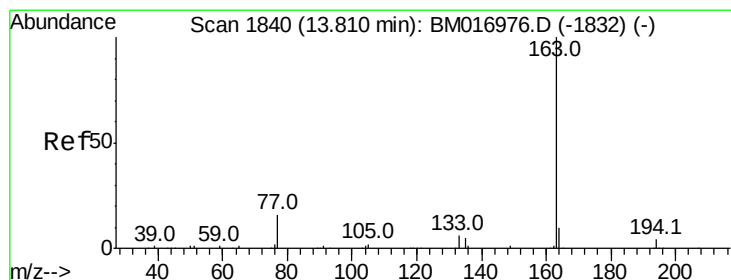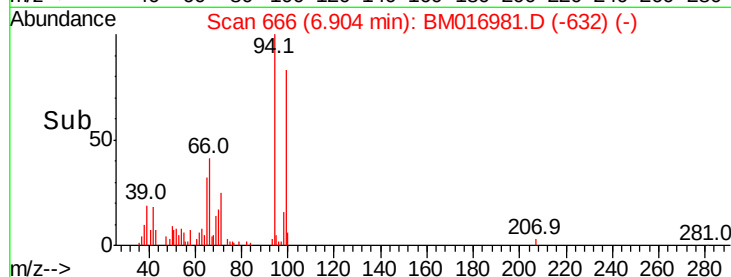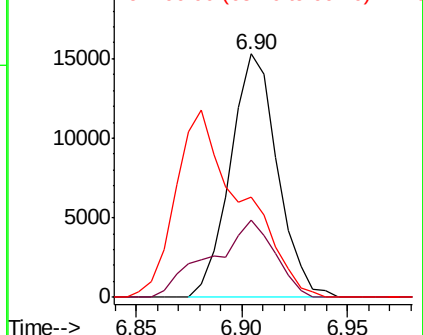

#45

Dimethylphthalate

Concen: 7.677 ng/ul

RT: 13.80 min Scan# 1839


Delta R.T. -0.01 min

Lab File: BM016981.D

Acq: 03 Oct 2018 17:25

Tgt Ion:163 Resp: 273659

Ion	Ratio	Lower	Upper
163	100		
194	4.3	4.0	6.0
164	10.5	8.4	12.6

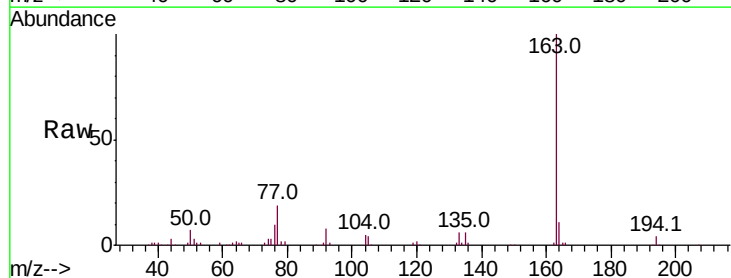

Abundance

Ion 163.00 (162.70 to 163.70): BM016976.D (-1832) (-)

Ion 194.00 (193.70 to 194.70): BM016976.D (-1832) (-)

Ion 164.00 (163.70 to 164.70): BM016976.D (-1832) (-)

