

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100318\
 Data File : BM016987.D
 Acq On : 03 Oct 2018 21:01
 Operator : MJ/SJ
 Sample : PB113406BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 04 01:54:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 04 01:52:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	226692	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	929638	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.34	164	478155	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	1067384	20.00	ng/ul	0.00
78) Chrysene-d12	21.29	240	1192513	20.00	ng/ul	0.00
86) Perylene-d12	23.51	264	1266659	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	30367	5.73	ng/uL	0.00
5) Phenol-d5	6.88	99	624040	32.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	390451	32.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.24	132	545163	34.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	494152	33.40	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	252077	41.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	259869	46.80	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	486306	34.46	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	668175	39.22	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	1348524	35.12	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	1795691	36.21	ng/ul	0.00
52) 4-Nitrophenol-d4	14.55	143	197153	31.29	ng/ul	0.00
58) Fluorene-d10	15.34	176	1206273	36.00	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.46	200	136865	31.24	ng/ul	0.00
71) Anthracene-d10	17.19	188	1824560	35.43	ng/ul	0.00
79) Pyrene-d10	19.49	212	2012887	34.79	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.38	264	2399701	36.32	ng/ul	0.00


Target Compounds				Ovalue	
46) 2,6-Dinitrotoluene	13.76	165	10383	1.802	ng/ul# 40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100318\
Data File : BM016987.D
Acq On : 03 Oct 2018 21:01
Operator : MJ/SJ
Sample : PB113406BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 04 01:54:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 04 01:52:46 2018
Response via : Initial Calibration

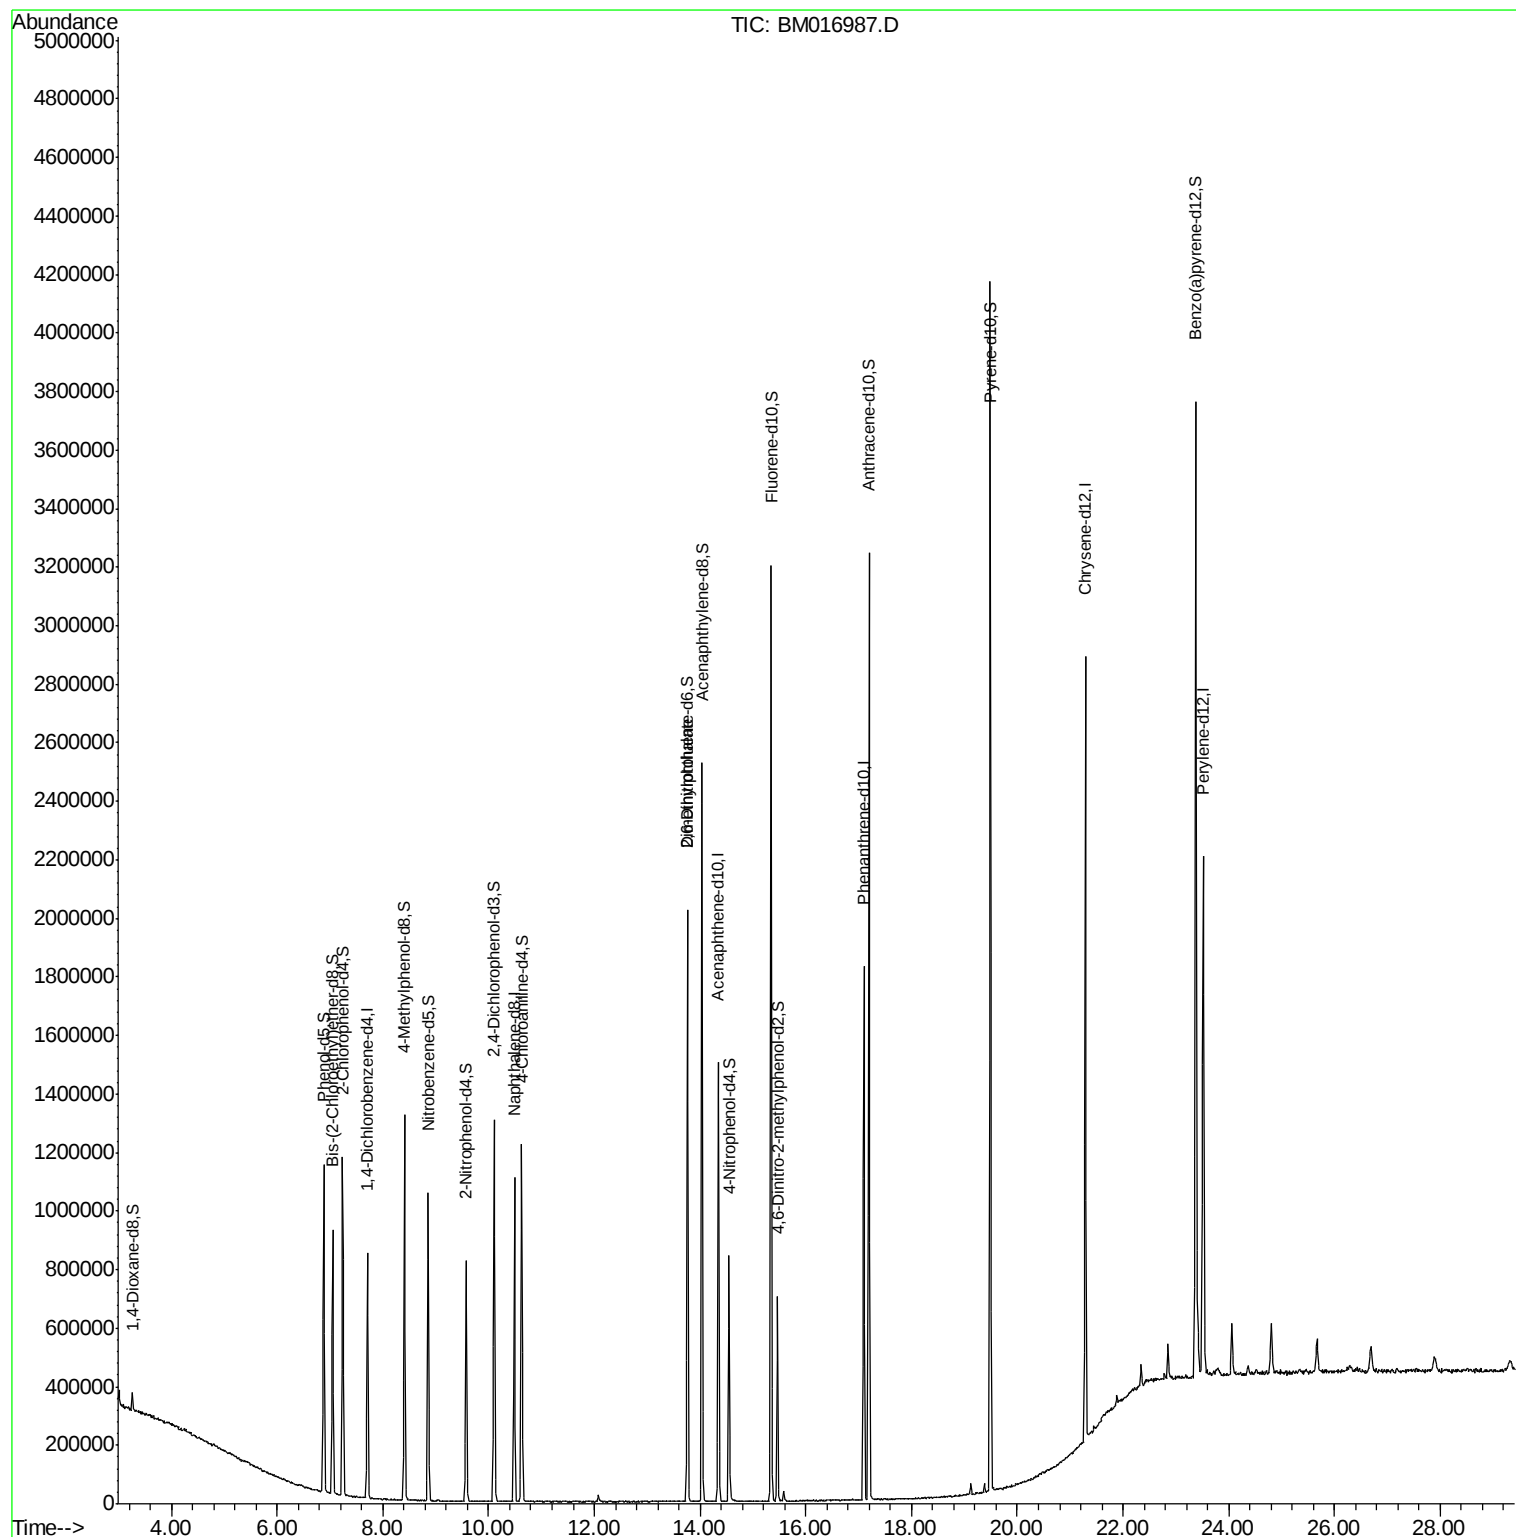

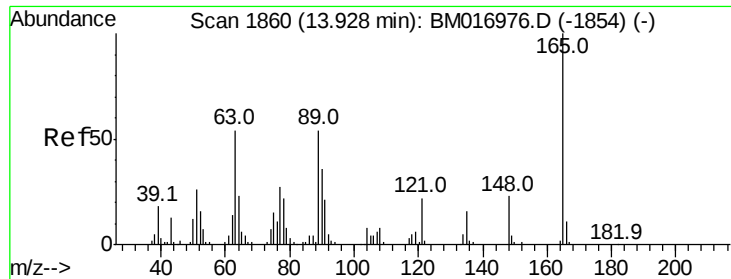

#46
 2,6-Dinitrotoluene
 Concen: 1.802 ng/ul
 RT: 13.76 min Scan# 1832
 Delta R.T. -0.17 min
 Lab File: BM016987.D
 Acq: 03 Oct 2018 21:01

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
89	0.0	43.8	65.8#
121	31.6	17.8	26.6#

