

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100318\
 Data File : BM016979.D
 Acq On : 03 Oct 2018 16:13
 Operator : MJ/SJ
 Sample : J5115-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLC12

Quant Time: Oct 04 01:53:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 04 01:52:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	215919	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	884983	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.34	164	466063	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	1017289	20.00	ng/ul	0.00
78) Chrysene-d12	21.29	240	1145123	20.00	ng/ul	0.00
86) Perylene-d12	23.51	264	1212627	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.26	96	16031	3.17	ng/uL	0.00
5) Phenol-d5	6.88	99	373645	20.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	234996	20.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	325524	21.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	295968	21.00	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	152243	26.18	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	154112	29.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.11	165	290952	21.66	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	412111	25.41	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	838978	22.42	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	1093929	22.63	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	95511	15.55	ng/ul	0.00
58) Fluorene-d10	15.34	176	751398	23.01	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.46	200	69826	16.72	ng/ul	0.00
71) Anthracene-d10	17.19	188	1135947	23.14	ng/ul	0.00
79) Pyrene-d10	19.49	212	1262187	22.72	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.37	264	1468180	23.21	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.90	94	24270	1.335	ng/ul	92
45) Dimethylphthalate	13.81	163	200664	5.487	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100318\
Data File : BM016979.D
Acq On : 03 Oct 2018 16:13
Operator : MJ/SJ
Sample : J5115-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLC12

Quant Time: Oct 04 01:53:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 04 01:52:46 2018
Response via : Initial Calibration

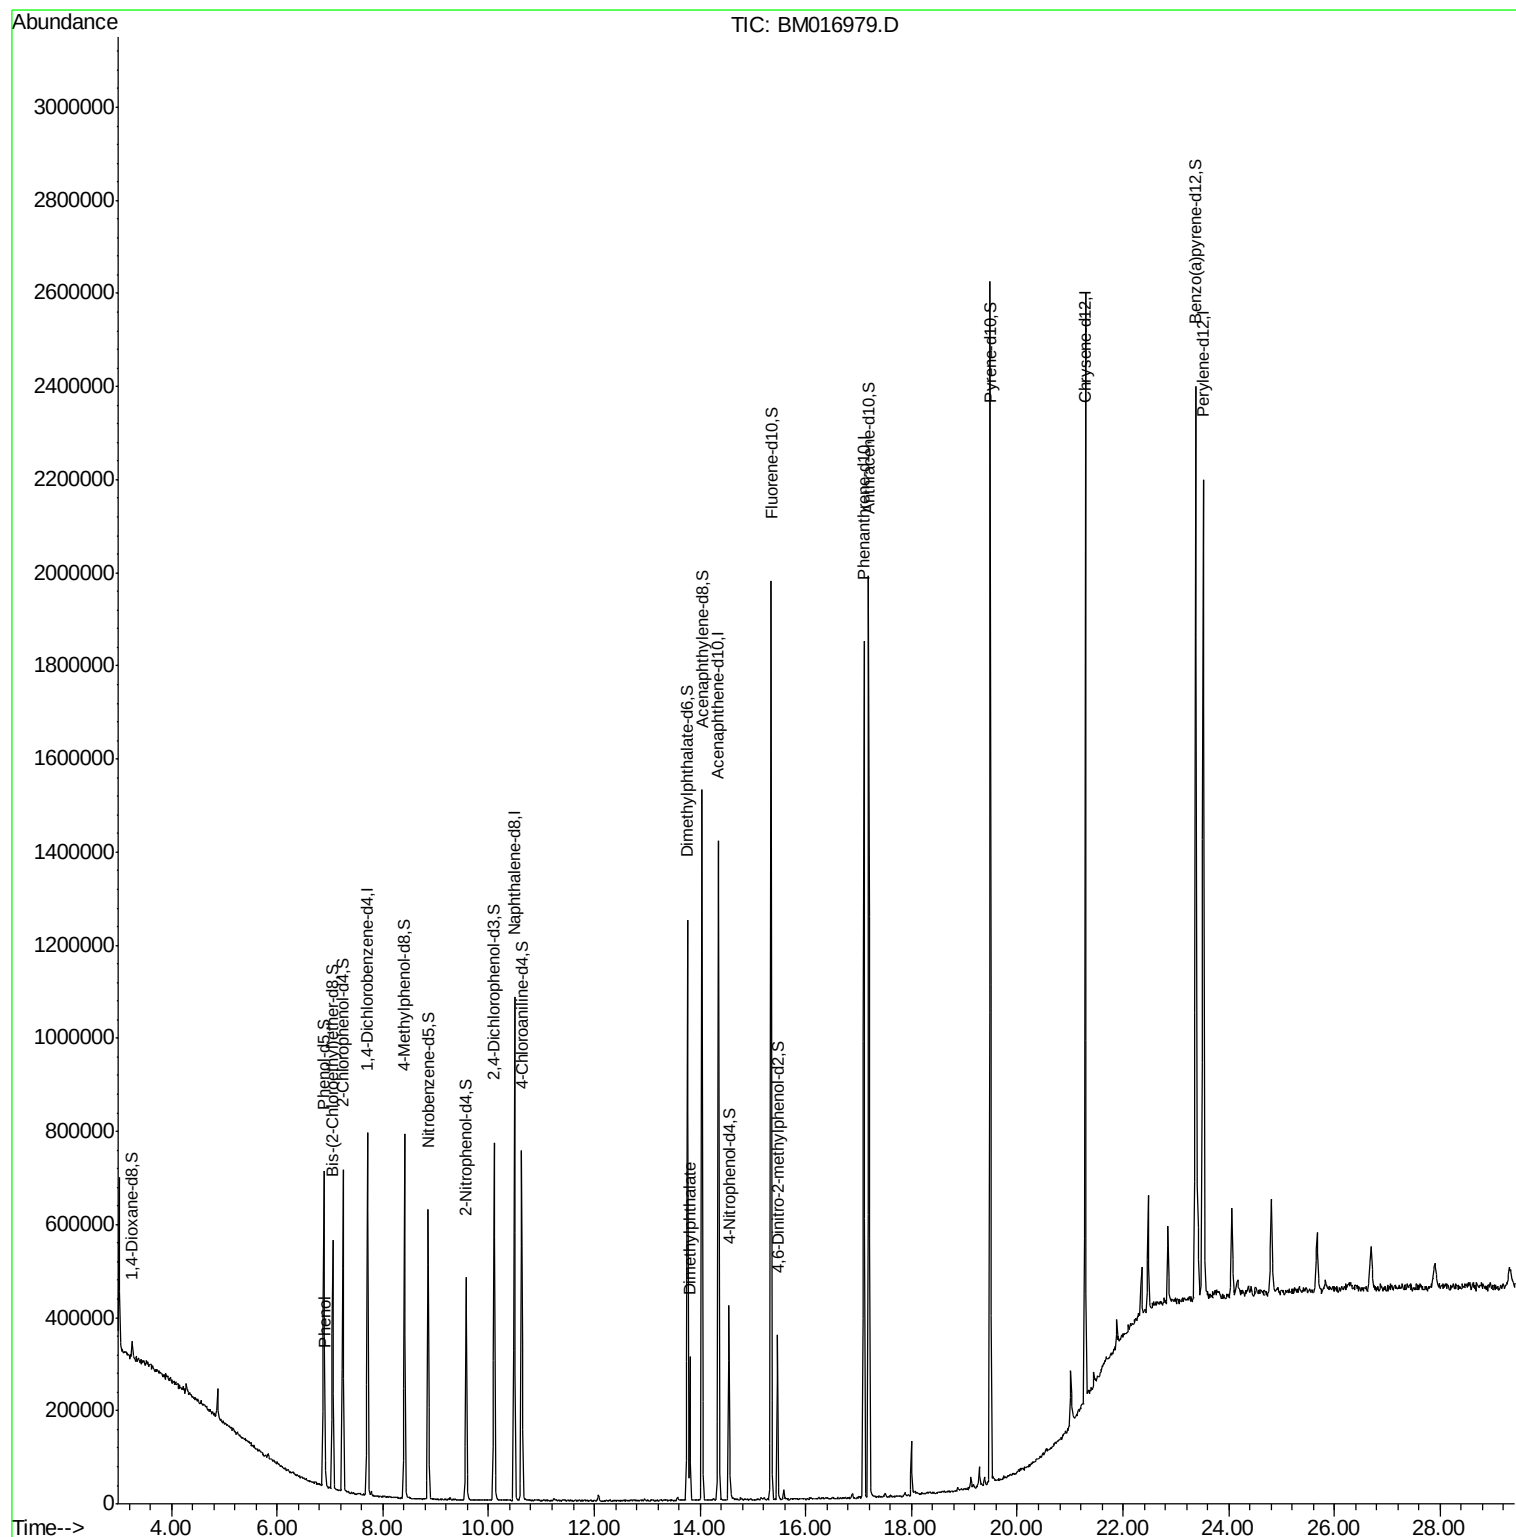

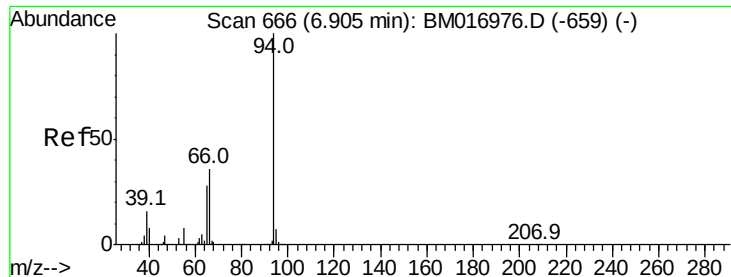

#6

Phenol

Concen: 1.335 ng/ul

RT: 6.90 min Scan# 666

Delta R.T. -0.00 min

Lab File: BM016979.D

Acq: 03 Oct 2018 16:13

Instrument :

BNA_M

ClientSampleId :

JLC12


Tot Ion: 94 Resp: 24270

Ion Ratio Lower Upper

94 100

65 30.1 23.0 34.6




66 45.5 30.4 45.6

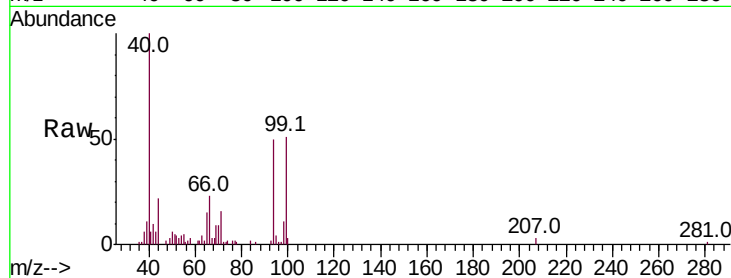

Abundance Ion 94.00 (93.70 to 94.70): BM016976.D (-659) (-)

Ion 65.00 (64.70 to 65.70): BM016976.D (-659) (-)

Ion 66.00 (65.70 to 66.70): BM016976.D (-659) (-)

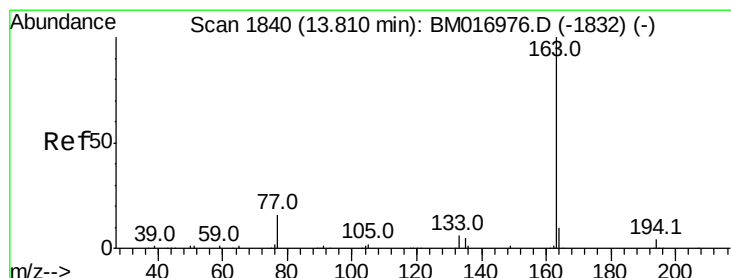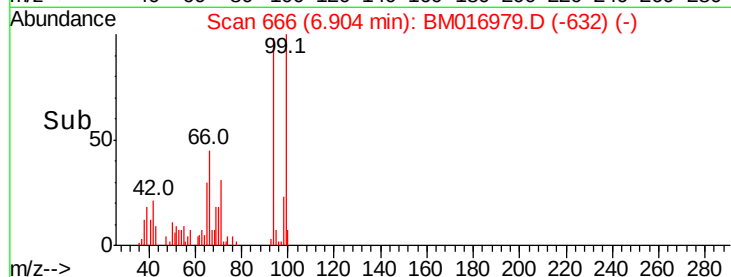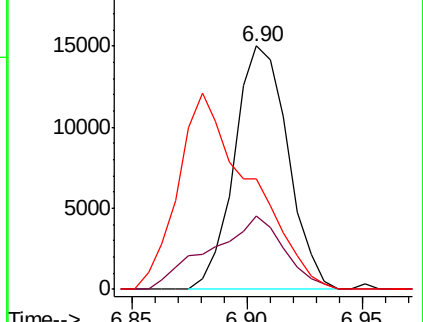

#45

Dimethylphthalate

Concen: 5.487 ng/ul

RT: 13.81 min Scan# 1840

Delta R.T. -0.00 min

Lab File: BM016979.D

Acq: 03 Oct 2018 16:13


Tgt Ion:163 Resp: 200664

Ion Ratio Lower Upper

163 100

194 4.3 4.0 6.0

164 10.1 8.4 12.6

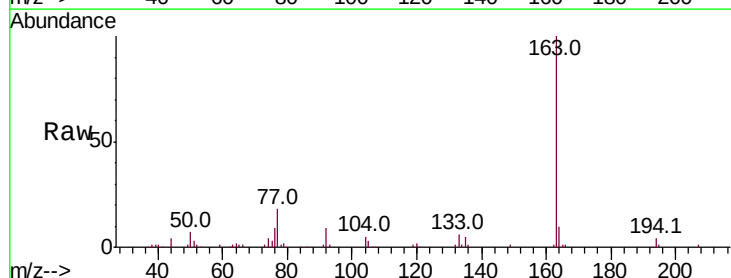

Abundance Ion 163.00 (162.70 to 163.70): BM016976.D (-1832) (-)

Ion 194.00 (193.70 to 194.70): BM016976.D (-1832) (-)

Ion 164.00 (163.70 to 164.70): BM016976.D (-1832) (-)

