

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100318\
 Data File : BM016980.D
 Acq On : 03 Oct 2018 16:49
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLC15

Quant Time: Oct 04 01:53:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 04 01:52:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	218660	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	894557	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.34	164	462411	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	1007454	20.00	ng/ul	0.00
78) Chrysene-d12	21.29	240	1139315	20.00	ng/ul	0.00
86) Perylene-d12	23.51	264	1221502	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.26	96	13164	2.57	ng/uL	0.00
5) Phenol-d5	6.88	99	281341	15.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	181635	15.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.24	132	245355	16.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	221763	15.54	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	110619	18.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	112752	21.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	216666	15.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	304257	18.56	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	636648	17.15	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	811253	16.92	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	64408	10.57	ng/ul	0.00
58) Fluorene-d10	15.34	176	564730	17.43	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.46	200	49548	11.98	ng/ul	0.00
71) Anthracene-d10	17.19	188	849142	17.47	ng/ul	0.00
79) Pyrene-d10	19.49	212	956807	17.31	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.37	264	1127707	17.70	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.81	163	196055	5.403	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100318\
Data File : BM016980.D
Acq On : 03 Oct 2018 16:49
Operator : MJ/SJ
Sample : J5115-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLC15

Quant Time: Oct 04 01:53:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 04 01:52:46 2018
Response via : Initial Calibration

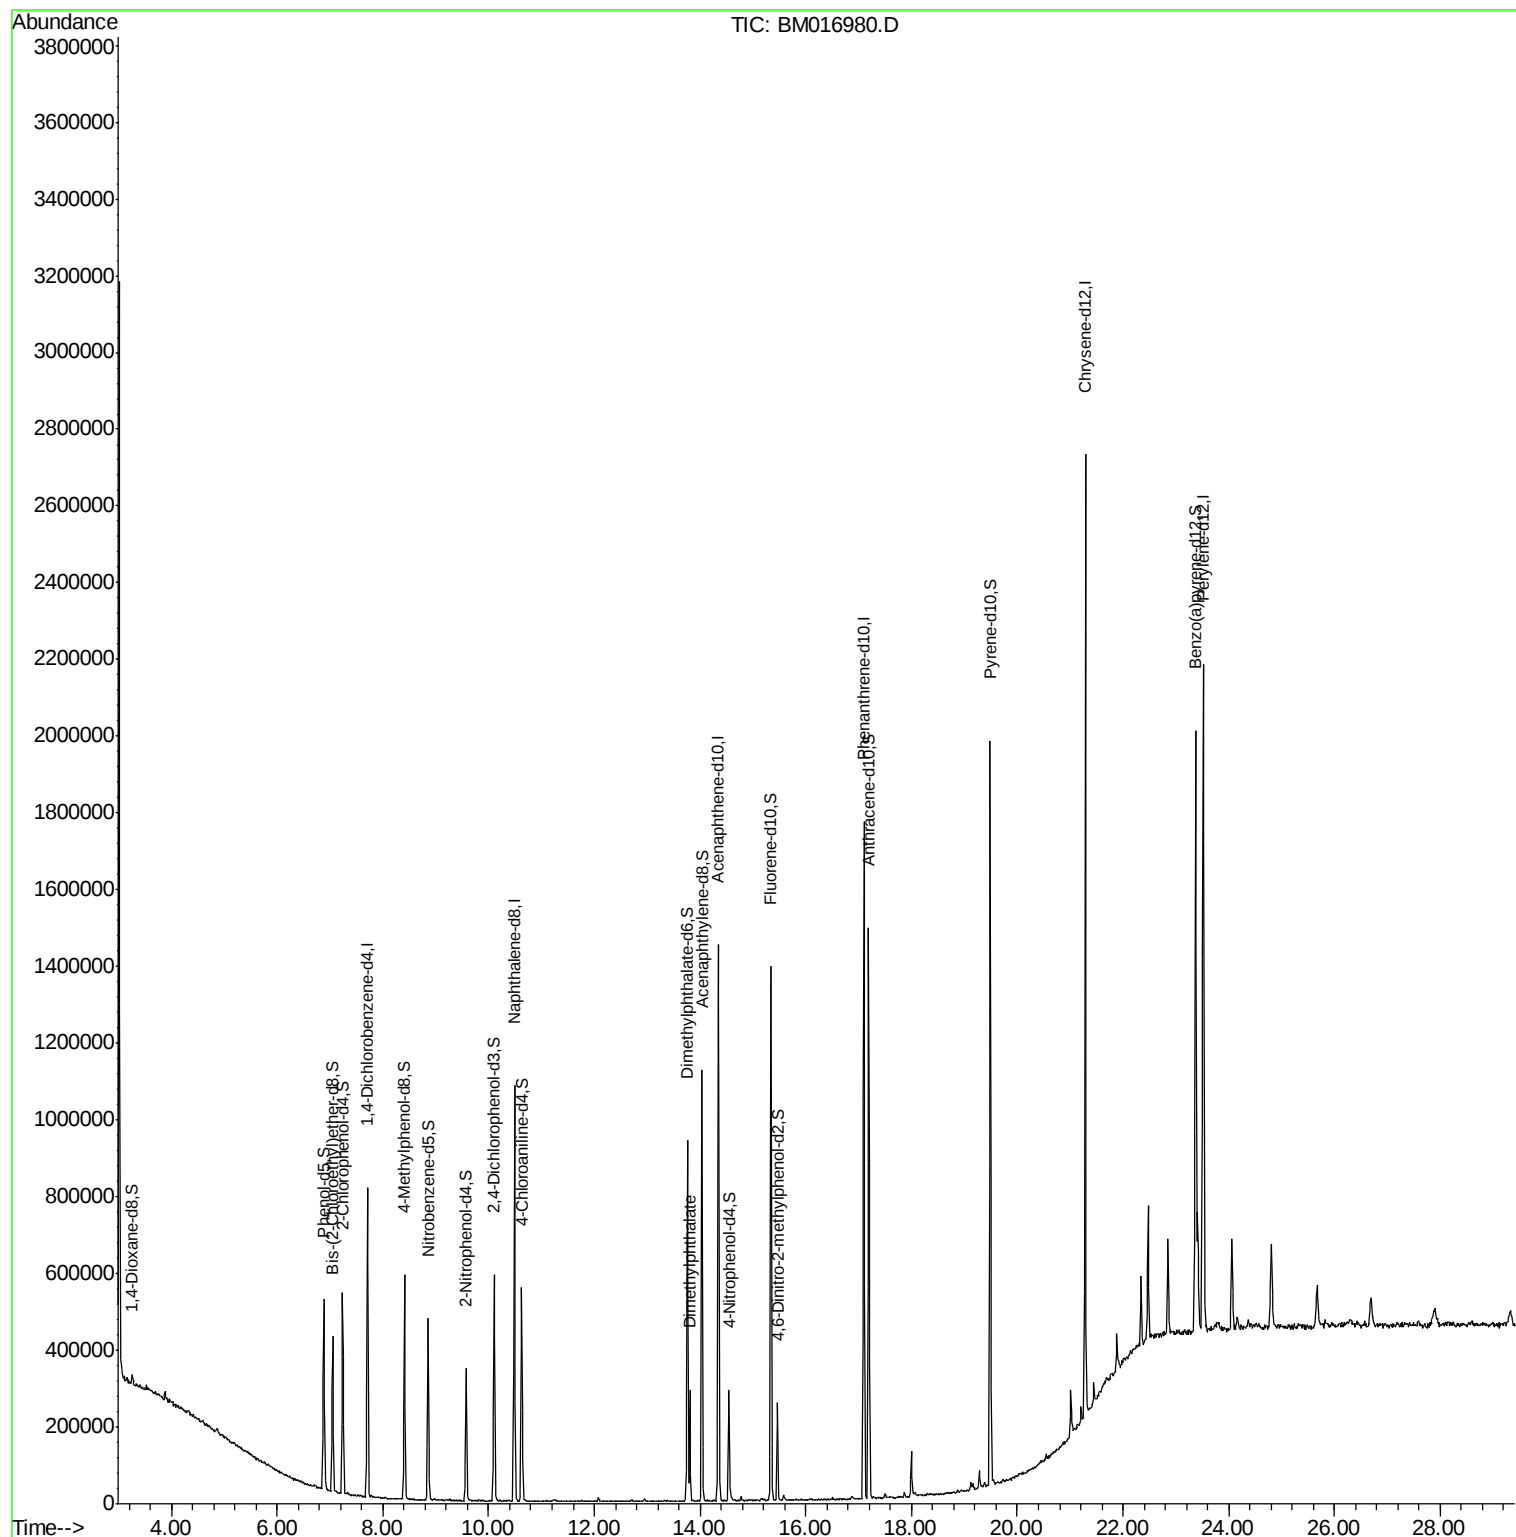

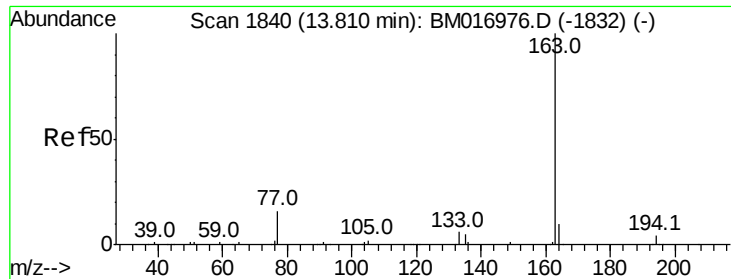

#45

Dimethylphthalate

Concen: 5.403 ng/ul

RT: 13.81 min Scan# 1840

Delta R.T. -0.00 min

Lab File: BM016980.D

Acq: 03 Oct 2018 16:49

Instrument :

BNA_M

ClientSampleId :

JLC15


Tot Ion:163 Resp: 196055

Ion Ratio Lower Upper

163 100

194 4.2 4.0 6.0

164 10.3 8.4 12.6

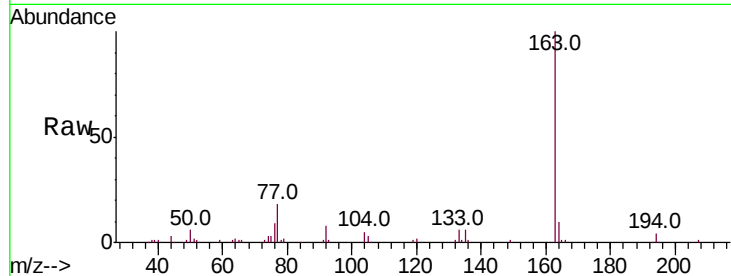

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

