

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100318\
 Data File : BM016982.D
 Acq On : 03 Oct 2018 18:01
 Operator : MJ/SJ
 Sample : J5115-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLC41

Quant Time: Oct 04 01:53:42 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 04 01:52:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	214349	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	889081	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.34	164	459610	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	1040918	20.00	ng/ul	0.00
78) Chrysene-d12	21.29	240	1180896	20.00	ng/ul	0.00
86) Perylene-d12	23.52	264	1261400	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	11145	2.22	ng/uL	0.00
5) Phenol-d5	6.88	99	257331	14.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	162206	14.49	ng/ul	0.00
9) 2-Chlorophenol-d4	7.24	132	218412	14.80	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	210641	15.06	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	102168	17.49	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	105266	19.82	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	210685	15.61	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	282577	17.34	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	638268	17.30	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	799733	16.78	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	77842	12.85	ng/ul	0.00
58) Fluorene-d10	15.34	176	574384	17.83	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.46	200	43059	10.08	ng/ul	0.00
71) Anthracene-d10	17.19	188	871994	17.36	ng/ul	0.00
79) Pyrene-d10	19.49	212	999509	17.44	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.37	264	1173471	17.83	ng/ul	0.00


Target Compounds				Ovalue
45) Dimethylphthalate	13.80	163	192159	5.328 ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100318\
Data File : BM016982.D
Acq On : 03 Oct 2018 18:01
Operator : MJ/SJ
Sample : J5115-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLC41

Quant Time: Oct 04 01:53:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 04 01:52:46 2018
Response via : Initial Calibration

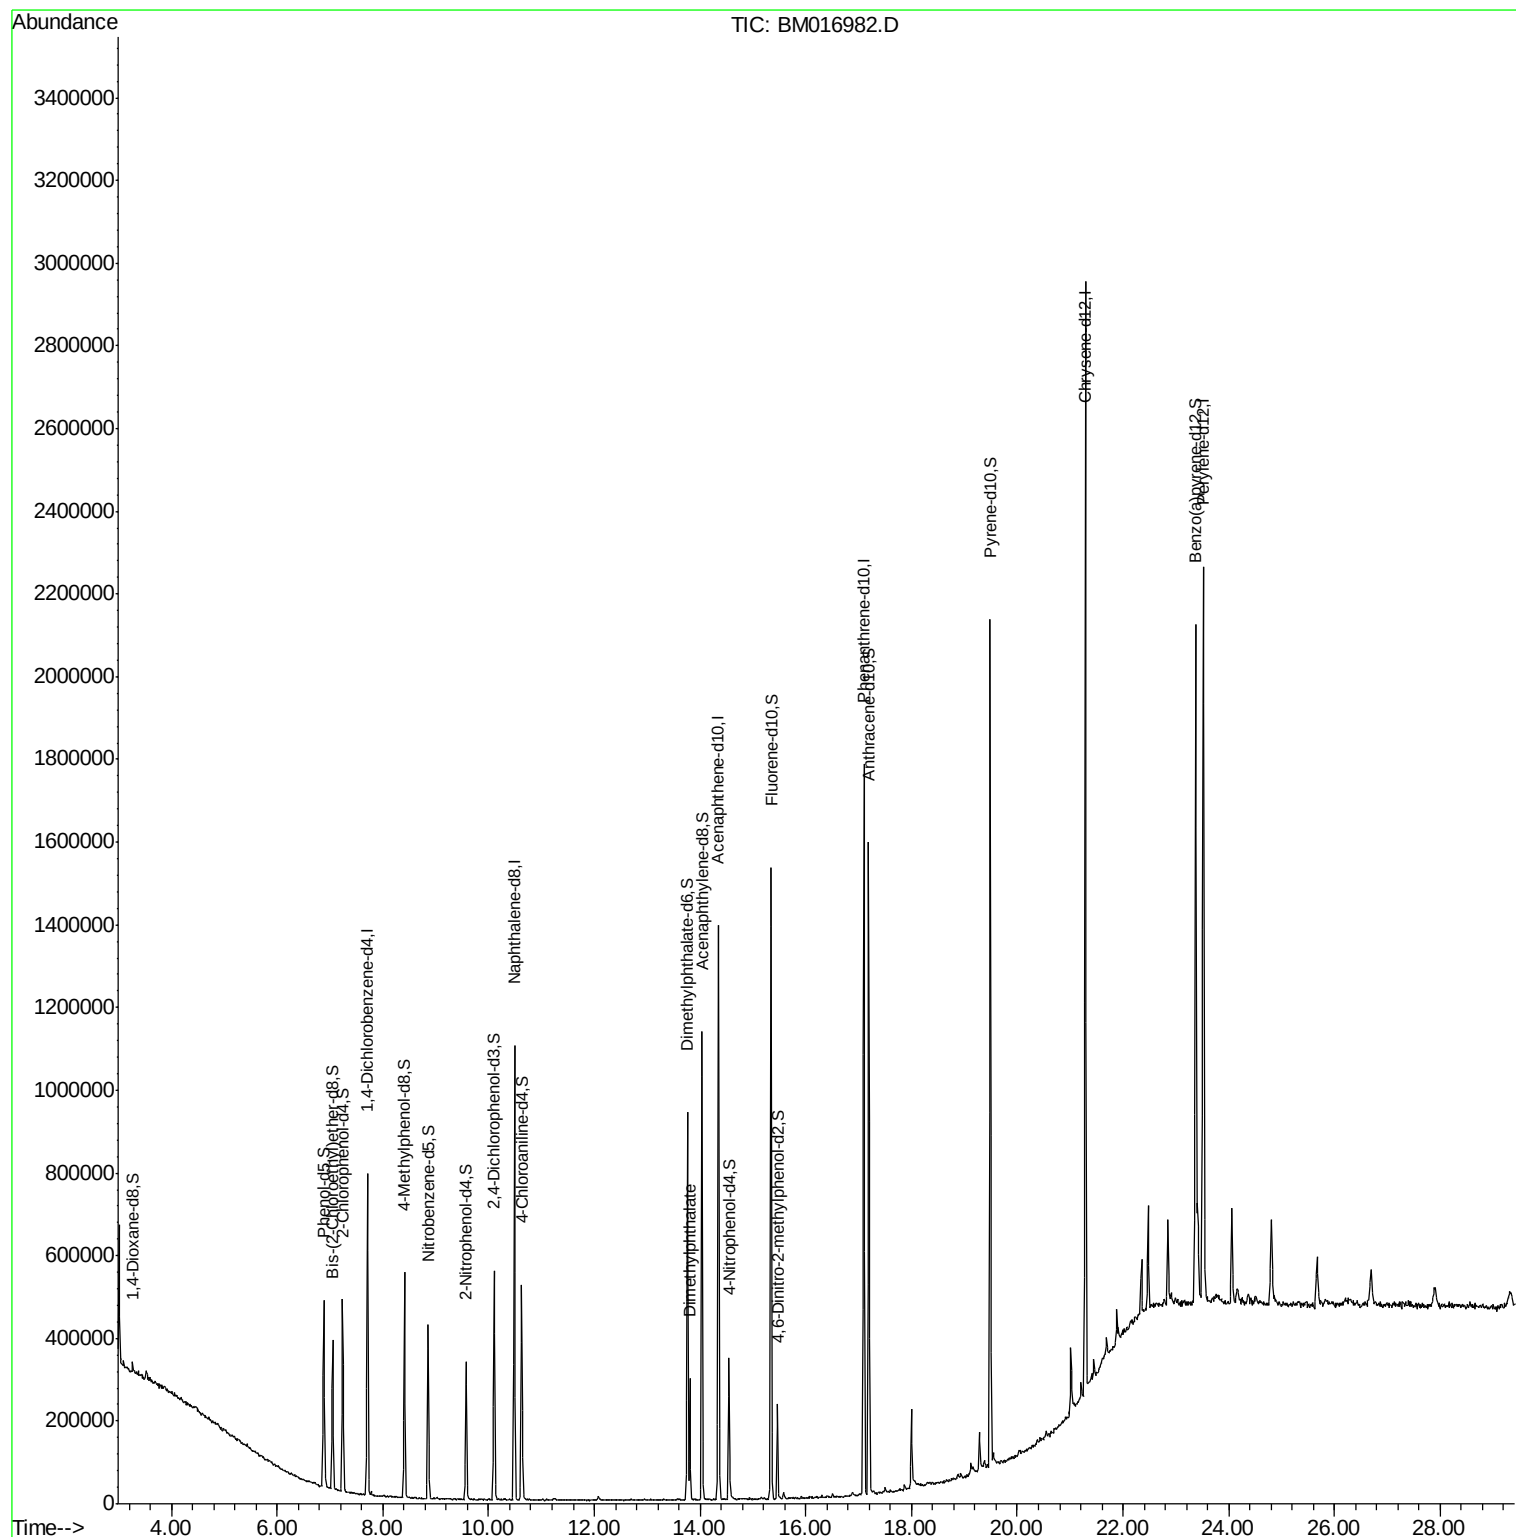

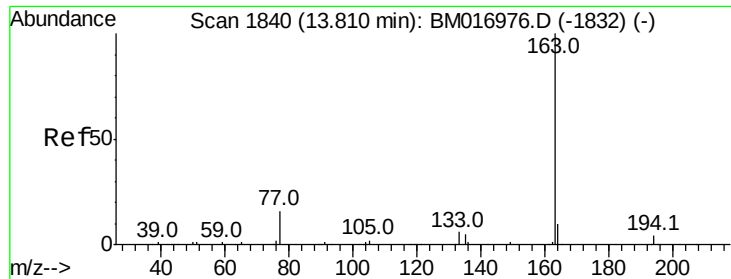

#45

Dimethylphthalate

Concen: 5.328 ng/ul

RT: 13.80 min Scan# 1839

Delta R.T. -0.01 min

Lab File: BM016982.D

Acq: 03 Oct 2018 18:01

Instrument :

BNA_M

ClientSampleId :

JLC41



Tot Ion:163 Resp: 192159

Ion Ratio Lower Upper

163 100

194 4.6 4.0 6.0

164 10.0 8.4 12.6

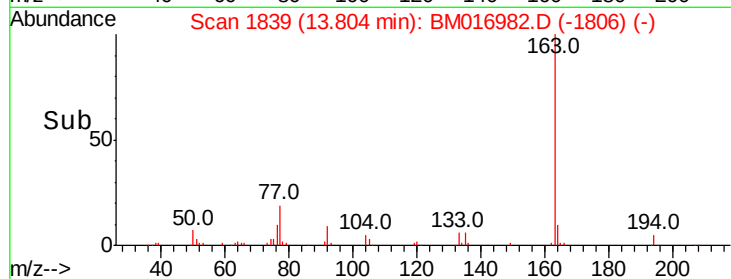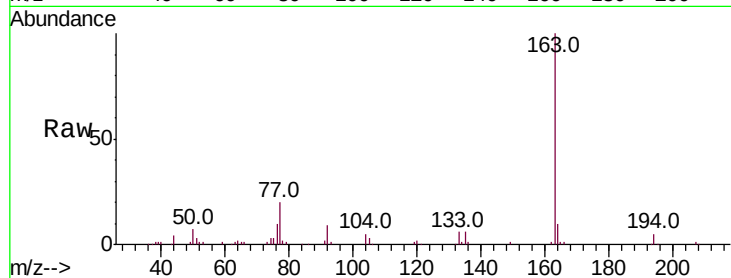

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

