

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100318\
 Data File : BM016986.D
 Acq On : 03 Oct 2018 20:25
 Operator : MJ/SJ
 Sample : J5115-21
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLC64

Quant Time: Oct 04 01:54:06 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 04 01:52:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	248802	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	1005871	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.35	164	495862	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.09	188	1057730	20.00	ng/ul	0.00
78) Chrysene-d12	21.29	240	1170924	20.00	ng/ul	0.00
86) Perylene-d12	23.52	264	1300080	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	17719	3.05	ng/uL	0.00
5) Phenol-d5	6.88	99	386734	18.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	246019	18.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.24	132	336222	19.63	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	294624	18.14	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	151408	22.91	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	153933	25.62	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	290262	19.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	360680	19.57	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	806825	20.26	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	1044792	20.32	ng/ul	0.00
52) 4-Nitrophenol-d4	14.55	143	84749	12.97	ng/ul	0.00
58) Fluorene-d10	15.34	176	720768	20.74	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.46	200	61868	14.25	ng/ul	0.00
71) Anthracene-d10	17.19	188	1034640	20.27	ng/ul	0.00
79) Pyrene-d10	19.49	212	1153100	20.29	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.37	264	1405627	20.73	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.90	94	38475	1.837 ng/ul	96
45) Dimethylphthalate	13.80	163	185987	4.780 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100318\
Data File : BM016986.D
Acq On : 03 Oct 2018 20:25
Operator : MJ/SJ
Sample : J5115-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
JLC64

Quant Time: Oct 04 01:54:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 04 01:52:46 2018
Response via : Initial Calibration

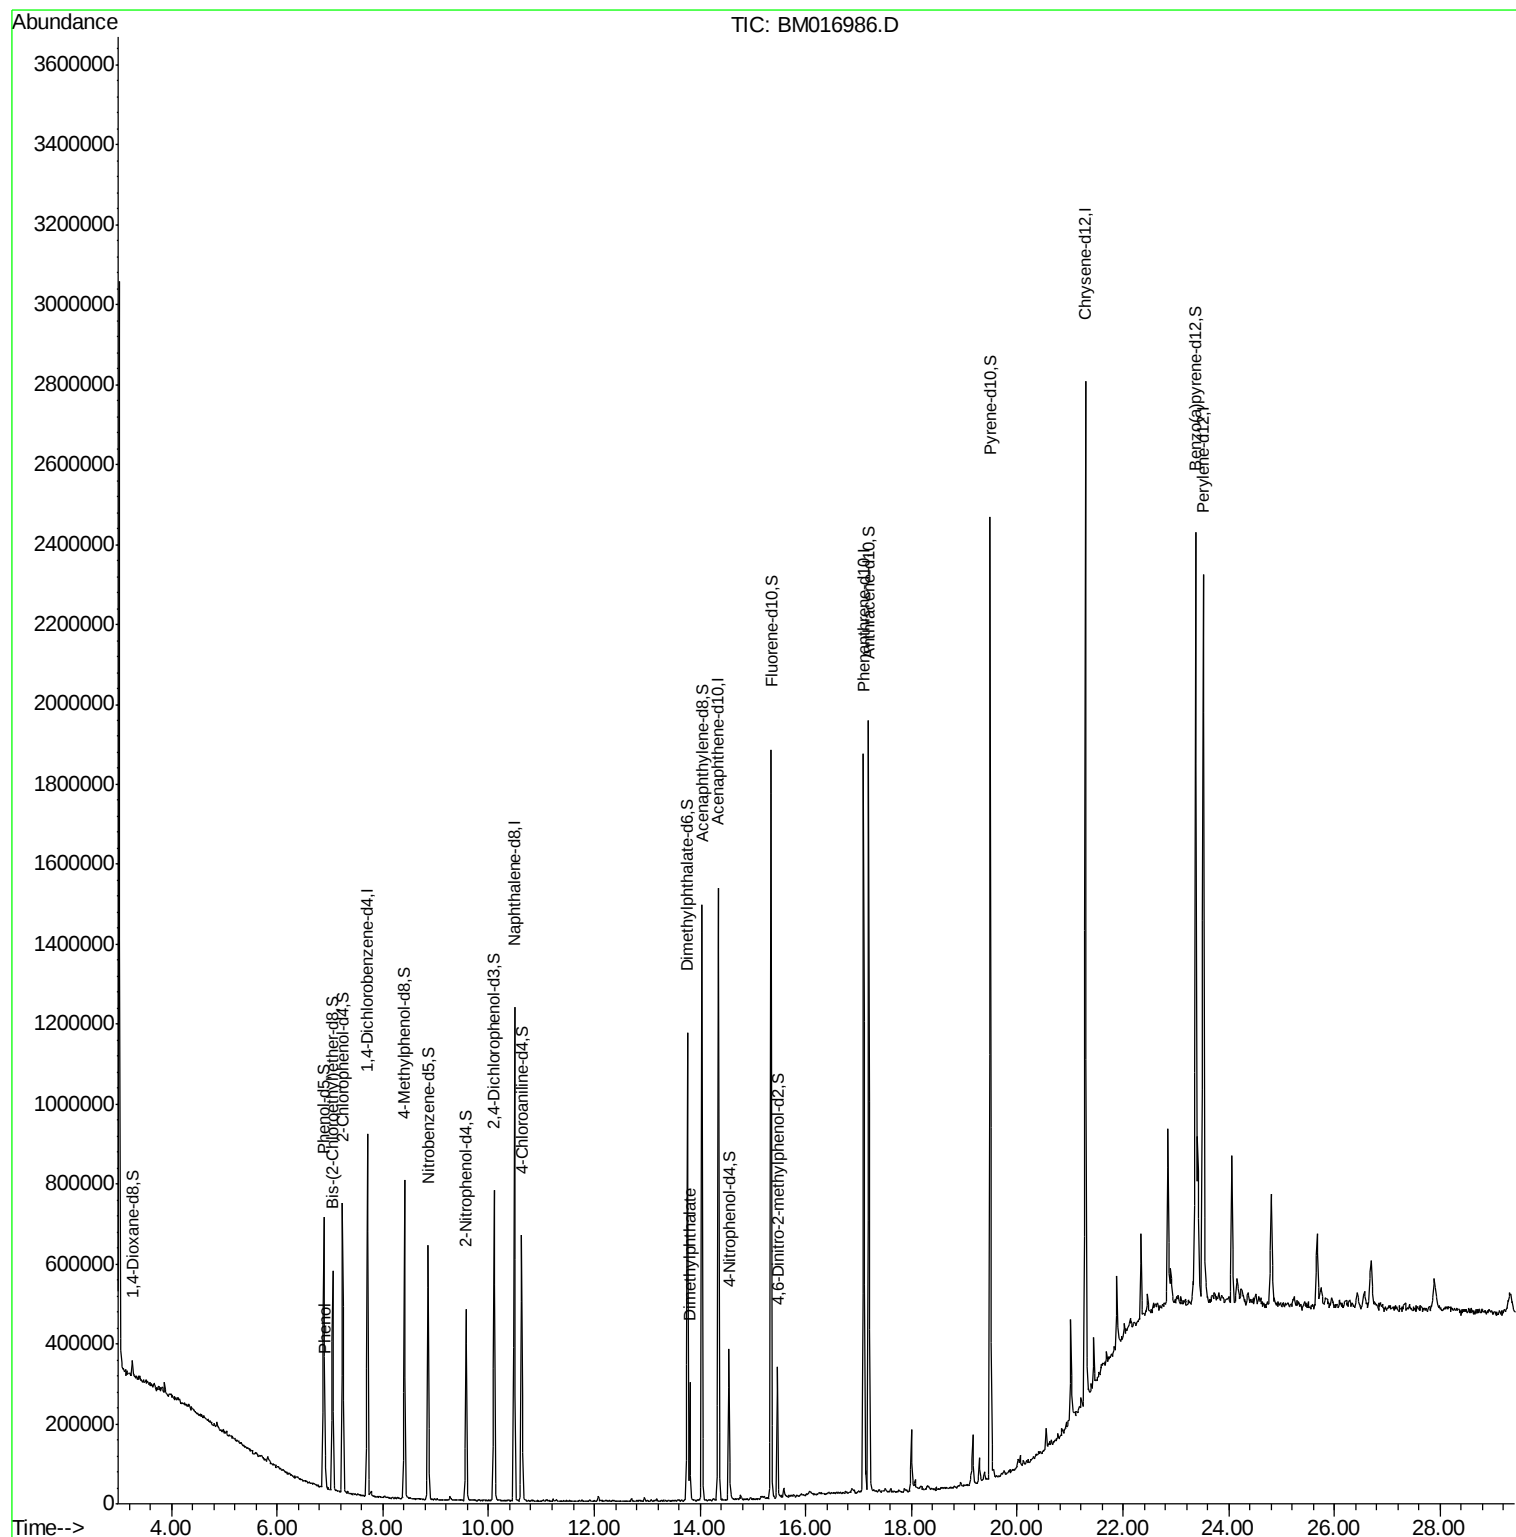

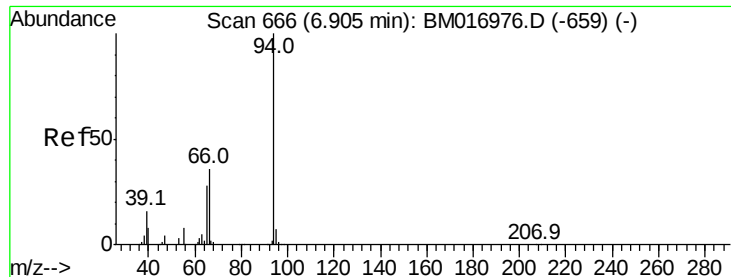

#6

Phenol

Concen: 1.837 ng/ul

RT: 6.90 min Scan# 666

Delta R.T. -0.00 min

Lab File: BM016986.D

Acq: 03 Oct 2018 20:25

Instrument :

BNA_M

ClientSampleId :

JLC64





Tot Ion: 94 Resp: 38475

Ion Ratio Lower Upper

94 100

65 30.8 23.0 34.6

66 41.0 30.4 45.6

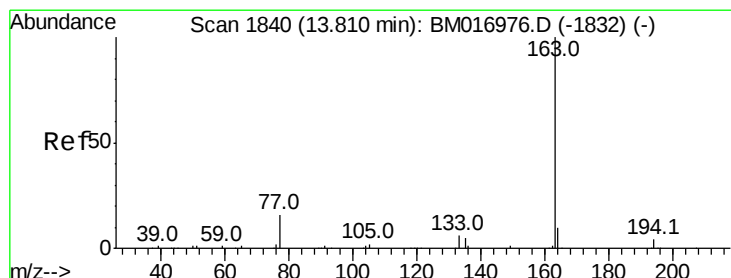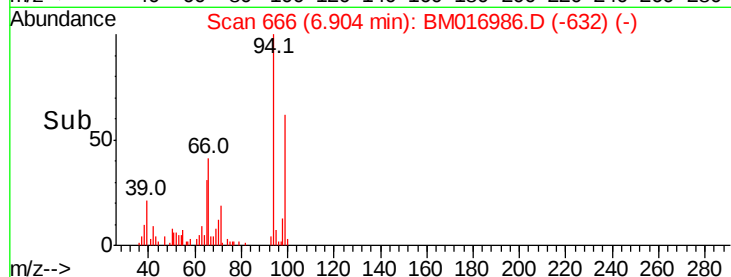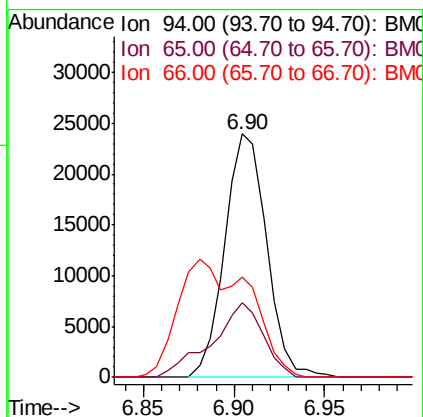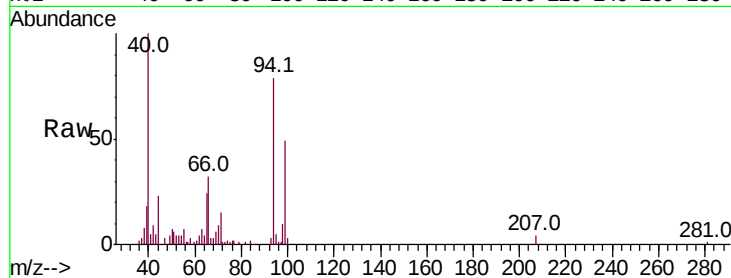

#45

Dimethylphthalate

Concen: 4.780 ng/ul

RT: 13.80 min Scan# 1839

Delta R.T. -0.01 min

Lab File: BM016986.D

Acq: 03 Oct 2018 20:25

Tgt Ion: 163 Resp: 185987

Ion Ratio Lower Upper

163 100

194 4.0 4.0 6.0

164 9.7 8.4 12.6

