

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047806.D
 Acq On : 03 Oct 2024 13:24
 Operator : RC/JU
 Sample : P4020-10DL 30X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCK1DL

Quant Time: Oct 03 14:09:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 02:30:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.804	152	216306	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.598	136	873944	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.433	164	566139	20.000	ng/u1	-0.02
64) Phenanthrene-d10	17.174	188	1235494	20.000	ng/u1	-0.01
79) Chrysene-d12	21.403	240	1189762	20.000	ng/u1	0.00
88) Perylene-d12	24.403	264	1403252	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	6.969	99	7305	0.357	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	6032	0.416	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.339	132	5680	0.382	ng/u1	0.00
15) 4-Methylphenol-d8	8.510	113	4745	0.312	ng/u1	0.00
21) Nitrobenzene-d5	8.957	128	2649	0.381	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.680	143	2273	0.341	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.222	165	4973	0.373	ng/u1	0.00
31) 4-Chloroaniline-d4	10.739	131	6299	0.306	ng/u1	0.00
46) Dimethylphthalate-d6	13.845	166	23778	0.579	ng/u1	-0.01
49) Acenaphthylene-d8	14.127	160	25185	0.518	ng/u1	-0.01
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	
60) Fluorene-d10	15.427	176	20384	0.573	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.539	200	1475	0.204	ng/u1	-0.01
73) Anthracene-d10	17.274	188	32793	0.540	ng/u1	-0.01
81) Pyrene-d10	19.562	212	36968	0.547	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.191	264	36331	0.499	ng/u1	-0.02
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.827	266	977672	103.743	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047806.D
Acq On : 03 Oct 2024 13:24
Operator : RC/JU
Sample : P4020-10DL 30X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCK1DL


Quant Time: Oct 03 14:09:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

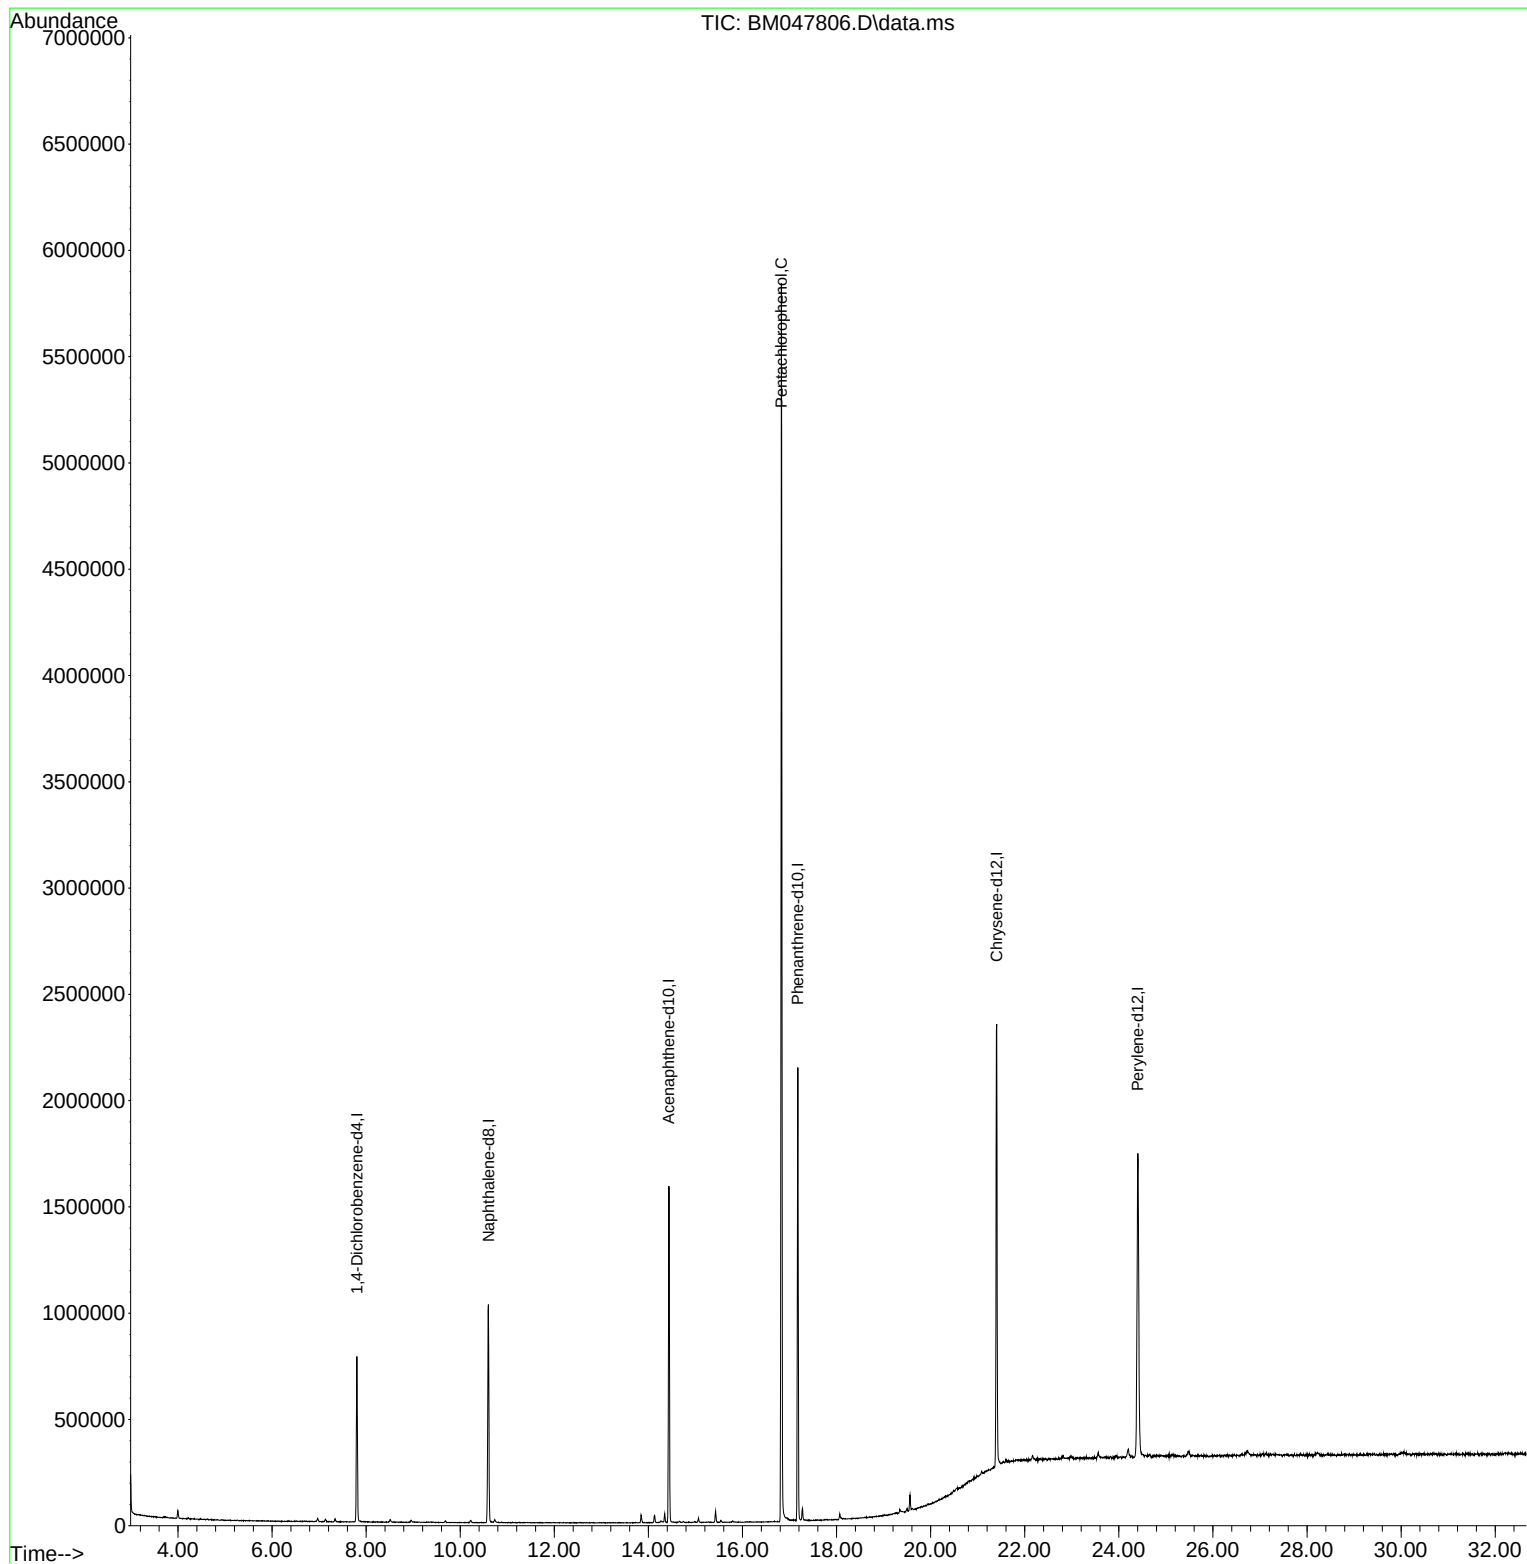

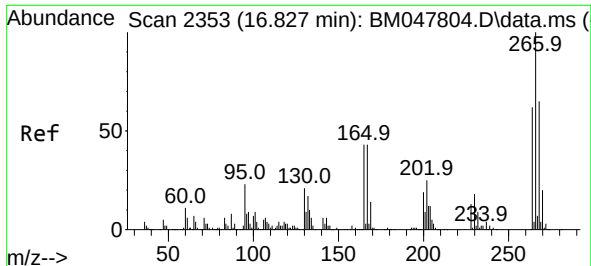

#71
 Pentachlorophenol
 Concen: 103.743 ng/ul
 RT: 16.827 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BM047806.D
 Acq: 03 Oct 2024 13:24

Instrument :
 BNA_M
 ClientSampleId :
 DDCK1DL

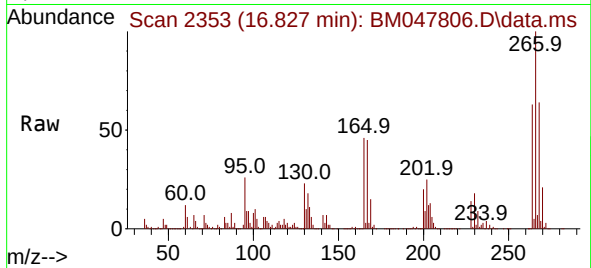

Tgt Ion:266 Resp: 977672
 Ion Ratio Lower Upper
 266 100
 264 62.5 50.2 75.2
 268 64.2 50.9 76.3

