

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047833.D
 Acq On : 04 Oct 2024 08:26
 Operator : RC/JU
 Sample : P4020-05DL 30X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCF9DL

Quant Time: Oct 04 09:01:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 08:32:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.804	152	190586	20.000	ng/ul	0.00
20) Naphthalene-d8	10.592	136	780956	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.433	164	499671	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.174	188	1078804	20.000	ng/ul	0.00
79) Chrysene-d12	21.397	240	1006663	20.000	ng/ul	0.00
88) Perylene-d12	24.397	264	1156575	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.969	99	9446	0.524	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	7587	0.593	ng/ul	0.00
11) 2-Chlorophenol-d4	7.328	132	8088	0.617	ng/ul	0.00
15) 4-Methylphenol-d8	8.510	113	6149	0.459	ng/ul	0.00
21) Nitrobenzene-d5	8.957	128	3486	0.561	ng/ul	0.00
24) 2-Nitrophenol-d4	9.675	143	3233	0.543	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	6586	0.553	ng/ul	0.00
31) 4-Chloroaniline-d4	10.739	131	8929	0.485	ng/ul	0.01
46) Dimethylphthalate-d6	13.845	166	32868	0.907	ng/ul	0.00
49) Acenaphthylene-d8	14.127	160	34425	0.801	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.427	176	28262	0.901	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.268	188	45258	0.853	ng/ul	0.00
81) Pyrene-d10	19.556	212	51070	0.894	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.191	264	48380	0.806	ng/ul	0.00
Target Compounds						
58) 2,3,4,6-Tetrachlorophenol	15.063	232	16215	1.999	ng/ul	97
71) Pentachlorophenol	16.827	266	1509093	183.392	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047833.D
Acq On : 04 Oct 2024 08:26
Operator : RC/JU
Sample : P4020-05DL 30X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCF9DL

Quant Time: Oct 04 09:01:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 08:32:31 2024
Response via : Initial Calibration

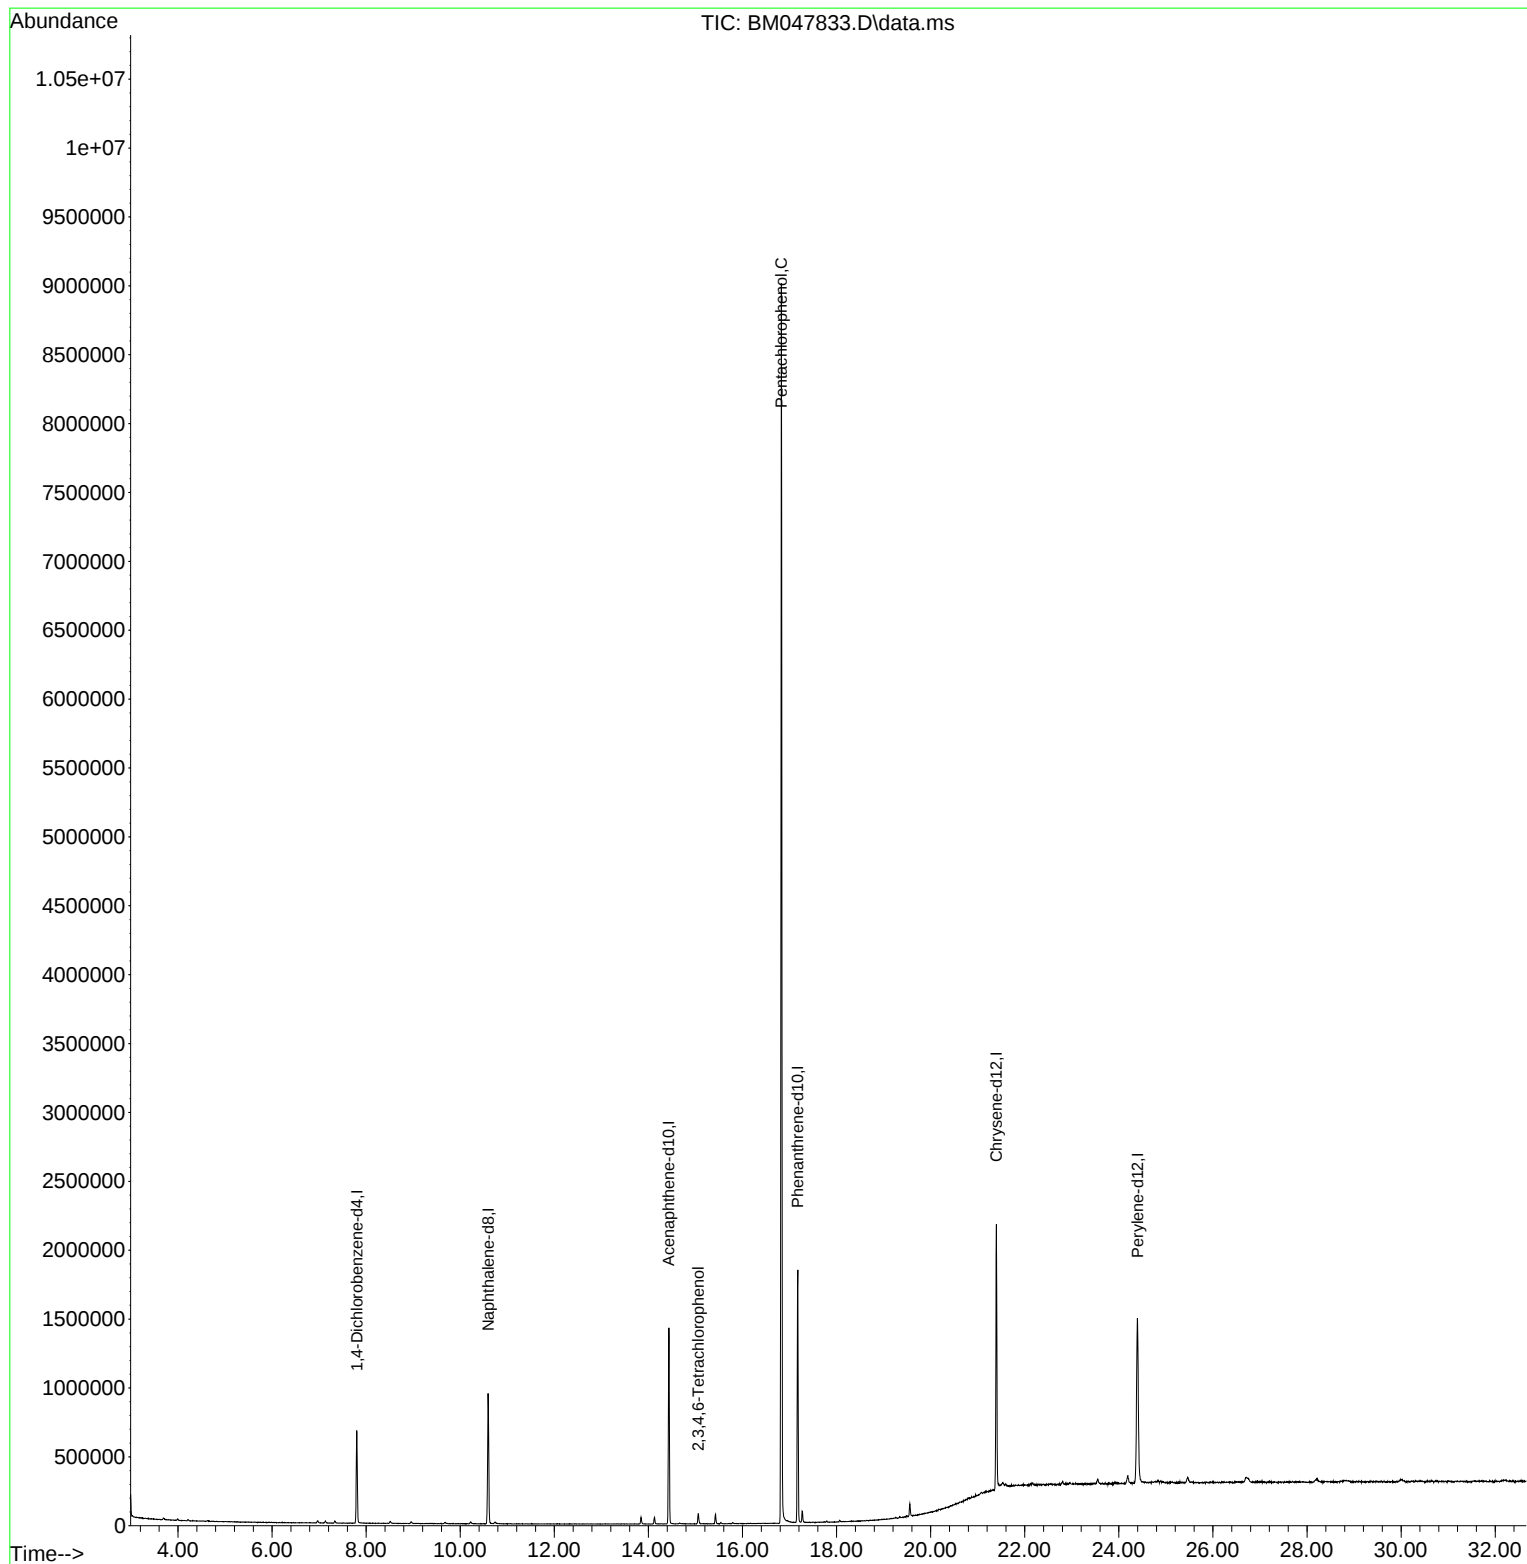




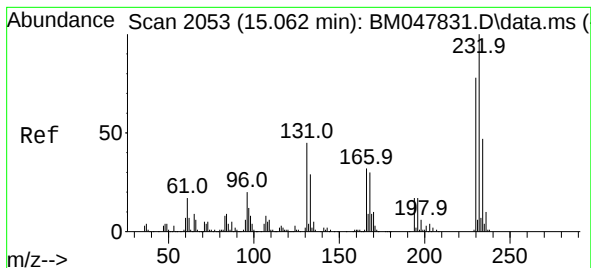


#58
2,3,4,6-Tetrachlorophenol
Concen: 1.999 ng/ul
RT: 15.063 min Scan# 2053
Delta R.T. 0.000 min
Lab File: BM047833.D
Acq: 04 Oct 2024 08:26

Instrument :
BNA_M
ClientSampleId :
DDCF9DL

Tgt Ion:232 Resp: 16215

Ion	Ratio	Lower	Upper
232	100		
131	46.5	40.2	60.4
130	3.5	2.6	4.0
166	31.4	25.3	37.9

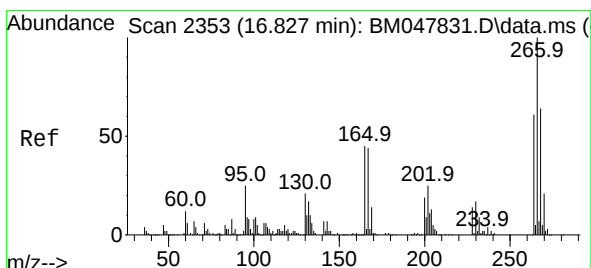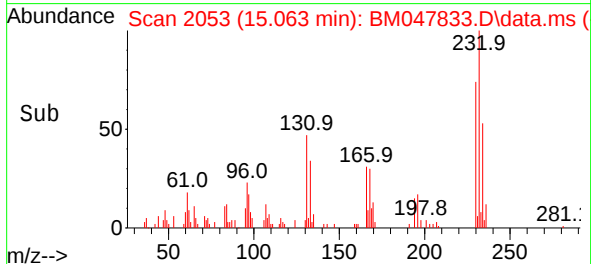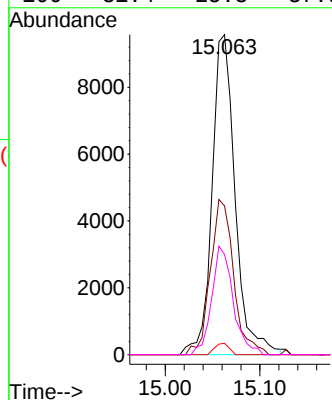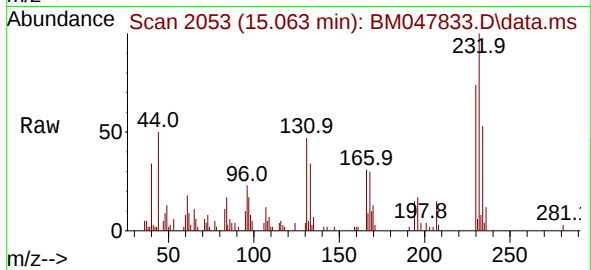

#71
Pentachlorophenol
Concen: 183.392 ng/ul
RT: 16.827 min Scan# 2353
Delta R.T. 0.000 min
Lab File: BM047833.D
Acq: 04 Oct 2024 08:26

Tgt Ion:266 Resp: 1509093

Ion	Ratio	Lower	Upper
266	100		
264	63.0	50.2	75.2
268	64.4	50.9	76.3

