

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047853.D
 Acq On : 04 Oct 2024 22:13
 Operator : RC/JU
 Sample : P4016-12MEDL 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCVW3MEDL

Quant Time: Oct 04 23:12:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 08:32:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.798	152	230692	20.000	ng/ul	0.00
20) Naphthalene-d8	10.592	136	940253	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.433	164	584173	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.168	188	1225628	20.000	ng/ul	0.00
79) Chrysene-d12	21.392	240	1103116	20.000	ng/ul	0.00
88) Perylene-d12	24.391	264	1238409	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	4034	0.565	ng/uL	0.00
4) Pyridine-d5	3.675	84	41275	1.975	ng/ul	0.01
7) Phenol-d5	6.963	99	54384	2.493	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	37890	2.448	ng/ul	0.00
11) 2-Chlorophenol-d4	7.334	132	47015	2.962	ng/ul	0.00
15) 4-Methylphenol-d8	8.504	113	43615	2.689	ng/ul	0.00
21) Nitrobenzene-d5	8.951	128	20876	2.789	ng/ul	0.00
24) 2-Nitrophenol-d4	9.675	143	19003	2.649	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	42441	2.961	ng/ul	0.00
31) 4-Chloroaniline-d4	10.728	131	60623	2.736	ng/ul	0.00
46) Dimethylphthalate-d6	13.839	166	151927	3.587	ng/ul	0.00
49) Acenaphthylene-d8	14.122	160	168828	3.362	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.421	176	132601	3.615	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.539	200	9339	1.302	ng/ul	0.00
73) Anthracene-d10	17.268	188	200509	3.327	ng/ul	0.00
81) Pyrene-d10	19.556	212	231513	3.698	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.180	264	208349	3.243	ng/ul	-0.01
Target Compounds						
					Qvalue	
58) 2,3,4,6-Tetrachlorophenol	15.057	232	23853	2.515	ng/ul	93
71) Pentachlorophenol	16.821	266	326601	34.935	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047853.D
Acq On : 04 Oct 2024 22:13
Operator : RC/JU
Sample : P4016-12MEDL 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCVW3MEDL

Quant Time: Oct 04 23:12:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 08:32:31 2024
Response via : Initial Calibration




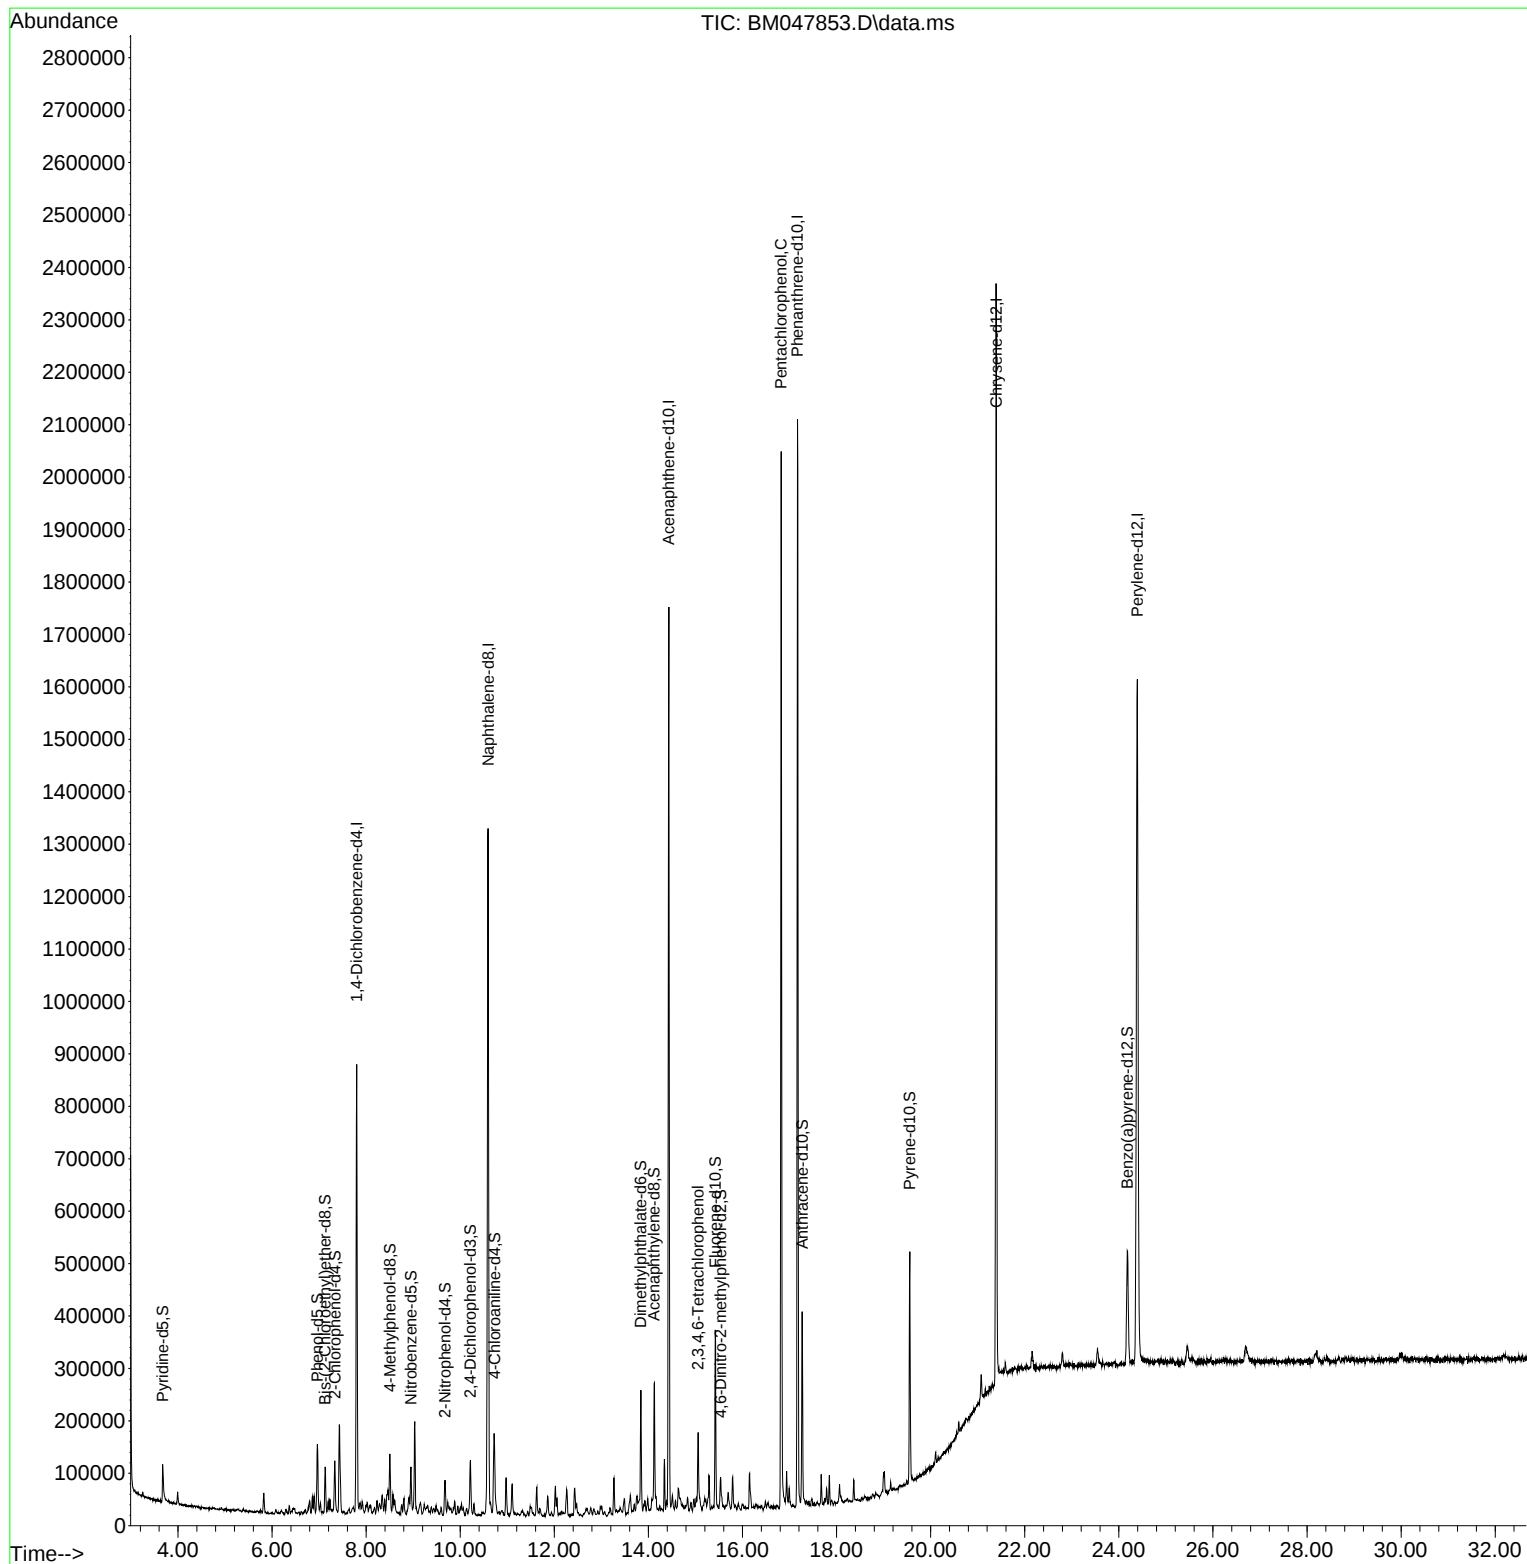


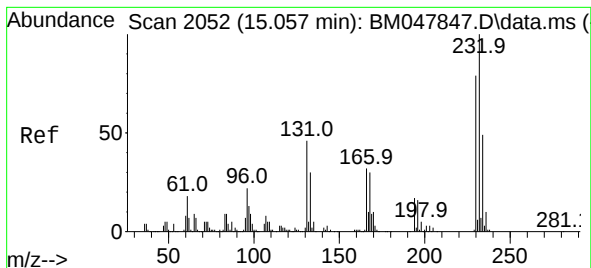

#58
2,3,4,6-Tetrachlorophenol
Concen: 2.515 ng/ul
RT: 15.057 min Scan# 2052
Delta R.T. -0.006 min
Lab File: BM047853.D
Acq: 04 Oct 2024 22:13

Instrument :
BNA_M
ClientSampleId :
DCVW3MEDL

Tgt Ion:	232	Resp:	23853
Ion	Ratio	Lower	Upper
232	100		
131	45.4	40.2	60.4
130	3.5	2.6	4.0
166	35.5	25.3	37.9

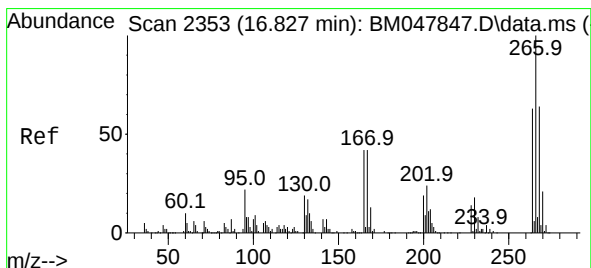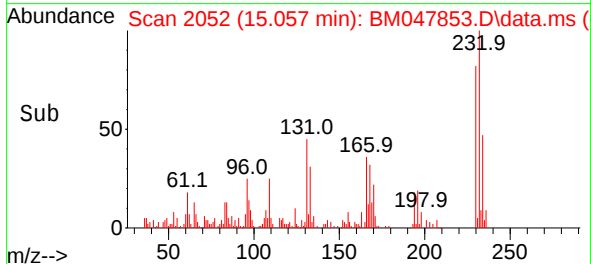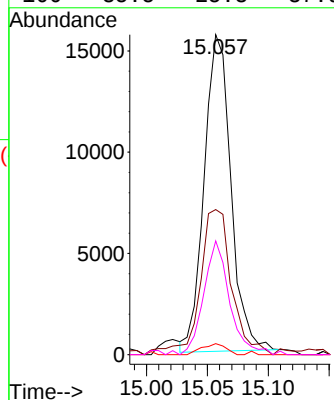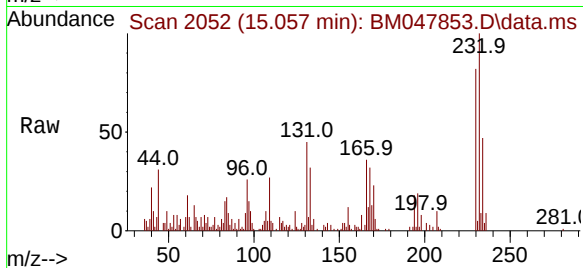

#71
Pentachlorophenol
Concen: 34.935 ng/ul
RT: 16.821 min Scan# 2352
Delta R.T. -0.006 min
Lab File: BM047853.D
Acq: 04 Oct 2024 22:13

Tgt Ion:	266	Resp:	326601
Ion	Ratio	Lower	Upper
266	100		
264	61.8	50.2	75.2
268	63.2	50.9	76.3

