

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047857.D
 Acq On : 05 Oct 2024 00:53
 Operator : RC/JU
 Sample : P4017-19MEDL 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCD5MEDL

Quant Time: Oct 05 04:59:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 08:32:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.798	152	217854	20.000	ng/ul	0.00
20) Naphthalene-d8	10.592	136	878222	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.433	164	529803	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.174	188	1114667	20.000	ng/ul	0.00
79) Chrysene-d12	21.392	240	1002627	20.000	ng/ul	0.00
88) Perylene-d12	24.391	264	1115466	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.969	99	41786	2.028	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	30778	2.105	ng/ul	0.00
11) 2-Chlorophenol-d4	7.334	132	37582	2.507	ng/ul	0.00
15) 4-Methylphenol-d8	8.504	113	31916	2.084	ng/ul	0.00
21) Nitrobenzene-d5	8.951	128	15470	2.212	ng/ul	0.00
24) 2-Nitrophenol-d4	9.675	143	13691	2.043	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	32706	2.443	ng/ul	0.00
31) 4-Chloroaniline-d4	10.727	131	40019	1.934	ng/ul	0.00
46) Dimethylphthalate-d6	13.839	166	122301	3.184	ng/ul	0.00
49) Acenaphthylene-d8	14.127	160	131853	2.895	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.421	176	107065	3.218	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.268	188	164059	2.993	ng/ul	0.00
81) Pyrene-d10	19.556	212	188909	3.320	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.180	264	169794	2.934	ng/ul	-0.01
Target Compounds						
58) 2,3,4,6-Tetrachlorophenol	15.057	232	28546	3.319	ng/ul	96
71) Pentachlorophenol	16.821	266	258591	30.414	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047857.D
Acq On : 05 Oct 2024 00:53
Operator : RC/JU
Sample : P4017-19MEDL 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCD5MEDL

Quant Time: Oct 05 04:59:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 08:32:31 2024
Response via : Initial Calibration




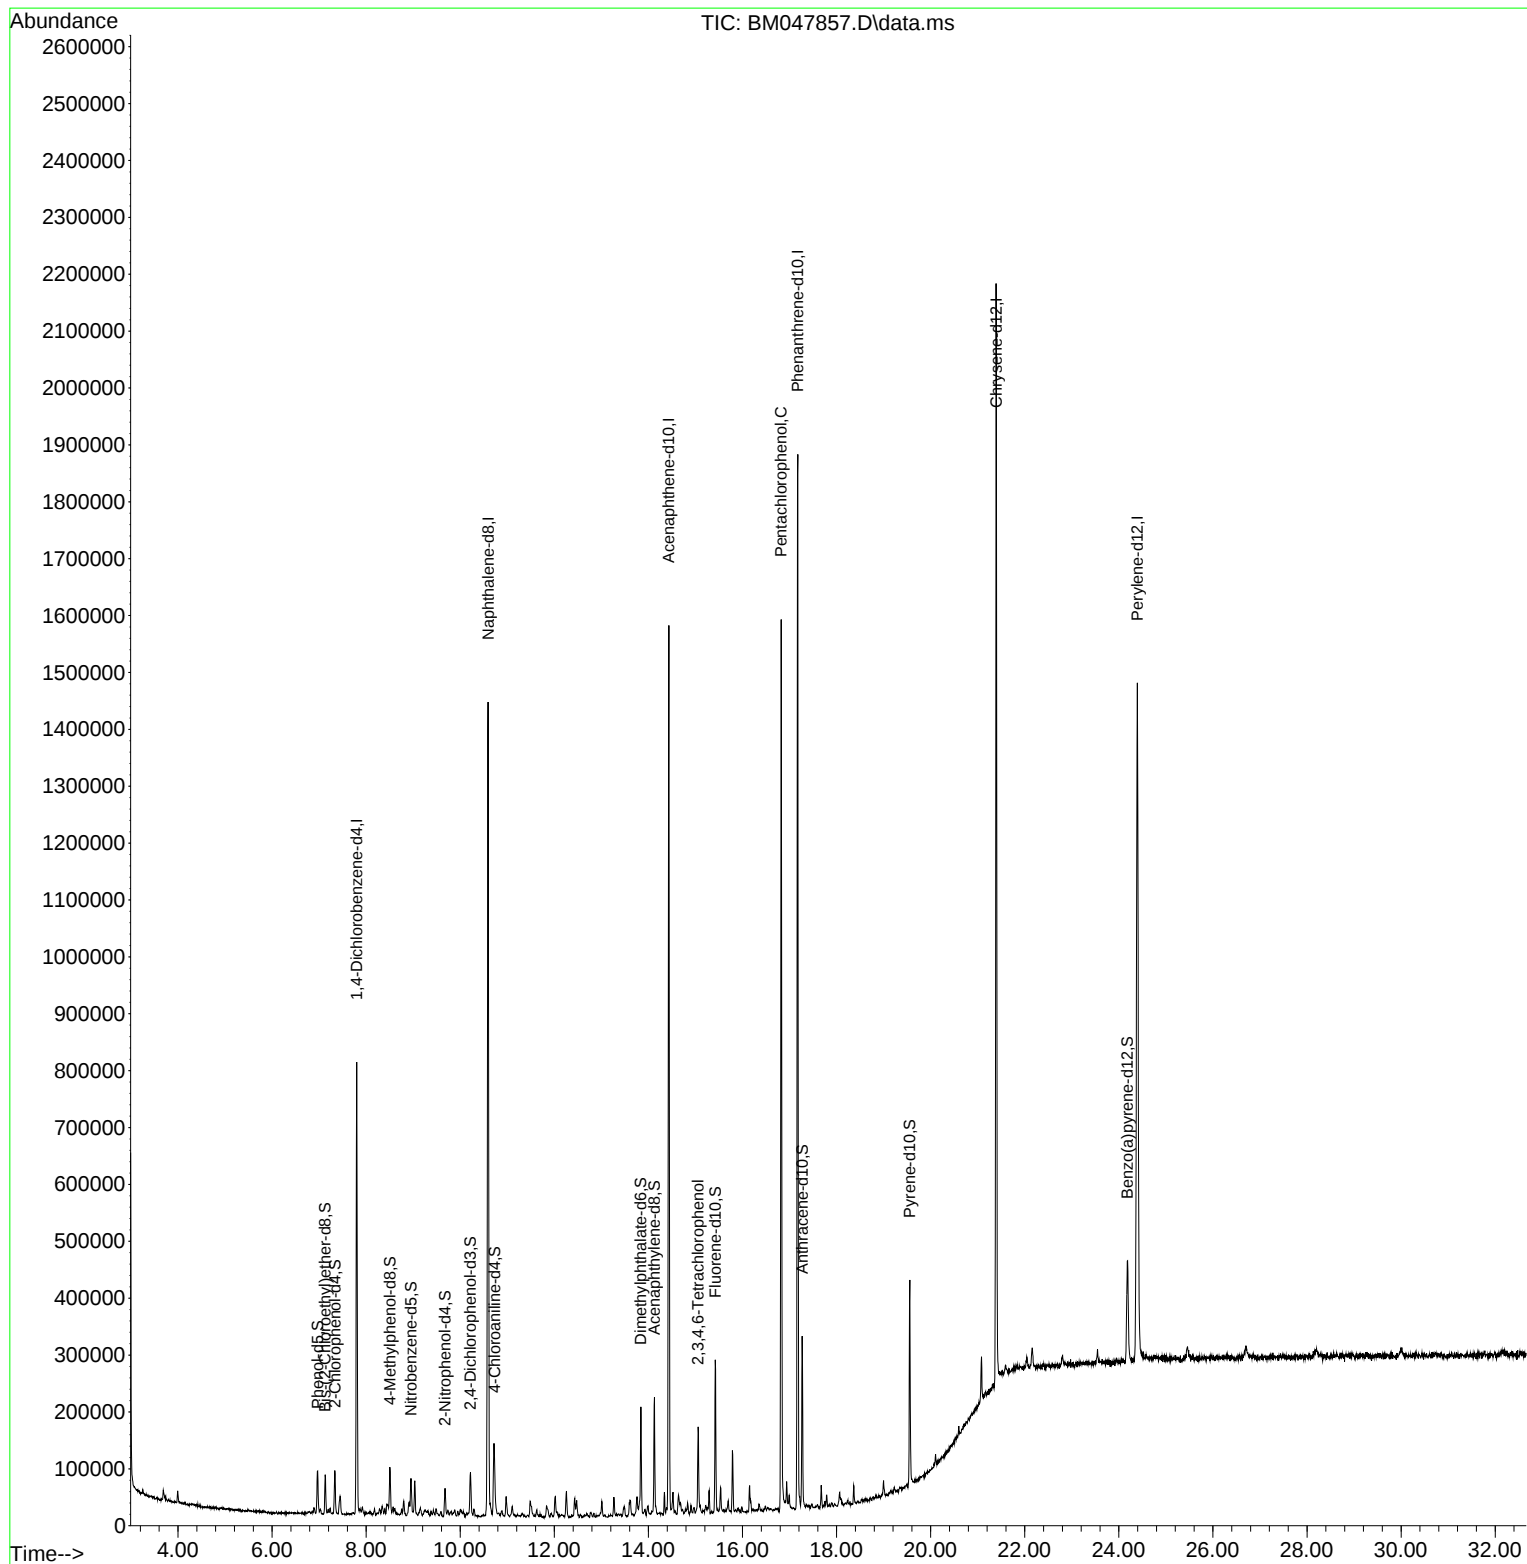


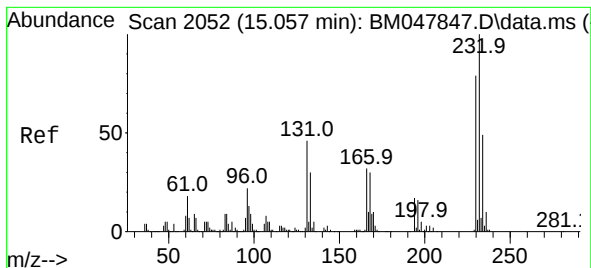

#58
2,3,4,6-Tetrachlorophenol
Concen: 3.319 ng/ul
RT: 15.057 min Scan# 2052
Delta R.T. -0.006 min
Lab File: BM047857.D
Acq: 05 Oct 2024 00:53

Instrument :
BNA_M
ClientSampleId :
DDCD5MEDL

Tgt Ion:	232	Resp:	28546
Ion Ratio	Lower	Upper	
232	100		
131	47.7	40.2	60.4
130	3.8	2.6	4.0
166	33.8	25.3	37.9

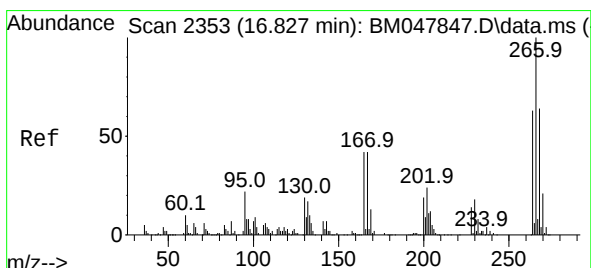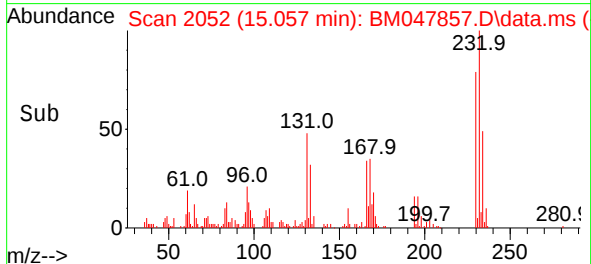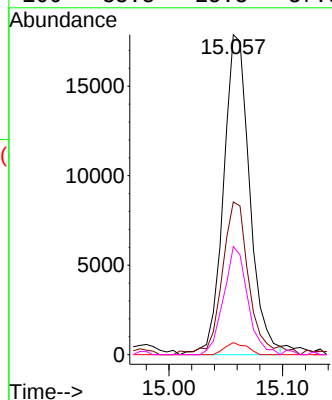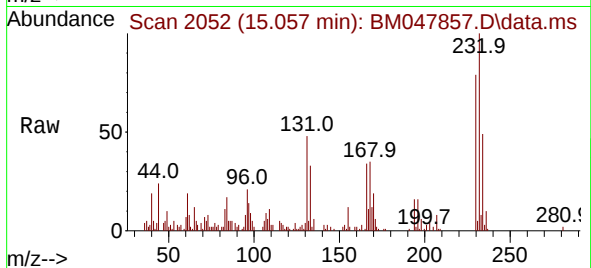

#71
Pentachlorophenol
Concen: 30.414 ng/ul
RT: 16.821 min Scan# 2352
Delta R.T. -0.006 min
Lab File: BM047857.D
Acq: 05 Oct 2024 00:53

Tgt Ion:	266	Resp:	258591
Ion Ratio	Lower	Upper	
266	100		
264	62.0	50.2	75.2
268	62.0	50.9	76.3

