

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047860.D
 Acq On : 05 Oct 2024 02:53
 Operator : RC/JU
 Sample : P4017-14MEDL 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDC96MEDL

Quant Time: Oct 05 03:48:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 08:32:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.798	152	218673	20.000	ng/ul	0.00
20) Naphthalene-d8	10.592	136	875623	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.433	164	527397	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.174	188	1100003	20.000	ng/ul	0.00
79) Chrysene-d12	21.392	240	989618	20.000	ng/ul	0.00
88) Perylene-d12	24.391	264	1114077	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	3.681	84	23259	1.174	ng/ul	0.02
7) Phenol-d5	6.969	99	31085	1.503	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	21731	1.481	ng/ul	0.00
11) 2-Chlorophenol-d4	7.334	132	25865	1.719	ng/ul	0.00
15) 4-Methylphenol-d8	8.504	113	24046	1.564	ng/ul	0.00
21) Nitrobenzene-d5	8.957	128	10640	1.526	ng/ul	0.00
24) 2-Nitrophenol-d4	9.675	143	9646	1.444	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	21601	1.618	ng/ul	0.00
31) 4-Chloroaniline-d4	10.727	131	32908	1.595	ng/ul	0.00
46) Dimethylphthalate-d6	13.839	166	84129	2.200	ng/ul	0.00
49) Acenaphthylene-d8	14.127	160	95730	2.112	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.421	176	75691	2.285	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.268	188	113805	2.104	ng/ul	0.00
81) Pyrene-d10	19.556	212	127031	2.262	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.180	264	115670	2.001	ng/ul	-0.01
Target Compounds						
					Qvalue	
58) 2,3,4,6-Tetrachlorophenol	15.057	232	39977	4.669	ng/ul	97
71) Pentachlorophenol	16.821	266	377403	44.980	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047860.D
Acq On : 05 Oct 2024 02:53
Operator : RC/JU
Sample : P4017-14MEDL 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDC96MEDL

Quant Time: Oct 05 03:48:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 08:32:31 2024
Response via : Initial Calibration




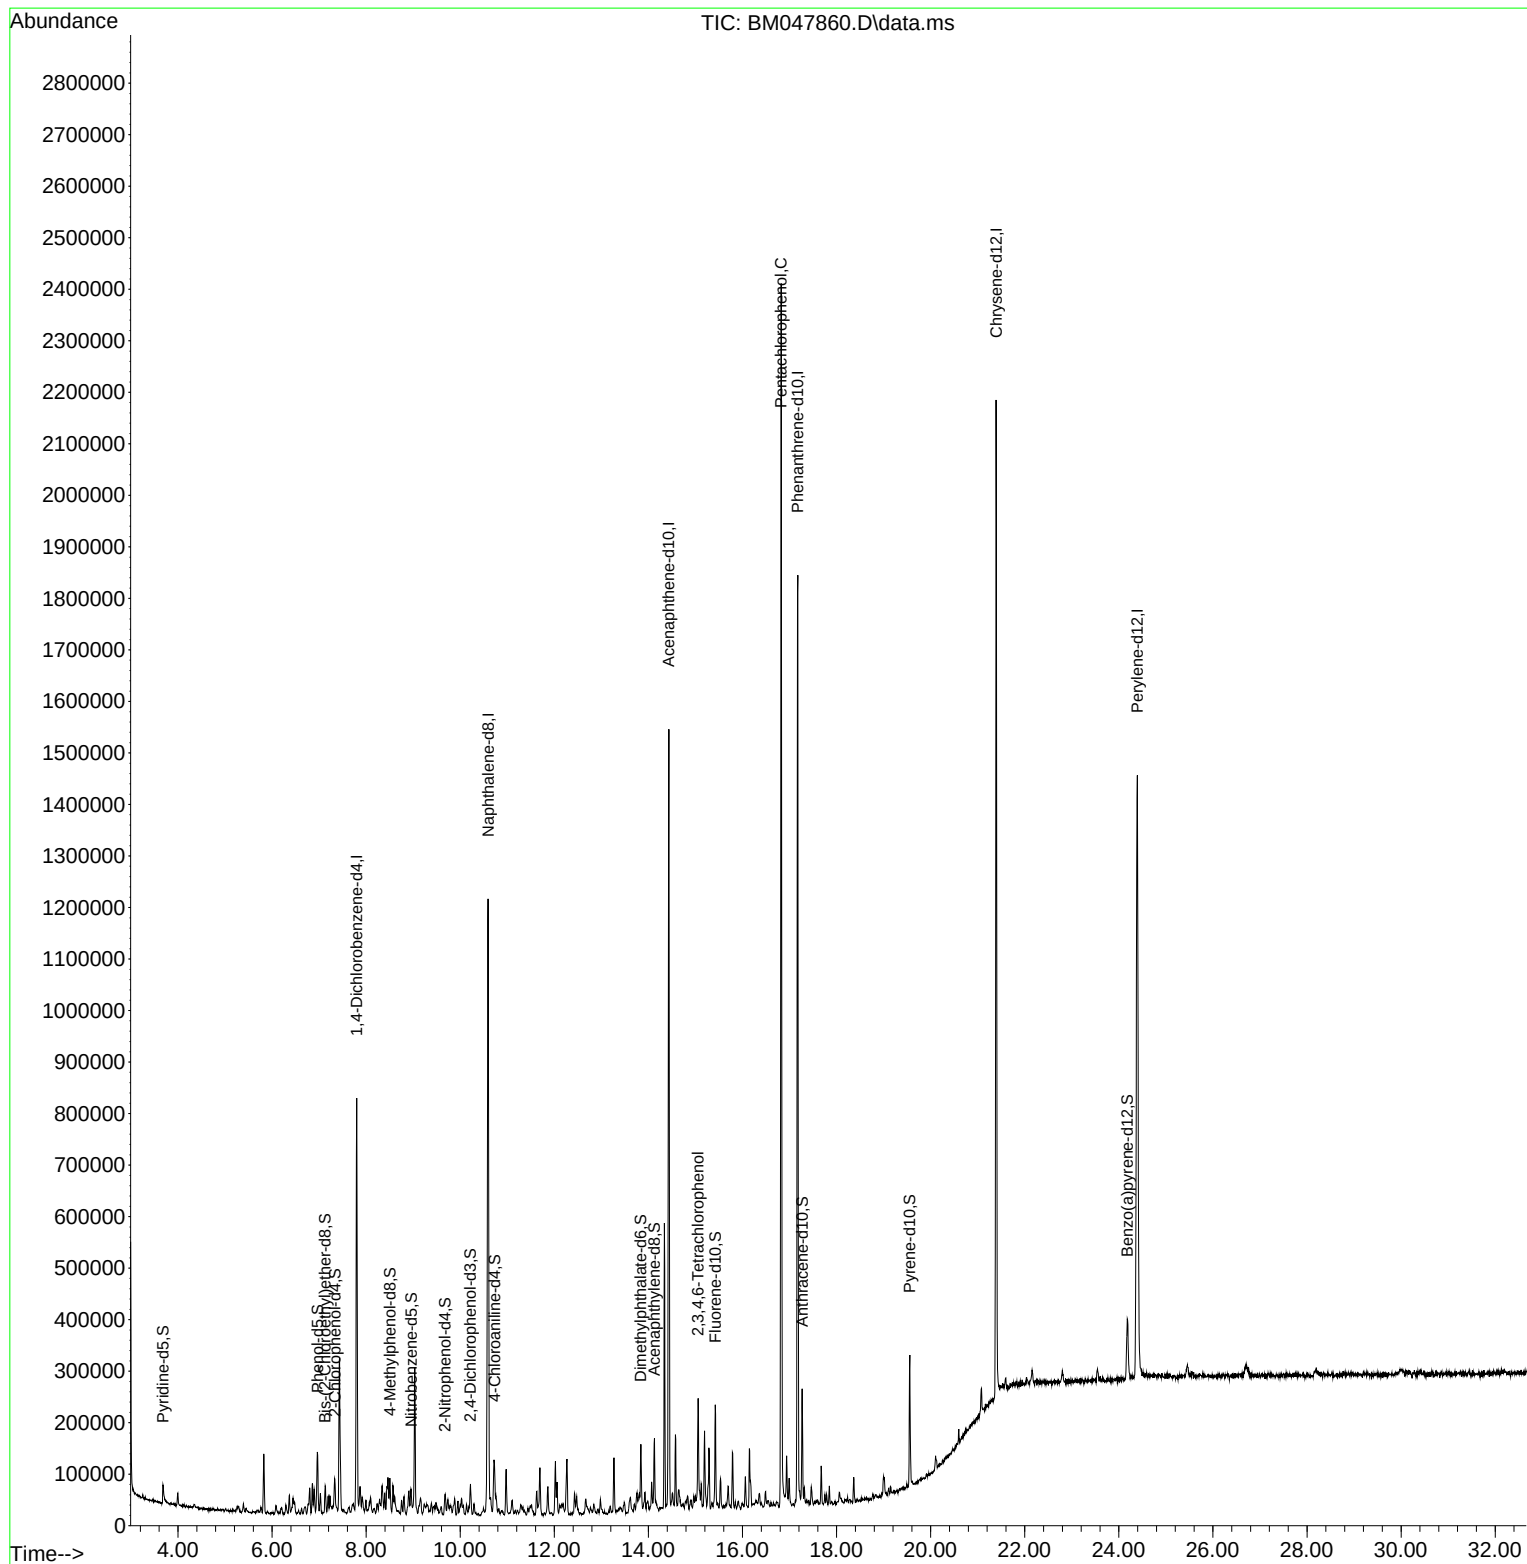


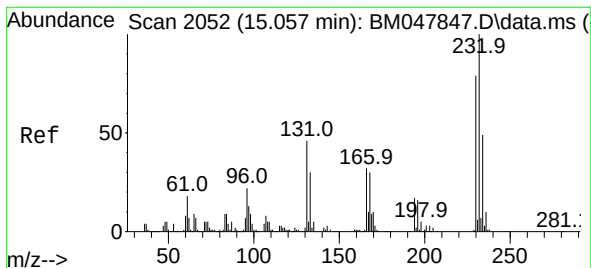

#58
2,3,4,6-Tetrachlorophenol
Concen: 4.669 ng/ul
RT: 15.057 min Scan# 2052
Delta R.T. -0.006 min
Lab File: BM047860.D
Acq: 05 Oct 2024 02:53

Instrument :
BNA_M
ClientSampleId :
DDC96MEDL

Tgt Ion:	232	Resp:	39977
Ion Ratio	Lower	Upper	
232	100		
131	46.6	40.2	60.4
130	3.2	2.6	4.0
166	31.5	25.3	37.9

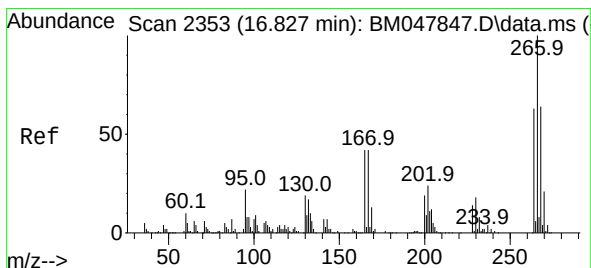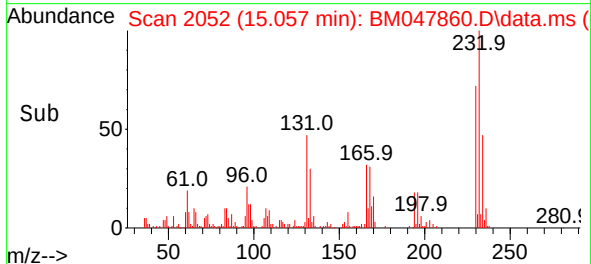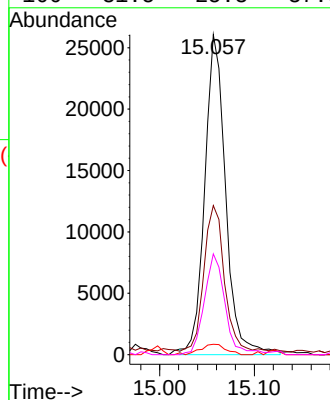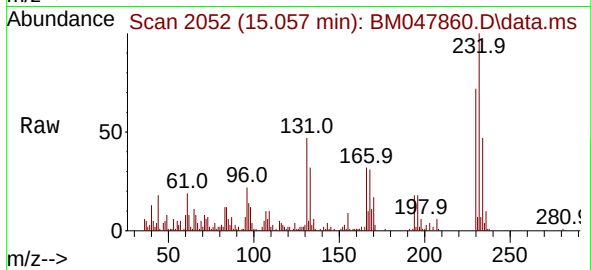

#71
Pentachlorophenol
Concen: 44.980 ng/ul
RT: 16.821 min Scan# 2352
Delta R.T. -0.006 min
Lab File: BM047860.D
Acq: 05 Oct 2024 02:53

Tgt Ion:	266	Resp:	377403
Ion Ratio	Lower	Upper	
266	100		
264	63.0	50.2	75.2
268	64.0	50.9	76.3

