

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047867.D
 Acq On : 05 Oct 2024 08:10
 Operator : RC/JU
 Sample : P4020-05MEDL 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCF9MEDL

Quant Time: Oct 06 00:33:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 08:32:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.798	152	195676	20.000	ng/u1	0.00
20) Naphthalene-d8	10.592	136	786633	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.433	164	473652	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.168	188	978780	20.000	ng/u1	0.00
79) Chrysene-d12	21.392	240	892475	20.000	ng/u1	0.00
88) Perylene-d12	24.385	264	1007056	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	3693	0.610	ng/uL	0.00
4) Pyridine-d5	3.675	84	43237	2.439	ng/u1	0.01
7) Phenol-d5	6.963	99	52281	2.826	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	37928	2.889	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	42869	3.184	ng/u1	0.00
15) 4-Methylphenol-d8	8.504	113	38724	2.815	ng/u1	0.00
21) Nitrobenzene-d5	8.951	128	18371	2.933	ng/u1	0.00
24) 2-Nitrophenol-d4	9.675	143	16693	2.781	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	35682	2.976	ng/u1	0.00
31) 4-Chloroaniline-d4	10.727	131	56380	3.042	ng/u1	0.00
46) Dimethylphthalate-d6	13.839	166	136830	3.985	ng/u1	0.00
49) Acenaphthylene-d8	14.121	160	150036	3.685	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	
60) Fluorene-d10	15.421	176	117722	3.958	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/u1	
73) Anthracene-d10	17.268	188	183813	3.819	ng/u1	0.00
81) Pyrene-d10	19.550	212	205618	4.059	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.180	264	193971	3.712	ng/u1	-0.01
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.821	266	436354	58.447	ng/u1	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047867.D
Acq On : 05 Oct 2024 08:10
Operator : RC/JU
Sample : P4020-05MEDL 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCF9MEDL

Quant Time: Oct 06 00:33:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 08:32:31 2024
Response via : Initial Calibration

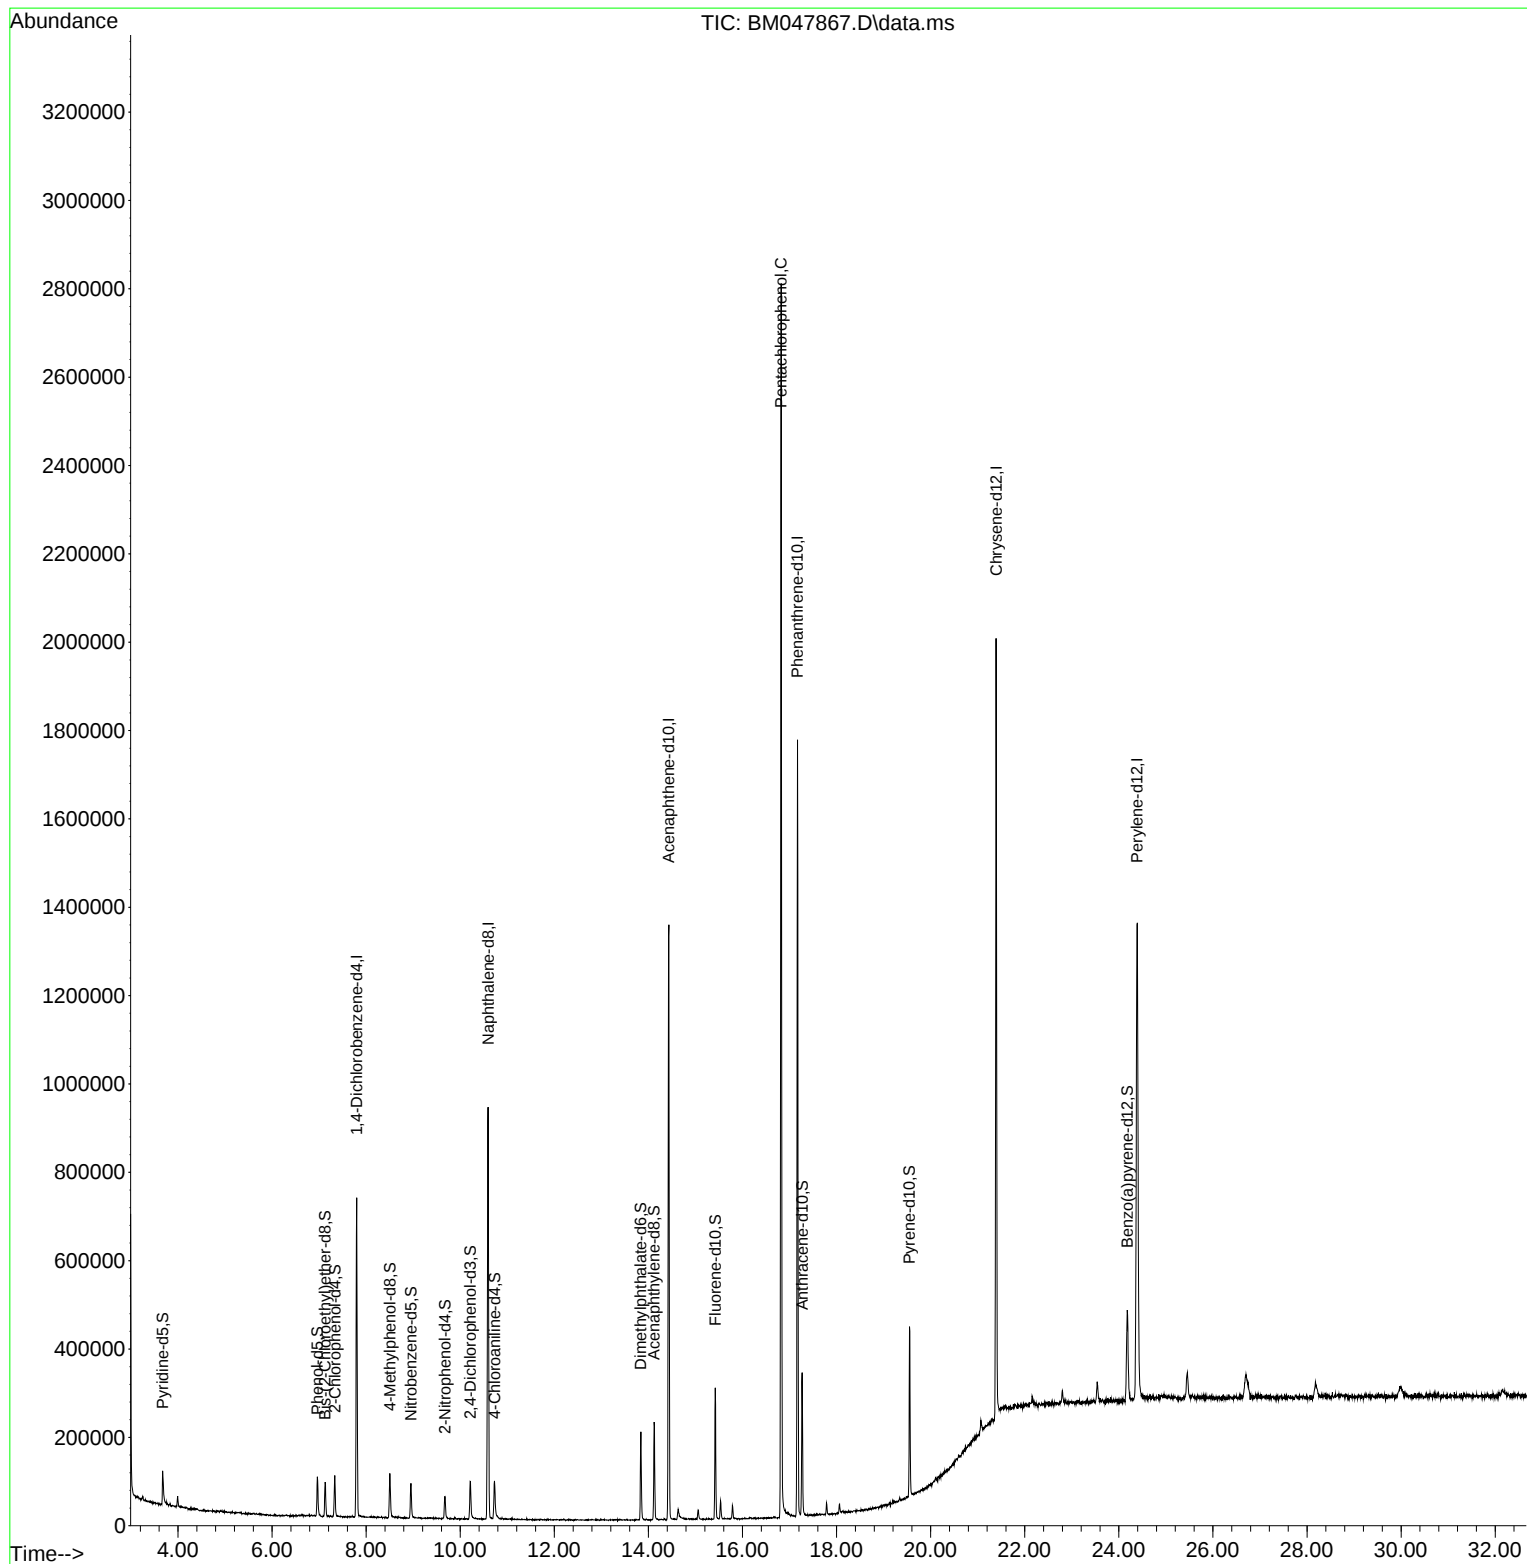

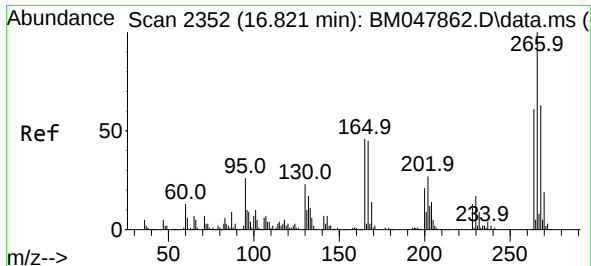

#71
 Pentachlorophenol
 Concen: 58.447 ng/ul
 RT: 16.821 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BM047867.D
 Acq: 05 Oct 2024 08:10

Instrument :
 BNA_M
 ClientSampleId :
 DDCF9MEDL

Tgt Ion:266 Resp: 436354
 Ion Ratio Lower Upper
 266 100
 264 62.9 50.2 75.2
 268 63.6 50.9 76.3

