

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047805.D
 Acq On : 03 Oct 2024 12:44
 Operator : RC/JU
 Sample : PB163635BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK635

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047805.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	41	45	53	rVB	65367	91408	2.11%	0.190%
2	3.669	112	116	139	rBV	758175	1233517	28.54%	2.559%
3	3.993	168	171	177	rVB	13485	20172	0.47%	0.042%
4	4.463	248	251	256	rBV5	4431	7910	0.18%	0.016%
5	5.510	425	429	431	rBV5	4593	6902	0.16%	0.014%
6	5.734	466	467	473	rVB5	3309	4523	0.10%	0.009%
7	6.969	671	677	686	rBV	822552	1302733	30.14%	2.702%
8	7.134	697	705	713	rBV	689957	1080587	25.00%	2.241%
9	7.334	732	739	747	rBV	861969	1381863	31.97%	2.866%
10	7.804	811	819	830	rBV	821957	1302058	30.12%	2.701%
11	8.504	930	938	950	rBV	951388	1560382	36.10%	3.237%
12	8.587	950	952	956	rVB5	3827	5288	0.12%	0.011%
13	8.957	1005	1015	1023	rBV	743845	1232950	28.53%	2.557%
14	9.675	1129	1137	1149	rBV	574105	979942	22.67%	2.033%
15	10.216	1222	1229	1242	rBV	912050	1529700	35.39%	3.173%
16	10.592	1286	1293	1302	rBV	1012570	1718013	39.75%	3.563%
17	10.728	1308	1316	1331	rBV	911260	1572684	36.39%	3.262%
18	12.186	1557	1564	1569	rBV2	15494	28489	0.66%	0.059%
19	13.845	1838	1846	1853	rBV	1577249	2183153	50.51%	4.528%
20	14.127	1885	1894	1902	rBV	1750338	2624054	60.71%	5.443%
21	14.269	1913	1918	1926	rVV8	9136	19746	0.46%	0.041%
22	14.433	1940	1946	1957	rVV	1438604	2196253	50.81%	4.555%
23	14.627	1971	1979	1991	rBV	649164	1010937	23.39%	2.097%
24	14.857	2014	2018	2022	rVV7	4294	5959	0.14%	0.012%
25	15.427	2109	2115	2128	rBV	2311781	3205794	74.17%	6.649%
26	15.539	2128	2134	2145	rVV	686980	906202	20.97%	1.880%
27	15.669	2152	2156	2161	rVB4	10897	13833	0.32%	0.029%
28	15.992	2208	2211	2216	rBV6	2865	4599	0.11%	0.010%
29	16.592	2306	2313	2314	rBV7	2612	4513	0.10%	0.009%
30	16.827	2350	2353	2355	rBV4	5503	6352	0.15%	0.013%
31	16.963	2372	2376	2380	rBV5	5107	8292	0.19%	0.017%
32	17.174	2406	2412	2422	rBV	1892017	2575726	59.59%	5.343%
33	17.274	2422	2429	2444	rBV	2441572	3445030	79.70%	7.146%
34	18.068	2560	2564	2569	rBV8	23250	42332	0.98%	0.088%
35	19.127	2740	2744	2750	rBV4	28189	43137	1.00%	0.089%
36	19.198	2752	2756	2759	rBV	27557	38408	0.89%	0.080%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047805.D
Acq On : 03 Oct 2024 12:44
Operator : RC/JU
Sample : PB163635BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK635

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37	19.351	2778	2782	2788	rBV7	16276	30745	0.71%	0.064%
38	19.562	2812	2818	2830	rBV	3074603	4069867	94.16%	8.442%
39	21.403	3125	3131	3140	rBV	1939849	2979087	68.92%	6.179%
40	24.197	3598	3606	3623	rVB	1745888	4322260	100.00%	8.965%
41	24.403	3633	3641	3658	rVB2	1292338	3416277	79.04%	7.086%




Sum of corrected areas: 48211677

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047805.D
Acq On : 03 Oct 2024 12:44
Operator : RC/JU
Sample : PB163635BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK635

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

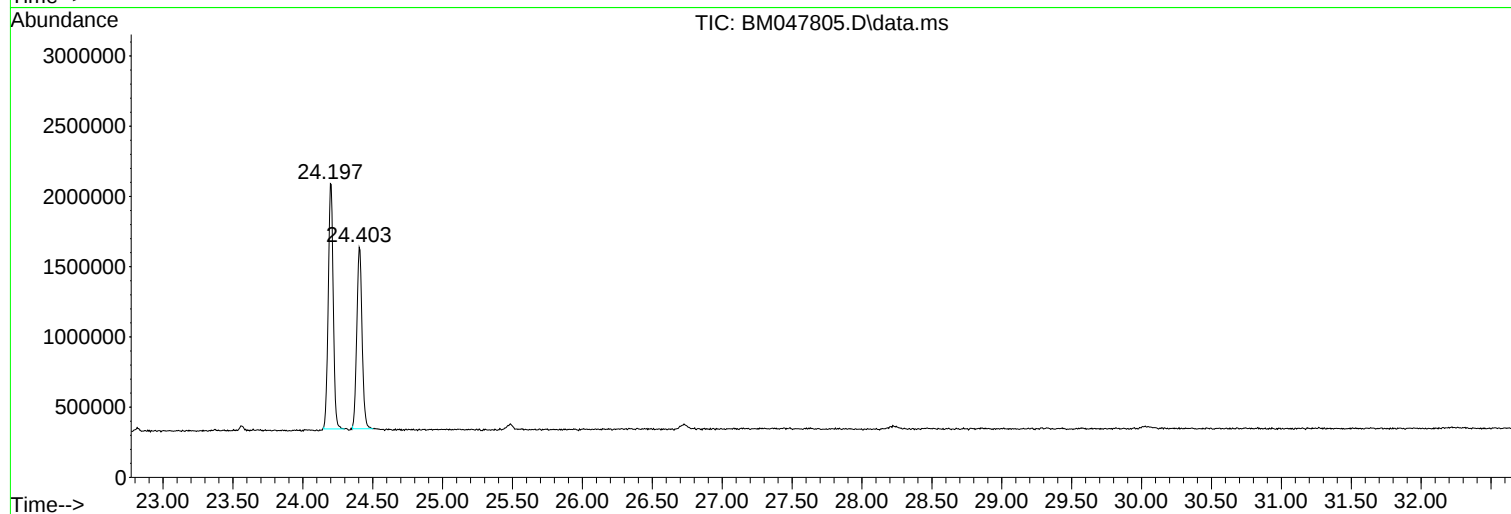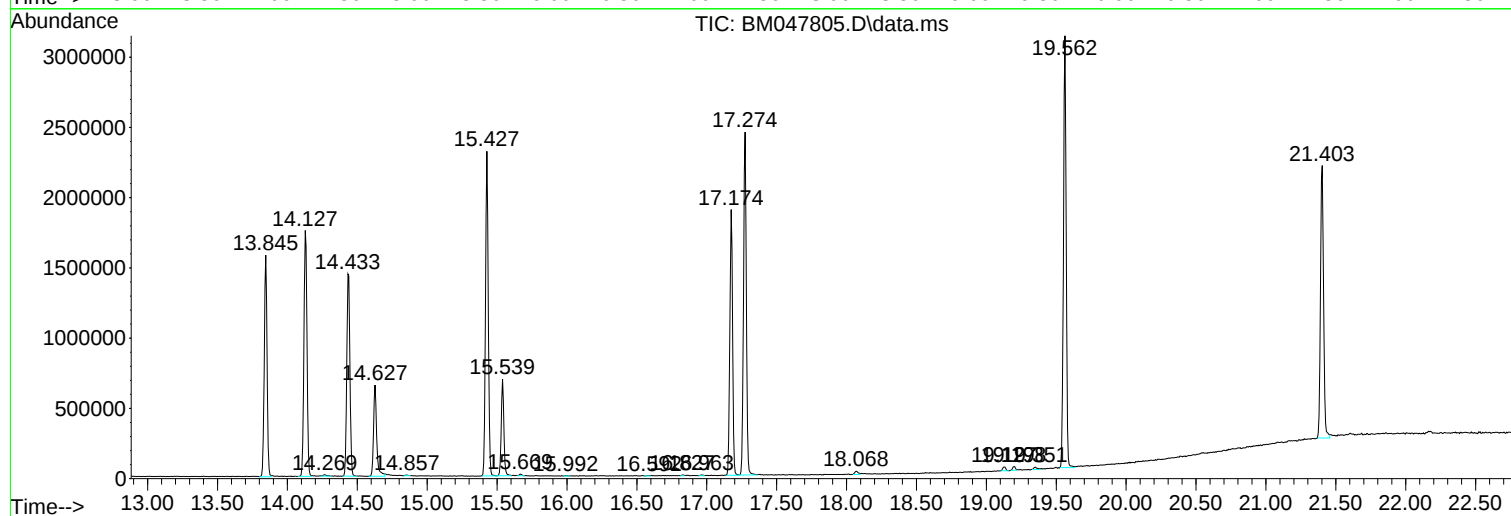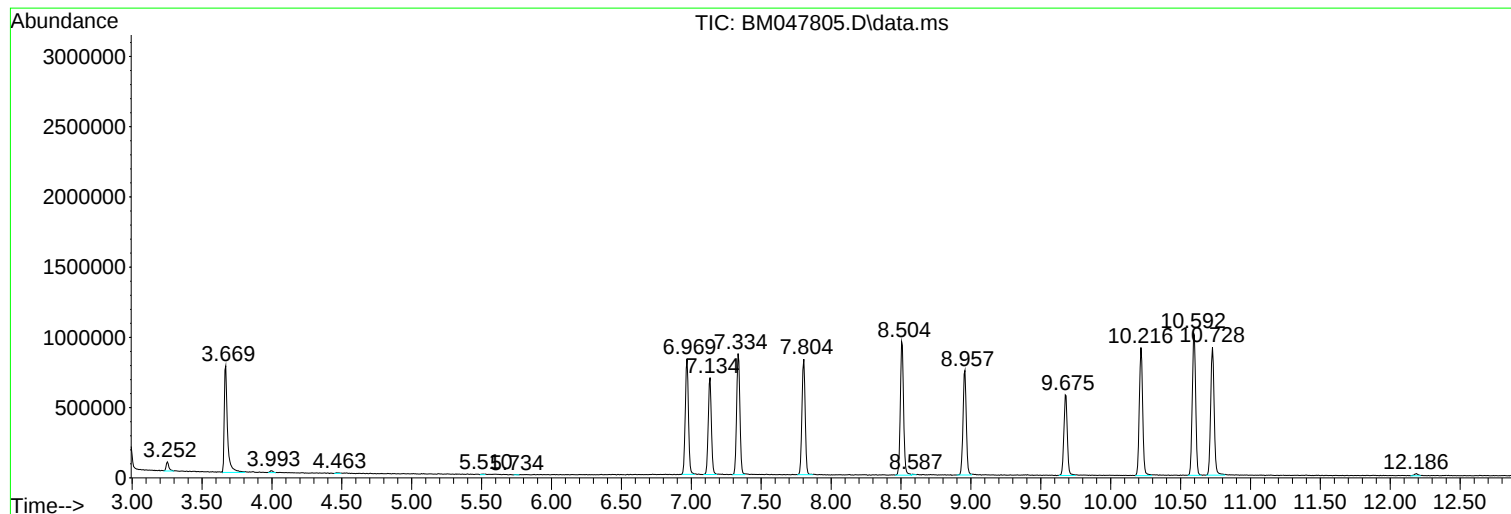

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047805.D
Acq On : 03 Oct 2024 12:44
Operator : RC/JU
Sample : PB163635BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK635

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047805.D
Acq On : 03 Oct 2024 12:44
Operator : RC/JU
Sample : PB163635BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK635

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------