

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047806.D
 Acq On : 03 Oct 2024 13:24
 Operator : RC/JU
 Sample : P4020-10DL 30X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCK1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047806.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.998	168	172	179	rVB	37342	53805	0.66%	0.222%
2	6.969	672	677	682	rVB4	14934	26777	0.33%	0.110%
3	7.134	699	705	709	rBV3	12566	20981	0.26%	0.086%
4	7.339	735	740	745	rBV	15118	22774	0.28%	0.094%
5	7.804	809	819	829	rBV	778975	1247788	15.31%	5.140%
6	8.510	934	939	948	rVB5	13589	26836	0.33%	0.111%
7	8.957	1011	1015	1021	rBV2	9893	16603	0.20%	0.068%
8	9.686	1131	1139	1142	rBV8	8181	14220	0.17%	0.059%
9	10.222	1224	1230	1235	rBV4	12129	25016	0.31%	0.103%
10	10.598	1285	1294	1304	rBV	1026275	1765368	21.66%	7.271%
11	10.733	1312	1317	1325	rVB3	13140	23026	0.28%	0.095%
12	13.845	1842	1846	1851	rBV	36688	49138	0.60%	0.202%
13	14.133	1886	1895	1901	rBV	36708	64209	0.79%	0.264%
14	14.268	1911	1918	1922	rBV5	7552	15139	0.19%	0.062%
15	14.345	1927	1931	1937	rVB2	42273	57409	0.70%	0.236%
16	14.433	1940	1946	1957	rBV	1581622	2375348	29.15%	9.784%
17	14.657	1978	1984	1990	rVB8	5889	11802	0.14%	0.049%
18	15.062	2046	2053	2063	rBV5	20960	31924	0.39%	0.131%
19	15.427	2109	2115	2121	rBV2	53303	77107	0.95%	0.318%
20	15.539	2131	2134	2142	rVB4	10309	16290	0.20%	0.067%
21	15.792	2173	2177	2180	rBV5	6768	8882	0.11%	0.037%
22	16.827	2346	2353	2369	rBV	5825801	8148949	100.00%	33.565%
23	17.174	2406	2412	2423	rBV	2131513	2937520	36.05%	12.100%
24	17.274	2423	2429	2435	rVB	56474	85917	1.05%	0.354%
25	18.068	2559	2564	2569	rBV5	27128	43682	0.54%	0.180%
26	19.345	2779	2781	2784	rBV3	13408	13740	0.17%	0.057%
27	19.562	2813	2818	2822	rBV	75128	106655	1.31%	0.439%
28	21.403	3125	3131	3146	rBV	2076469	3301989	40.52%	13.601%
29	24.403	3633	3641	3655	rVB	1416780	3689057	45.27%	15.195%




Sum of corrected areas: 24277951

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047806.D
Acq On : 03 Oct 2024 13:24
Operator : RC/JU
Sample : P4020-10DL 30X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCK1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

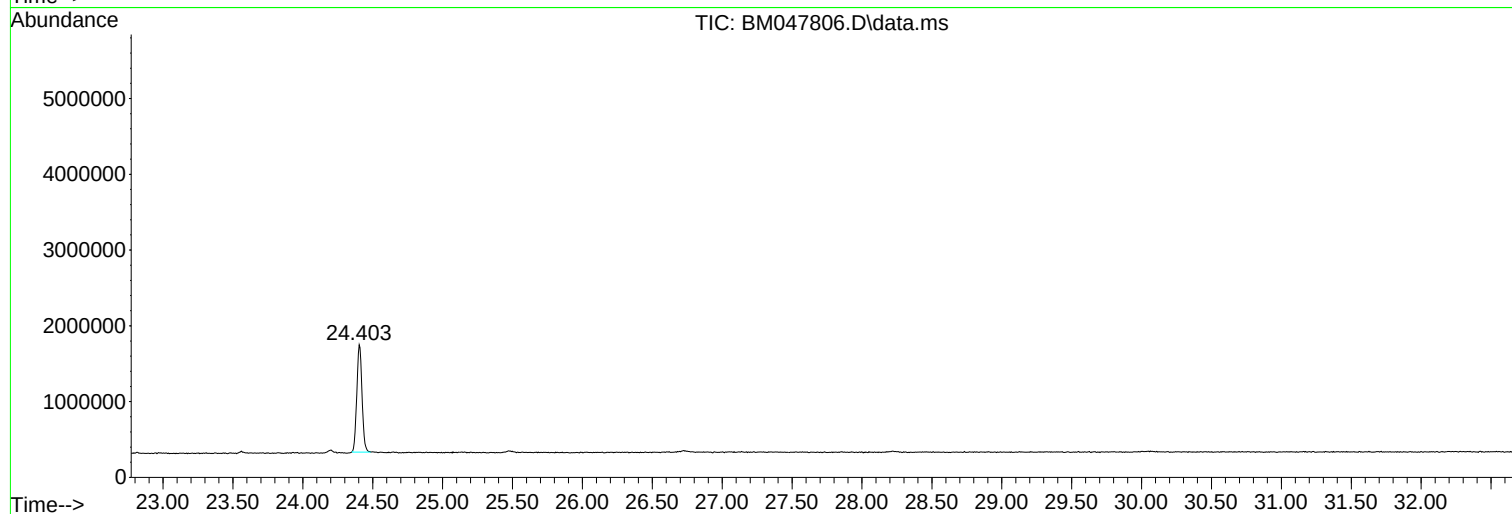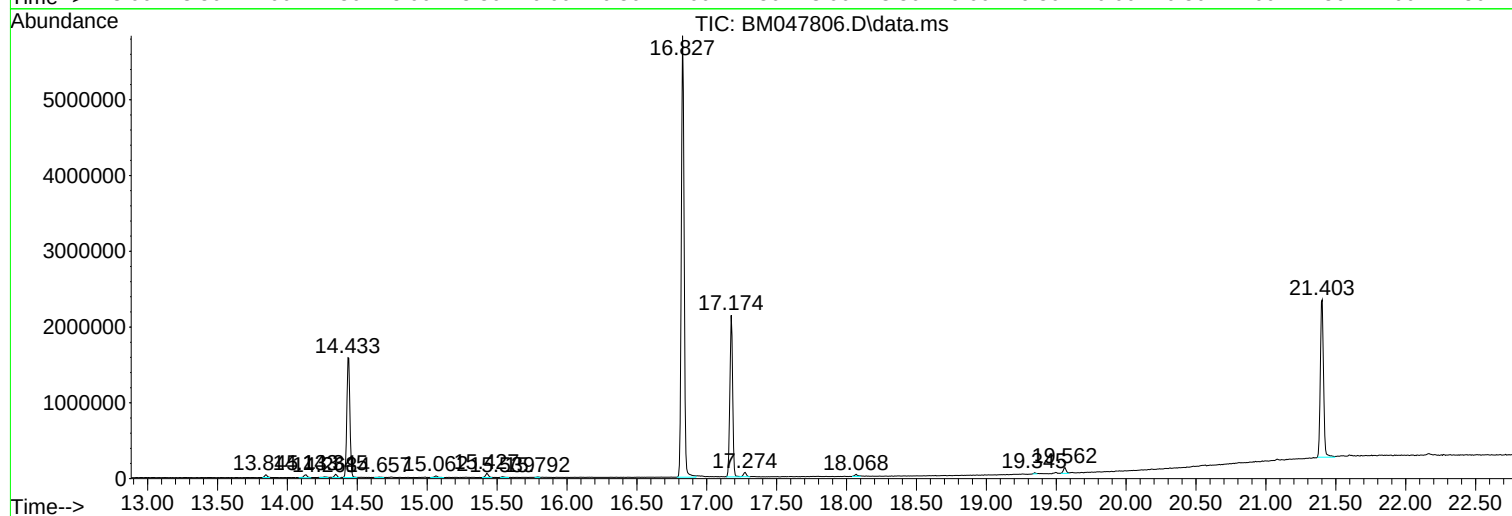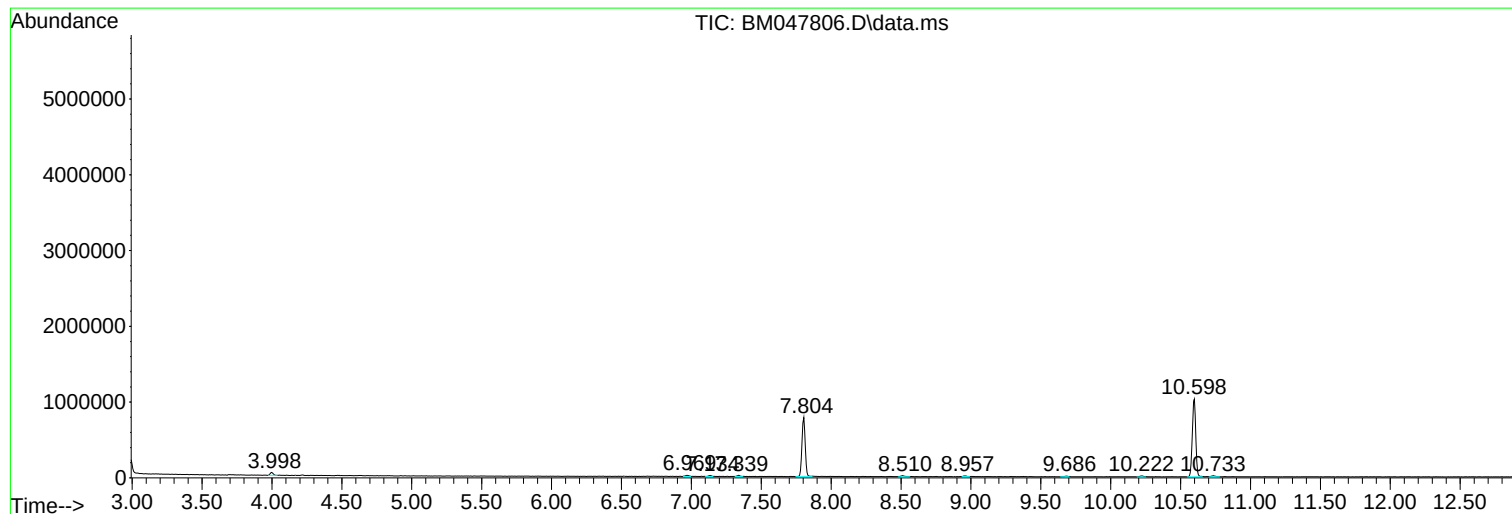

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047806.D
Acq On : 03 Oct 2024 13:24
Operator : RC/JU
Sample : P4020-10DL 30X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCK1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047806.D
Acq On : 03 Oct 2024 13:24
Operator : RC/JU
Sample : P4020-10DL 30X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCK1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
