

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047813.D
 Acq On : 03 Oct 2024 18:00
 Operator : RC/JU
 Sample : P4020-05DL 30X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCF9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047813.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.693	117	120	125	rBV4	10880	15804	0.15%	0.081%
2	4.216	207	209	213	rVB4	11771	13711	0.13%	0.071%
3	6.963	671	676	682	rBV4	13711	25799	0.24%	0.133%
4	7.134	700	705	709	rBV	15165	23531	0.22%	0.121%
5	7.339	735	740	745	rVB2	14045	22461	0.21%	0.116%
6	7.804	812	819	827	rBV	403812	642437	5.92%	3.308%
7	8.510	935	939	945	rVB3	15247	22806	0.21%	0.117%
8	8.963	1006	1016	1020	rBV3	11800	24575	0.23%	0.127%
9	9.675	1133	1137	1146	rVB6	9057	17278	0.16%	0.089%
10	10.222	1224	1230	1235	rBV4	11160	23845	0.22%	0.123%
11	10.592	1283	1293	1303	rBV	521917	899707	8.30%	4.632%
12	10.739	1312	1318	1325	rBV5	11770	22547	0.21%	0.116%
13	13.845	1839	1846	1853	rBV	41733	62889	0.58%	0.324%
14	14.127	1889	1894	1902	rBV2	43993	65992	0.61%	0.340%
15	14.263	1911	1917	1924	rBV5	9901	25003	0.23%	0.129%
16	14.433	1940	1946	1956	rBV	789704	1202936	11.09%	6.194%
17	15.063	2048	2053	2062	rBV2	66041	105106	0.97%	0.541%
18	15.427	2110	2115	2122	rBV	58533	89213	0.82%	0.459%
19	15.539	2128	2134	2139	rVB8	7945	12961	0.12%	0.067%
20	15.792	2174	2177	2182	rVB4	8704	11196	0.10%	0.058%
21	16.827	2346	2353	2368	rBV	7845251	10846012	100.00%	55.843%
22	16.980	2377	2379	2387	rVB9	8725	14168	0.13%	0.073%
23	17.174	2406	2412	2422	rVV	1066500	1474685	13.60%	7.593%
24	17.274	2424	2429	2439	rVB2	61808	93329	0.86%	0.481%
25	17.792	2513	2517	2520	rVB6	7813	11646	0.11%	0.060%
26	18.068	2560	2564	2570	rBV8	14104	24956	0.23%	0.128%
27	19.556	2813	2817	2823	rBV2	80479	117762	1.09%	0.606%
28	21.397	3125	3130	3142	rBV2	1144084	1665425	15.36%	8.575%
29	24.397	3633	3640	3652	rVB	735727	1844476	17.01%	9.497%




Sum of corrected areas: 19422256

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047813.D
Acq On : 03 Oct 2024 18:00
Operator : RC/JU
Sample : P4020-05DL 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCF9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

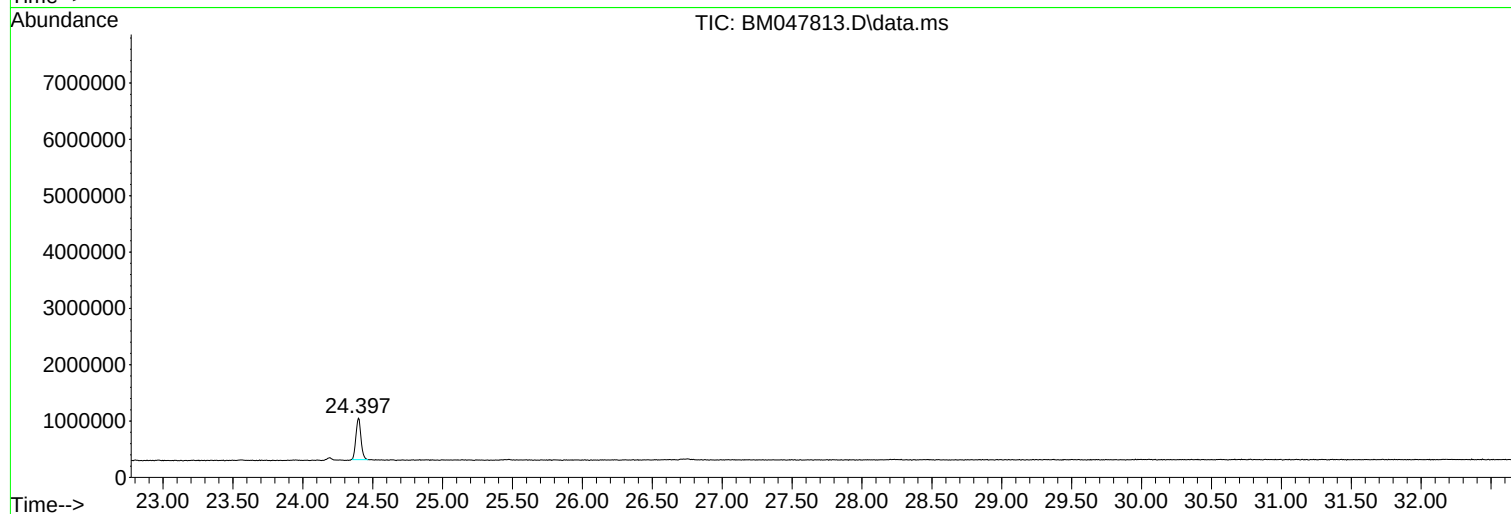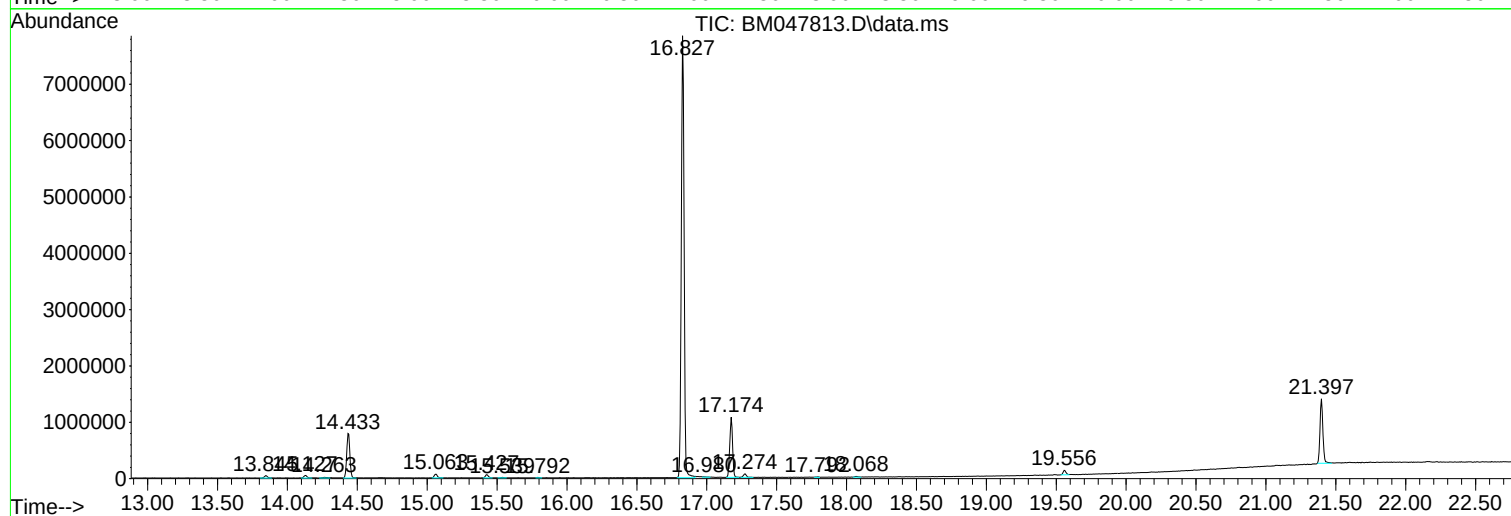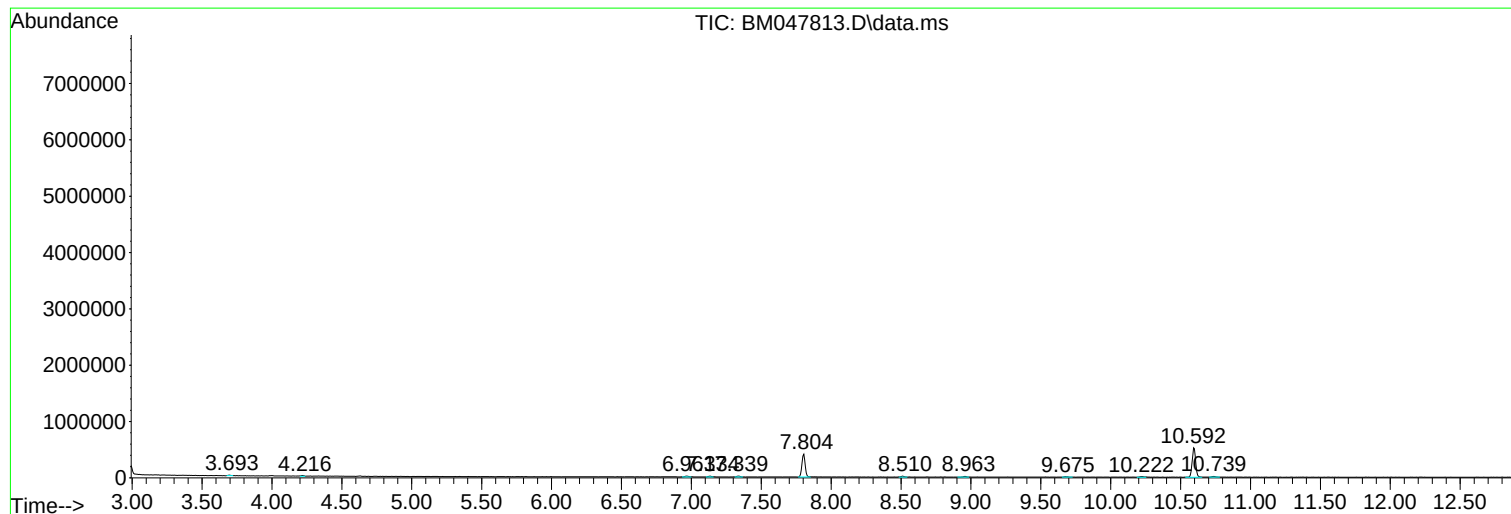

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047813.D
Acq On : 03 Oct 2024 18:00
Operator : RC/JU
Sample : P4020-05DL 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCF9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047813.D
Acq On : 03 Oct 2024 18:00
Operator : RC/JU
Sample : P4020-05DL 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCF9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc