

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047819.D
 Acq On : 03 Oct 2024 22:36
 Operator : RC/JU
 Sample : PB163635BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK635

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047819.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	41	45	52	rVB	74167	101133	2.17%	0.190%
2	3.663	112	115	138	rBV	838153	1349853	29.00%	2.533%
3	3.999	168	172	177	rVB3	15443	23747	0.51%	0.045%
4	6.969	670	677	689	rBV	901709	1450877	31.17%	2.723%
5	7.134	698	705	715	rVB	739490	1191681	25.60%	2.236%
6	7.334	732	739	749	rBV	955010	1509773	32.44%	2.833%
7	7.804	811	819	828	rBV	873744	1410240	30.30%	2.646%
8	8.504	929	938	950	rBV	1092251	1733236	37.24%	3.253%
9	8.957	1007	1015	1027	rBV	814509	1385833	29.77%	2.601%
10	9.675	1128	1137	1149	rBV	655522	1078985	23.18%	2.025%
11	10.216	1222	1229	1242	rBV	1027198	1696464	36.45%	3.184%
12	10.592	1285	1293	1303	rBV	1130171	1926803	41.40%	3.616%
13	10.728	1308	1316	1332	rBV	993953	1765636	37.93%	3.313%
14	12.186	1557	1564	1570	rBV3	15616	29835	0.64%	0.056%
15	13.845	1839	1846	1858	rBV	1767797	2410507	51.79%	4.524%
16	14.127	1887	1894	1905	rBV	2022511	2951966	63.42%	5.540%
17	14.263	1913	1917	1923	rBV8	8572	15986	0.34%	0.030%
18	14.433	1939	1946	1957	rBV	1669113	2487799	53.45%	4.669%
19	14.627	1973	1979	1996	rBV	697445	1129634	24.27%	2.120%
20	15.239	2081	2083	2088	rBV5	3476	5351	0.11%	0.010%
21	15.427	2108	2115	2125	rBV	2605385	3607827	77.51%	6.771%
22	15.539	2126	2134	2144	rBV	708473	980346	21.06%	1.840%
23	15.668	2151	2156	2162	rVB5	11792	19857	0.43%	0.037%
24	16.004	2208	2213	2217	rVV8	2622	5129	0.11%	0.010%
25	16.674	2323	2327	2331	rBV5	4573	7548	0.16%	0.014%
26	16.968	2372	2377	2380	rBV5	4407	7420	0.16%	0.014%
27	17.174	2405	2412	2421	rBV	2043225	2879234	61.86%	5.403%
28	17.268	2422	2428	2441	rVV	2590938	3822903	82.13%	7.174%
29	19.127	2740	2744	2748	rBV2	31224	39077	0.84%	0.073%
30	19.198	2751	2756	2762	rBV2	34075	56713	1.22%	0.106%
31	19.562	2812	2818	2825	rBV	3229901	4457360	95.77%	8.365%
32	21.397	3124	3130	3145	rBV	2099438	3290113	70.69%	6.174%
33	24.191	3597	3605	3625	rVB	1908682	4654455	100.00%	8.735%
34	24.403	3632	3641	3656	rVB	1408280	3803728	81.72%	7.138%

Sum of corrected areas: 53287049

Instrument :

BNA_M

ClientSampleId :




SBLK635

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047819.D
Acq On : 03 Oct 2024 22:36
Operator : RC/JU
Sample : PB163635BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK635

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

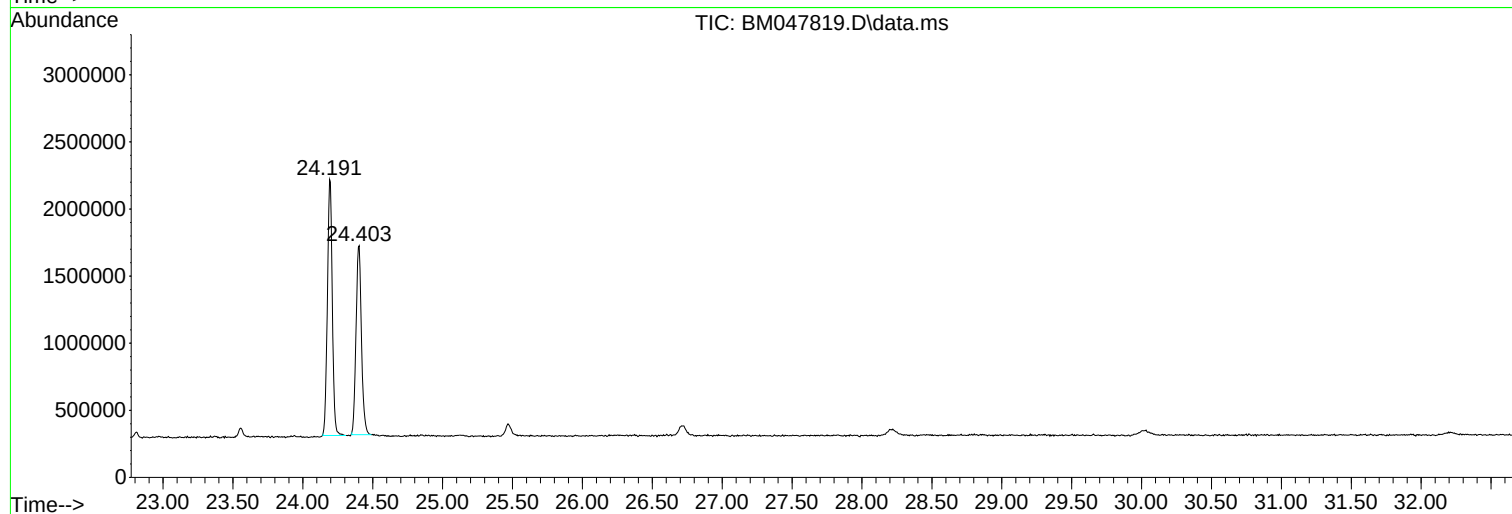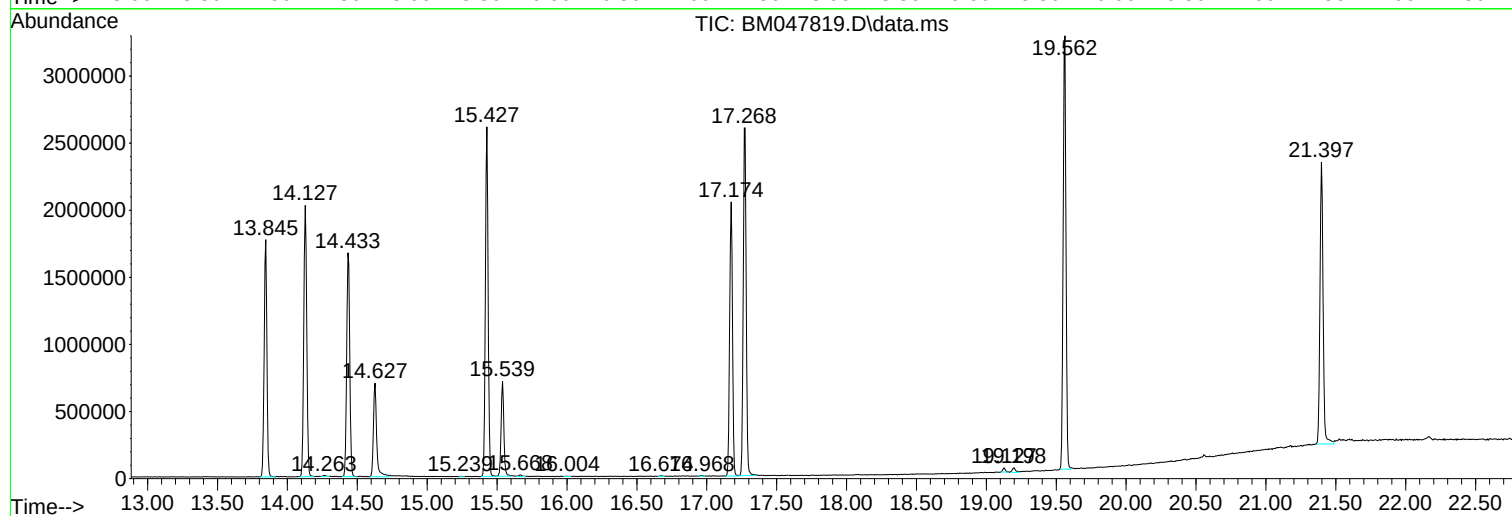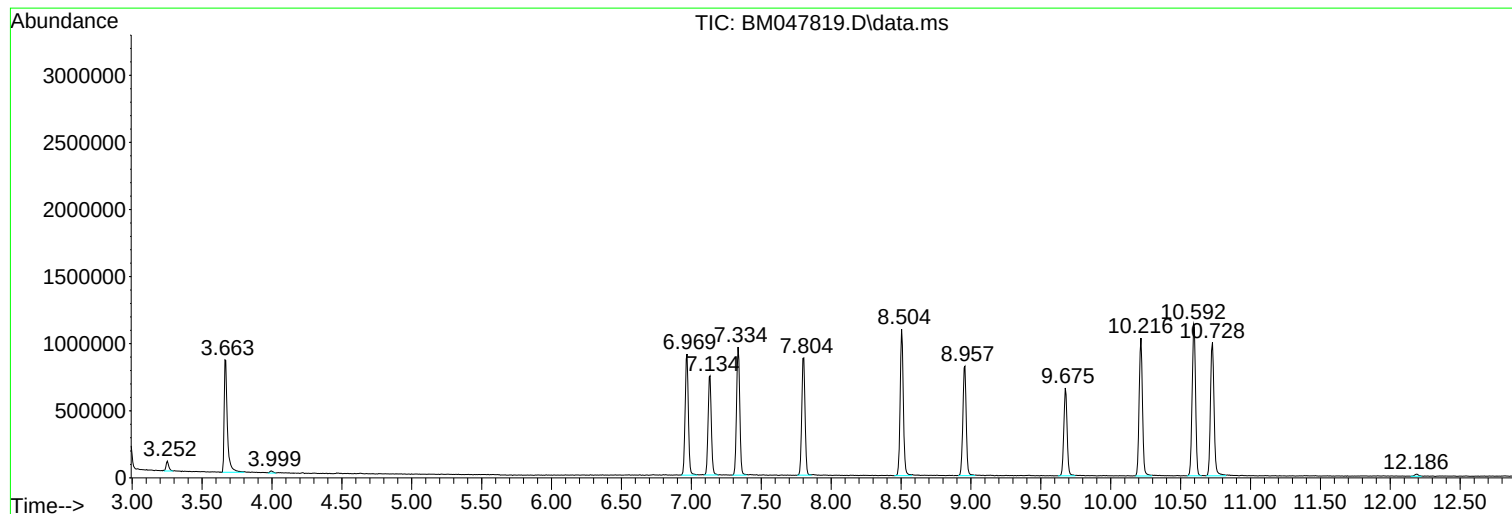

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047819.D
Acq On : 03 Oct 2024 22:36
Operator : RC/JU
Sample : PB163635BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK635

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047819.D
Acq On : 03 Oct 2024 22:36
Operator : RC/JU
Sample : PB163635BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK635

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc