

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047832.D
 Acq On : 04 Oct 2024 07:46
 Operator : RC/JU
 Sample : PB163456BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK456

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047832.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	41	45	53	rVB	93359	130116	1.89%	0.172%
2	3.663	111	115	130	rBV	1206166	1778817	25.86%	2.355%
3	3.999	168	172	180	rVB	29823	45595	0.66%	0.060%
4	4.216	207	209	216	rVB4	12284	14199	0.21%	0.019%
5	6.969	670	677	687	rBV	1261787	2027650	29.48%	2.684%
6	7.128	698	704	716	rVB	1046091	1655302	24.06%	2.191%
7	7.334	732	739	754	rBV	1341852	2082212	30.27%	2.756%
8	7.798	811	818	826	rBV	1117116	1778102	25.85%	2.354%
9	8.504	930	938	954	rBV	1525142	2470928	35.92%	3.271%
10	8.951	1007	1014	1025	rBV	1180412	1942426	28.24%	2.571%
11	9.675	1128	1137	1148	rBV	977136	1593202	23.16%	2.109%
12	10.216	1220	1229	1240	rBV	1441978	2441775	35.50%	3.232%
13	10.292	1240	1242	1245	rVV4	5859	7374	0.11%	0.010%
14	10.592	1286	1293	1302	rBV	1520103	2537264	36.88%	3.358%
15	10.728	1308	1316	1330	rBV	1429653	2535601	36.86%	3.356%
16	12.186	1559	1564	1571	rVB3	20248	36708	0.53%	0.049%
17	13.845	1839	1846	1856	rBV	2572691	3467808	50.41%	4.590%
18	14.127	1887	1894	1904	rBV	2917800	4215924	61.29%	5.580%
19	14.433	1938	1946	1953	rBV	2258025	3280460	47.69%	4.342%
20	14.627	1971	1979	2000	rBV	1189028	1802354	26.20%	2.386%
21	15.427	2107	2115	2124	rBV	3565908	5124505	74.49%	6.783%
22	15.539	2128	2134	2145	rVV	1205816	1607838	23.37%	2.128%
23	15.668	2150	2156	2162	rVB2	15718	29171	0.42%	0.039%
24	16.210	2243	2248	2255	rBV8	8581	15358	0.22%	0.020%
25	16.827	2346	2353	2356	rBV7	12361	21663	0.31%	0.029%
26	16.957	2370	2375	2380	rBV4	5354	8993	0.13%	0.012%
27	17.174	2405	2412	2421	rBV	2621300	3761240	54.68%	4.979%
28	17.268	2422	2428	2448	rVB	3806817	5512261	80.13%	7.296%
29	17.839	2522	2525	2531	rVB6	6131	11170	0.16%	0.015%
30	18.057	2560	2562	2571	rBV9	10737	19366	0.28%	0.026%
31	18.962	2712	2716	2722	rBV7	13199	22165	0.32%	0.029%
32	19.127	2739	2744	2747	rBV2	47741	64227	0.93%	0.085%
33	19.192	2751	2755	2760	rBV	44316	67014	0.97%	0.089%
34	19.492	2804	2806	2809	rVB3	18476	17984	0.26%	0.024%
35	19.556	2811	2817	2824	rBV	4768786	6504513	94.56%	8.610%
36	21.398	3124	3130	3140	rBV	2840107	4193877	60.97%	5.551%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047832.D
Acq On : 04 Oct 2024 07:46
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK456

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37	23.550	3492	3496	3502	rVB2	139447	257857	3.75%	0.341%
38	24.191	3596	3605	3619	rBV2	2860629	6879011	100.00%	9.105%
39	24.397	3631	3640	3655	rBV	1850579	5101248	74.16%	6.752%
40	25.462	3817	3821	3833	rVB3	192683	485080	7.05%	0.642%




Sum of corrected areas: 75548358

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047832.D
Acq On : 04 Oct 2024 07:46
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

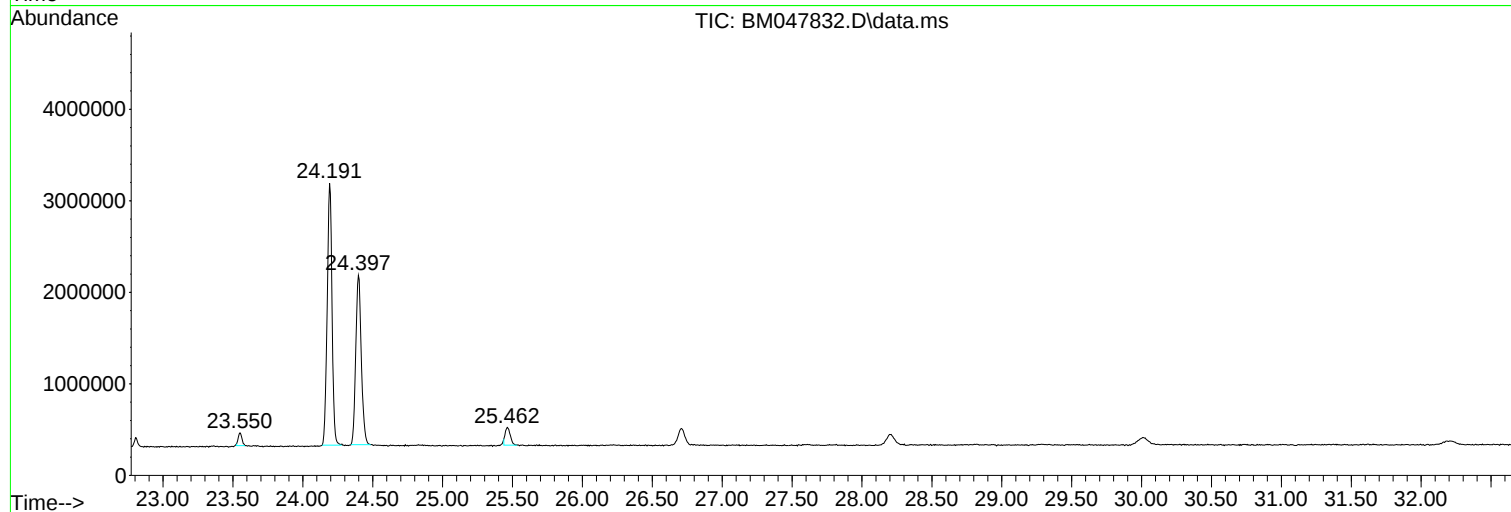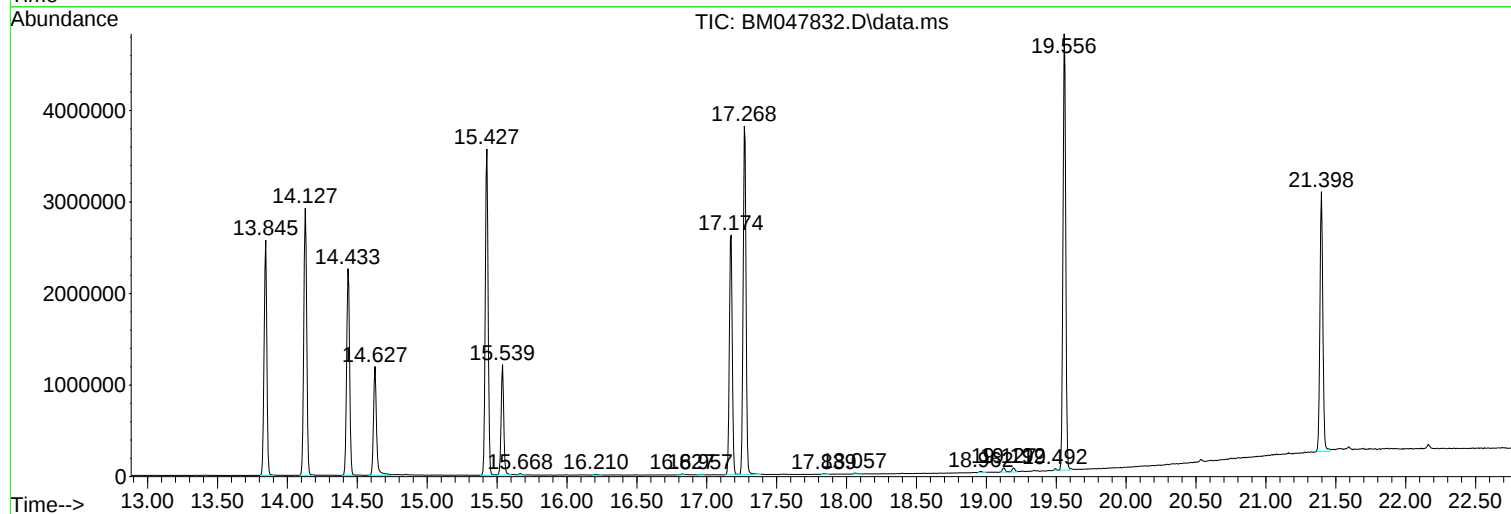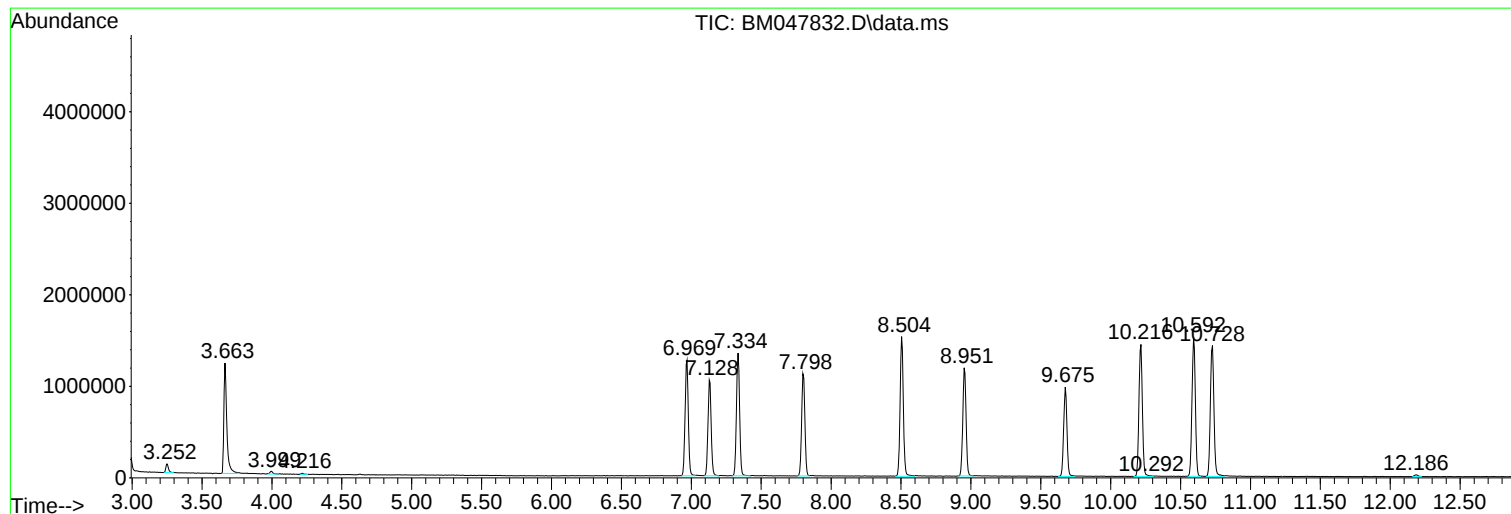

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047832.D
Acq On : 04 Oct 2024 07:46
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047832.D
Acq On : 04 Oct 2024 07:46
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------