

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047833.D
 Acq On : 04 Oct 2024 08:26
 Operator : RC/JU
 Sample : P4020-05DL 30X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCF9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047833.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.687	117	119	123	rBV3	11031	14872	0.12%	0.055%
2	3.993	169	171	176	rVB3	12012	14875	0.12%	0.055%
3	4.216	206	209	213	rVB4	10451	14107	0.11%	0.052%
4	6.969	672	677	682	rBV3	16349	29904	0.23%	0.110%
5	7.134	701	705	712	rVB2	16862	27908	0.22%	0.103%
6	7.334	734	739	745	rBV2	16151	28498	0.22%	0.105%
7	7.798	811	818	827	rBV	672698	1103849	8.64%	4.070%
8	8.510	934	939	947	rBV5	15168	31328	0.25%	0.116%
9	8.957	1008	1015	1023	rBV3	13799	28133	0.22%	0.104%
10	9.675	1133	1137	1143	rBV6	9335	17070	0.13%	0.063%
11	10.222	1223	1230	1237	rBV5	14545	32858	0.26%	0.121%
12	10.592	1284	1293	1306	rBV	947709	1593773	12.48%	5.877%
13	10.739	1312	1318	1324	rBV5	11718	25613	0.20%	0.094%
14	13.845	1839	1846	1855	rBV	48893	73935	0.58%	0.273%
15	14.127	1888	1894	1900	rBV	49864	77647	0.61%	0.286%
16	14.433	1937	1946	1954	rBV	1423384	2116587	16.57%	7.805%
17	15.063	2044	2053	2058	rBV	74357	121605	0.95%	0.448%
18	15.427	2107	2115	2122	rBV	70140	107772	0.84%	0.397%
19	15.539	2129	2134	2140	rBV8	10205	17525	0.14%	0.065%
20	15.792	2172	2177	2180	rBV3	8847	12833	0.10%	0.047%
21	16.827	2346	2353	2372	rBV	8999682	12770181	100.00%	47.089%
22	17.174	2405	2412	2421	rBV	1832577	2593558	20.31%	9.564%
23	17.268	2423	2428	2438	rVB	82211	127717	1.00%	0.471%
24	18.062	2560	2563	2567	rBV5	12800	20014	0.16%	0.074%
25	19.492	2803	2806	2810	rBV6	12269	18753	0.15%	0.069%
26	19.556	2813	2817	2826	rVB	89787	141724	1.11%	0.523%
27	21.397	3124	3130	3136	rBV	1919819	2820304	22.09%	10.400%
28	24.391	3632	3639	3655	rVB	1191264	3136056	24.56%	11.564%




Sum of corrected areas: 27118999

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047833.D
Acq On : 04 Oct 2024 08:26
Operator : RC/JU
Sample : P4020-05DL 30X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCF9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

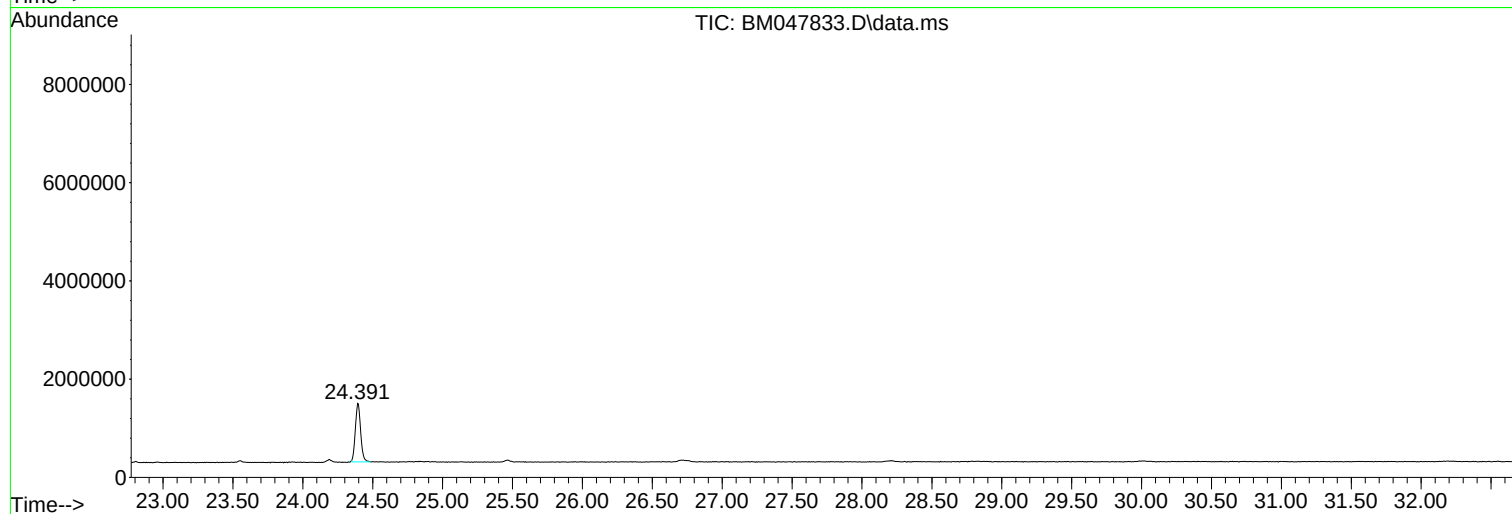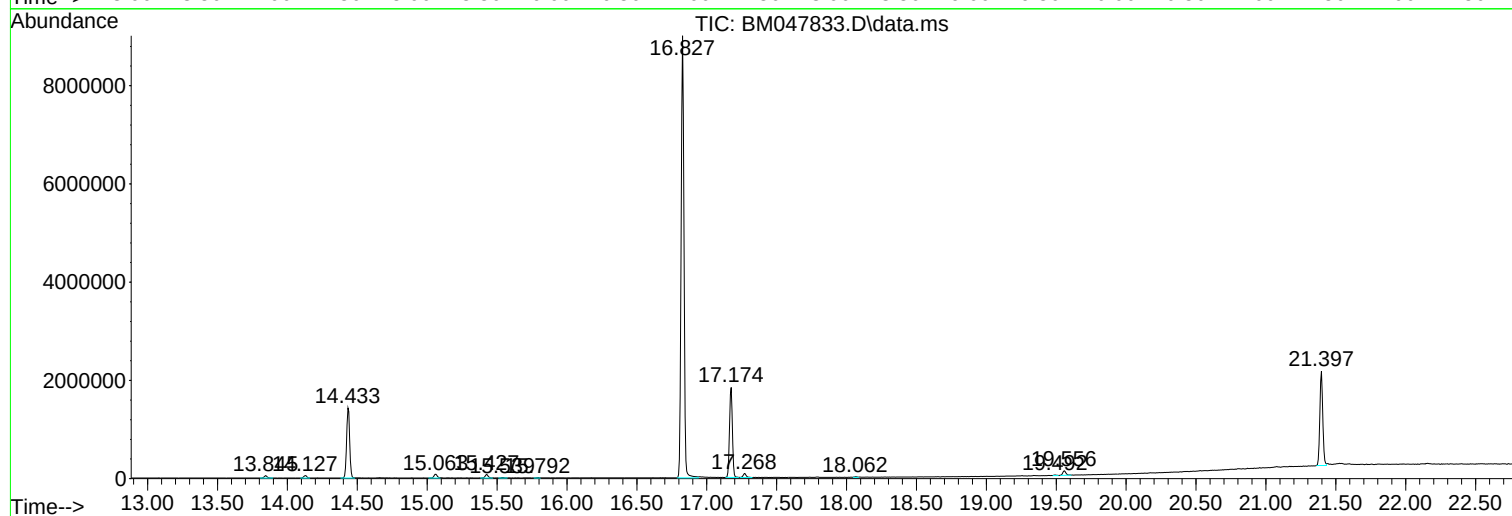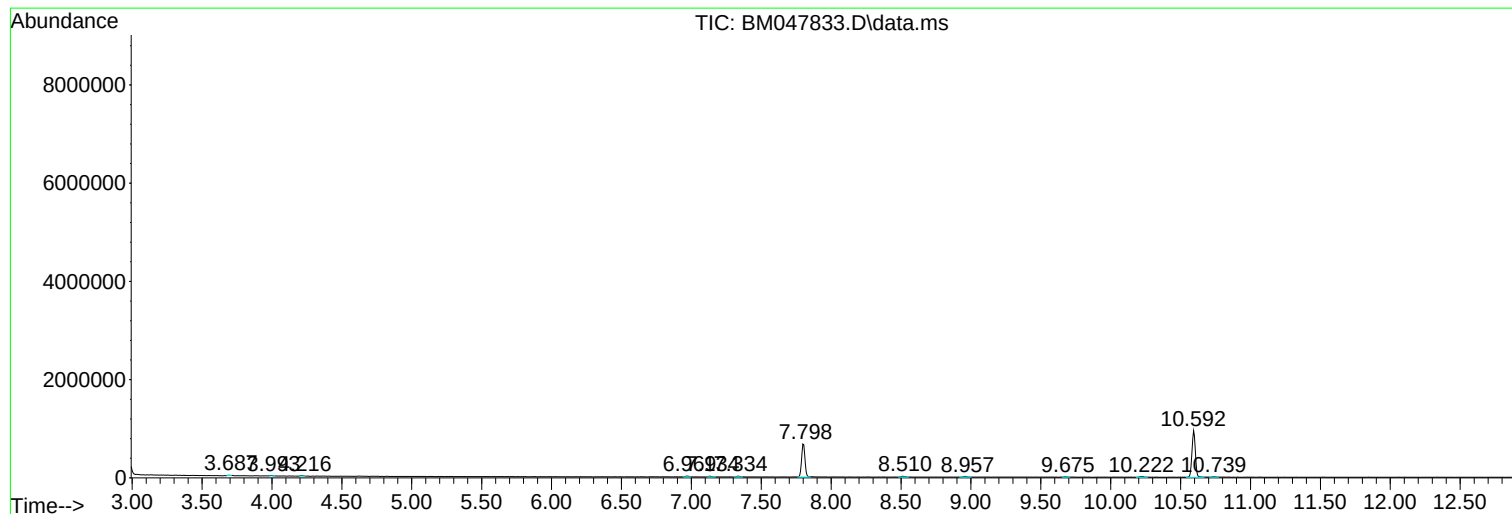

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047833.D
Acq On : 04 Oct 2024 08:26
Operator : RC/JU
Sample : P4020-05DL 30X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCF9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047833.D
Acq On : 04 Oct 2024 08:26
Operator : RC/JU
Sample : P4020-05DL 30X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCF9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------