

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047857.D
 Acq On : 05 Oct 2024 00:53
 Operator : RC/JU
 Sample : P4017-19MEDL 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DD5CD5MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047857.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.687	116	119	125	rBV4	16332	25905	0.86%	0.110%
2	3.993	168	171	177	rVB2	21208	28855	0.96%	0.123%
3	6.887	660	663	670	rVV4	10223	16961	0.56%	0.072%
4	6.969	670	677	683	rVV	75057	137190	4.56%	0.585%
5	7.028	683	687	692	rVB4	9081	15461	0.51%	0.066%
6	7.128	698	704	711	rBV	69998	112196	3.73%	0.479%
7	7.192	712	715	717	rVV3	8822	11551	0.38%	0.049%
8	7.234	719	722	728	rVV4	11149	17044	0.57%	0.073%
9	7.334	732	739	748	rVV	77473	137737	4.58%	0.587%
10	7.445	751	758	766	rVB2	32174	75348	2.51%	0.321%
11	7.798	810	818	827	rBV	794986	1274332	42.38%	5.435%
12	7.869	827	830	835	rVV6	8744	16149	0.54%	0.069%
13	7.922	835	839	846	rVB3	13754	26074	0.87%	0.111%
14	8.175	878	882	887	rVB3	11629	18272	0.61%	0.078%
15	8.286	896	901	904	rVV7	8794	14603	0.49%	0.062%
16	8.339	906	910	916	rVV3	13759	25471	0.85%	0.109%
17	8.398	916	920	923	rVB5	9524	11515	0.38%	0.049%
18	8.439	923	927	930	rBV3	17697	30580	1.02%	0.130%
19	8.504	933	938	945	rVV	81923	143957	4.79%	0.614%
20	8.575	945	950	952	rVV4	11748	19766	0.66%	0.084%
21	8.610	952	956	960	rVB2	9038	15285	0.51%	0.065%
22	8.757	977	981	983	rBV3	9613	12218	0.41%	0.052%
23	8.798	983	988	997	rVB4	26303	50282	1.67%	0.214%
24	8.916	997	1008	1010	rBV3	23936	53072	1.77%	0.226%
25	8.951	1010	1014	1020	rVV	61875	110809	3.69%	0.473%
26	9.033	1023	1028	1033	rVB	57994	85705	2.85%	0.366%
27	9.151	1044	1048	1055	rVB8	13988	29232	0.97%	0.125%
28	9.428	1091	1095	1101	rVB7	8774	11492	0.38%	0.049%
29	9.486	1101	1105	1109	rBV4	10580	18716	0.62%	0.080%
30	9.586	1117	1122	1129	rVB7	9130	19460	0.65%	0.083%
31	9.675	1132	1137	1144	rBV4	49448	91494	3.04%	0.390%
32	9.739	1144	1148	1152	rVB6	8088	12560	0.42%	0.054%
33	9.810	1154	1160	1163	rVB6	6512	11423	0.38%	0.049%
34	9.880	1169	1172	1179	rVB5	10774	17896	0.60%	0.076%
35	9.945	1179	1183	1187	rBV7	8211	12381	0.41%	0.053%
36	10.004	1187	1193	1195	rBV6	9776	16602	0.55%	0.071%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047857.D
 Acq On : 05 Oct 2024 00:53
 Operator : RC/JU
 Sample : P4017-19MEDL 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DD5CD5MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

37	10.063	1202	1203	1211	rVB7	9728	12846	0.43%	0.055%
38	10.216	1219	1229	1238	rVV	76972	162884	5.42%	0.695%
39	10.286	1238	1241	1246	rVB5	12006	20650	0.69%	0.088%
40	10.592	1281	1293	1299	rBV2	1431071	2444670	81.31%	10.427%
41	10.639	1299	1301	1306	rVV2	20742	29771	0.99%	0.127%
42	10.716	1308	1314	1327	rVV3	124995	288523	9.60%	1.231%
43	10.886	1337	1343	1348	rVB8	9421	19572	0.65%	0.083%
44	10.975	1353	1358	1366	rBV2	34972	63566	2.11%	0.271%
45	11.104	1371	1380	1386	rBV5	18648	42857	1.43%	0.183%
46	11.486	1440	1445	1453	rBV6	27011	68411	2.28%	0.292%
47	11.627	1463	1469	1475	rBV7	11876	20524	0.68%	0.088%
48	11.833	1498	1504	1514	rBV7	20177	56080	1.87%	0.239%
49	12.022	1529	1536	1540	rBV3	35719	69131	2.30%	0.295%
50	12.257	1570	1576	1585	rVB	46463	82414	2.74%	0.352%
51	12.433	1601	1606	1609	rBV4	31320	52284	1.74%	0.223%
52	12.474	1609	1613	1618	rVV3	27811	47479	1.58%	0.203%
53	12.980	1695	1699	1700	rVV4	7556	10679	0.36%	0.046%
54	13.010	1700	1704	1709	rVV	27522	44441	1.48%	0.190%
55	13.263	1743	1747	1755	rBV3	34009	53894	1.79%	0.230%
56	13.486	1776	1785	1791	rBV7	17730	42224	1.40%	0.180%
57	13.610	1798	1806	1813	rBV7	27979	74659	2.48%	0.318%
58	13.757	1821	1831	1835	rBV3	33312	68967	2.29%	0.294%
59	13.839	1837	1845	1851	rVV	189078	301491	10.03%	1.286%
60	13.927	1855	1860	1864	rVB7	11087	20340	0.68%	0.087%
61	13.992	1864	1871	1876	rBV8	17196	38565	1.28%	0.164%
62	14.127	1888	1894	1898	rBV	201717	290471	9.66%	1.239%
63	14.339	1925	1930	1935	rBV2	40925	55757	1.85%	0.238%
64	14.386	1935	1938	1940	rVV4	10188	13884	0.46%	0.059%
65	14.433	1940	1946	1954	rVV	1560662	2290368	76.18%	9.769%
66	14.521	1956	1961	1965	rVB4	35878	56096	1.87%	0.239%
67	14.639	1976	1981	1986	rBV6	32791	73582	2.45%	0.314%
68	14.680	1986	1988	1992	rVB4	14715	19258	0.64%	0.082%
69	14.786	2002	2006	2009	rBV6	7147	10790	0.36%	0.046%
70	14.833	2009	2014	2020	rVB3	20687	36307	1.21%	0.155%
71	14.904	2020	2026	2031	rBV4	16314	27439	0.91%	0.117%
72	14.968	2033	2037	2041	rVB7	10253	19383	0.64%	0.083%
73	15.057	2041	2052	2058	rBV	151978	253226	8.42%	1.080%
74	15.104	2058	2060	2067	rVB3	13549	16020	0.53%	0.068%
75	15.221	2075	2080	2084	rVV7	12728	25325	0.84%	0.108%
76	15.292	2088	2092	2095	rVB2	40241	51506	1.71%	0.220%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047857.D
 Acq On : 05 Oct 2024 00:53
 Operator : RC/JU
 Sample : P4017-19MEDL 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCD5MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

77	15.421	2108	2114	2121	rVV	268052	405558	13.49%	1.730%
78	15.533	2127	2133	2140	rVV4	43512	71061	2.36%	0.303%
79	15.698	2154	2161	2166	rVB5	18428	30150	1.00%	0.129%
80	15.786	2171	2176	2183	rBV	108598	159585	5.31%	0.681%
81	15.986	2207	2210	2214	rBV6	10317	16237	0.54%	0.069%
82	16.151	2234	2238	2241	rBV	46484	69856	2.32%	0.298%
83	16.351	2266	2272	2278	rBV7	12670	25229	0.84%	0.108%
84	16.486	2292	2295	2299	rVB6	7532	10560	0.35%	0.045%
85	16.821	2346	2352	2365	rBV	1565931	2244521	74.65%	9.573%
86	16.939	2368	2372	2377	rVV2	49028	77446	2.58%	0.330%
87	16.992	2377	2381	2391	rVB6	24263	45441	1.51%	0.194%
88	17.174	2405	2412	2418	rBV	1853120	2697718	89.73%	11.506%
89	17.268	2422	2428	2440	rVB	301190	441329	14.68%	1.882%
90	17.674	2492	2497	2502	rBV	40001	53278	1.77%	0.227%
91	17.756	2507	2511	2513	rVV3	10224	16130	0.54%	0.069%
92	17.786	2513	2516	2520	rVB6	20580	27328	0.91%	0.117%
93	18.068	2557	2564	2566	rBV6	21862	37520	1.25%	0.160%
94	18.362	2610	2614	2620	rBV2	33505	43878	1.46%	0.187%
95	18.998	2718	2722	2727	rBV3	25084	34637	1.15%	0.148%
96	19.556	2812	2817	2823	rBV	359120	515128	17.13%	2.197%
97	21.080	3073	3076	3081	rVB3	70566	85397	2.84%	0.364%
98	21.392	3124	3129	3138	rBV	1924063	2791272	92.84%	11.905%
99	24.185	3598	3604	3617	rVB	176268	435525	14.49%	1.858%
100	24.391	3631	3639	3655	rVB	1181031	3006649	100.00%	12.824%


Sum of corrected areas: 23445361

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047857.D
Acq On : 05 Oct 2024 00:53
Operator : RC/JU
Sample : P4017-19MEDL 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCD5MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

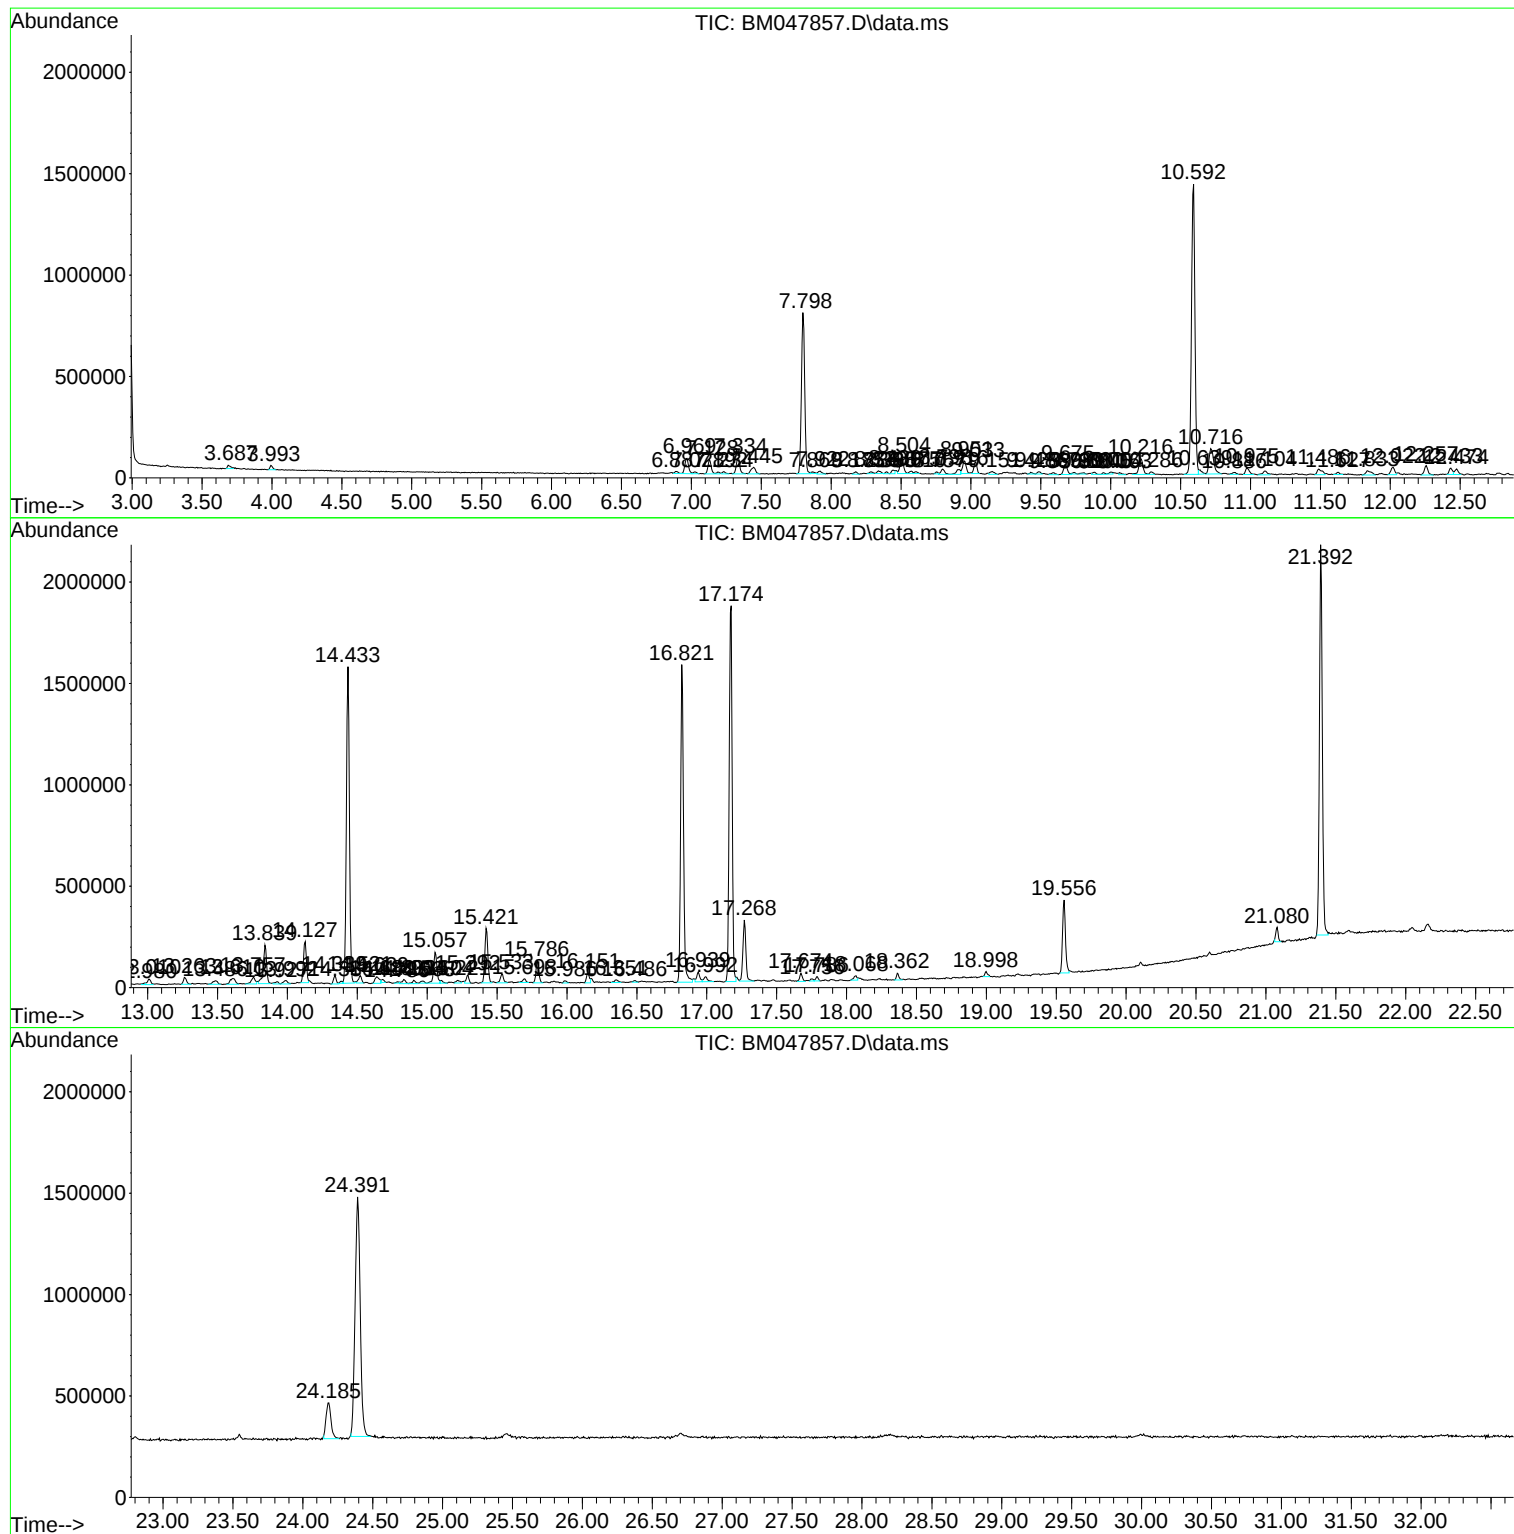

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047857.D
Acq On : 05 Oct 2024 00:53
Operator : RC/JU
Sample : P4017-19MEDL 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCD5MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047857.D
Acq On : 05 Oct 2024 00:53
Operator : RC/JU
Sample : P4017-19MEDL 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCD5MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------