

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047859.D
 Acq On : 05 Oct 2024 02:13
 Operator : RC/JU
 Sample : P4017-11MEDL 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDC86MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047859.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.681	115	118	125	rBV	50213	79763	1.12%	0.233%
2	3.999	168	172	180	rVB	23760	34258	0.48%	0.100%
3	6.963	669	676	683	rBV	111509	197602	2.77%	0.576%
4	7.022	684	686	692	rVB4	10791	17530	0.25%	0.051%
5	7.128	699	704	710	rBV	99417	159652	2.24%	0.466%
6	7.334	733	739	751	rVB	114139	199915	2.80%	0.583%
7	7.445	751	758	763	rBV4	17351	41929	0.59%	0.122%
8	7.728	803	806	810	rVV4	9038	15516	0.22%	0.045%
9	7.798	810	818	827	rVV	908968	1485856	20.85%	4.334%
10	7.875	827	831	836	rVV5	12856	25177	0.35%	0.073%
11	8.339	905	910	914	rVB4	11430	19085	0.27%	0.056%
12	8.392	917	919	923	rVB3	13885	16021	0.22%	0.047%
13	8.439	923	927	929	rBV3	10955	16601	0.23%	0.048%
14	8.504	933	938	945	rVB	123219	194859	2.73%	0.568%
15	8.569	945	949	952	rBV2	14478	16571	0.23%	0.048%
16	8.798	983	988	996	rVB5	21275	40945	0.57%	0.119%
17	8.910	997	1007	1009	rBV6	19067	40150	0.56%	0.117%
18	8.951	1009	1014	1020	rVV	96422	171882	2.41%	0.501%
19	9.034	1023	1028	1033	rVV2	38345	59327	0.83%	0.173%
20	9.151	1039	1048	1054	rBV2	14714	39788	0.56%	0.116%
21	9.263	1065	1067	1071	rVV4	11073	17423	0.24%	0.051%
22	9.586	1116	1122	1130	rVB5	16460	30720	0.43%	0.090%
23	9.675	1130	1137	1143	rBV2	71889	127673	1.79%	0.372%
24	9.734	1143	1147	1151	rVB7	10354	16225	0.23%	0.047%
25	9.798	1151	1158	1165	rBV7	8123	22184	0.31%	0.065%
26	10.004	1187	1193	1196	rBV5	7773	15862	0.22%	0.046%
27	10.216	1220	1229	1240	rVV	116452	225527	3.16%	0.658%
28	10.592	1282	1293	1304	rBV2	1705466	2975503	41.75%	8.679%
29	10.716	1307	1314	1327	rVB4	258106	545324	7.65%	1.591%
30	10.875	1334	1341	1351	rVB9	24821	61292	0.86%	0.179%
31	10.986	1355	1360	1368	rBV6	17875	31476	0.44%	0.092%
32	11.104	1373	1380	1392	rBV	136361	230391	3.23%	0.672%
33	11.486	1440	1445	1459	rVB7	35125	85950	1.21%	0.251%
34	11.628	1464	1469	1475	rVV7	13212	22662	0.32%	0.066%
35	11.716	1478	1484	1489	rBV3	15125	24556	0.34%	0.072%
36	11.839	1498	1505	1516	rVB7	23710	69540	0.98%	0.203%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047859.D
Acq On : 05 Oct 2024 02:13
Operator : RC/JU
Sample : P4017-11MEDL 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDC86MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37	11.939	1516	1522	1526	rBV	25163	35284	0.50%	0.103%
38	12.016	1529	1535	1546	rBV4	53386	100448	1.41%	0.293%
39	12.139	1551	1556	1563	rVB7	10158	17485	0.25%	0.051%
40	12.257	1569	1576	1582	rVB4	17070	31928	0.45%	0.093%
41	12.375	1589	1596	1599	rBV7	12659	23764	0.33%	0.069%
42	12.433	1599	1606	1611	rVV4	166828	311686	4.37%	0.909%
43	12.475	1611	1613	1620	rVB	31944	40359	0.57%	0.118%
44	12.686	1643	1649	1658	rVB	25078	49698	0.70%	0.145%
45	12.780	1658	1665	1669	rBV6	27626	48701	0.68%	0.142%
46	12.833	1670	1674	1679	rVB2	18392	28770	0.40%	0.084%
47	12.886	1679	1683	1687	rBV6	8645	15239	0.21%	0.044%
48	13.010	1692	1704	1709	rVV2	47551	95429	1.34%	0.278%
49	13.069	1709	1714	1719	rVB5	13881	22126	0.31%	0.065%
50	13.169	1725	1731	1737	rVB10	11002	18463	0.26%	0.054%
51	13.263	1743	1747	1753	rVV	59771	93886	1.32%	0.274%
52	13.322	1753	1757	1761	rVV4	16222	32651	0.46%	0.095%
53	13.398	1766	1770	1774	rVV	19636	30642	0.43%	0.089%
54	13.486	1778	1785	1792	rVB2	102325	172897	2.43%	0.504%
55	13.616	1798	1807	1812	rBV4	54637	123580	1.73%	0.360%
56	13.657	1812	1814	1821	rVB6	14409	20498	0.29%	0.060%
57	13.751	1821	1830	1834	rBV	40915	88885	1.25%	0.259%
58	13.792	1834	1837	1841	rVV4	23109	41574	0.58%	0.121%
59	13.839	1841	1845	1853	rVB	239926	340970	4.78%	0.995%
60	13.986	1868	1870	1874	rVB4	13386	16251	0.23%	0.047%
61	14.127	1886	1894	1898	rBV	269402	415646	5.83%	1.212%
62	14.239	1909	1913	1917	rVB4	13850	17407	0.24%	0.051%
63	14.339	1925	1930	1934	rBV	97983	133375	1.87%	0.389%
64	14.380	1934	1937	1940	rBV4	20577	28804	0.40%	0.084%
65	14.433	1940	1946	1954	rVV	1803693	2652710	37.22%	7.738%
66	14.633	1973	1980	1986	rBV6	40046	108560	1.52%	0.317%
67	14.686	1986	1989	1993	rVB2	30246	39339	0.55%	0.115%
68	14.833	2011	2014	2020	rVB2	22798	36743	0.52%	0.107%
69	14.904	2020	2026	2030	rBV5	20235	35417	0.50%	0.103%
70	14.968	2033	2037	2041	rVB6	22080	36861	0.52%	0.108%
71	15.057	2043	2052	2058	rBV	657534	930551	13.06%	2.714%
72	15.163	2064	2070	2076	rBV6	20341	44226	0.62%	0.129%
73	15.286	2088	2091	2096	rVB	49206	63462	0.89%	0.185%
74	15.421	2108	2114	2120	rVV	367956	530566	7.44%	1.548%
75	15.533	2126	2133	2142	rBV3	73154	133363	1.87%	0.389%
76	15.698	2155	2161	2169	rVB5	33617	63795	0.90%	0.186%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047859.D
 Acq On : 05 Oct 2024 02:13
 Operator : RC/JU
 Sample : P4017-11MEDL 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDC86MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

77	15.792	2171	2177	2183	rVB	44584	70521	0.99%	0.206%
78	15.992	2206	2211	2215	rBV7	9869	17215	0.24%	0.050%
79	16.151	2233	2238	2241	rBV	53339	79454	1.11%	0.232%
80	16.239	2249	2253	2258	rBV7	9944	18153	0.25%	0.053%
81	16.821	2346	2352	2366	rBV	5028137	7127654	100.00%	20.790%
82	16.939	2368	2372	2376	rVV	65710	105267	1.48%	0.307%
83	16.992	2378	2381	2387	rVB3	32374	51050	0.72%	0.149%
84	17.174	2405	2412	2417	rBV	2175443	3132104	43.94%	9.136%
85	17.268	2422	2428	2437	rVB	395087	570918	8.01%	1.665%
86	17.474	2459	2463	2468	rBV8	12725	17372	0.24%	0.051%
87	17.674	2493	2497	2503	rVB	47549	56979	0.80%	0.166%
88	17.745	2507	2509	2513	rVV3	15688	21775	0.31%	0.064%
89	17.786	2513	2516	2522	rVB3	27319	36289	0.51%	0.106%
90	17.892	2531	2534	2540	rVB4	10702	17618	0.25%	0.051%
91	18.062	2557	2563	2567	rBV6	29893	56329	0.79%	0.164%
92	18.233	2588	2592	2597	rBV8	9011	15919	0.22%	0.046%
93	18.362	2611	2614	2621	rBV	35866	49433	0.69%	0.144%
94	18.998	2719	2722	2728	rVB2	31900	44541	0.62%	0.130%
95	19.227	2757	2761	2763	rBV3	15380	19769	0.28%	0.058%
96	19.492	2802	2806	2810	rVB3	32777	43799	0.61%	0.128%
97	19.556	2812	2817	2824	rBV	461239	683915	9.60%	1.995%
98	21.392	3123	3129	3140	rBV	2246809	3390615	47.57%	9.890%
99	24.180	3598	3603	3615	rVB	228142	550327	7.72%	1.605%
100	24.391	3630	3639	3654	rBV	1407008	3659684	51.34%	10.675%




Sum of corrected areas: 34283474

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047859.D
Acq On : 05 Oct 2024 02:13
Operator : RC/JU
Sample : P4017-11MEDL 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDC86MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

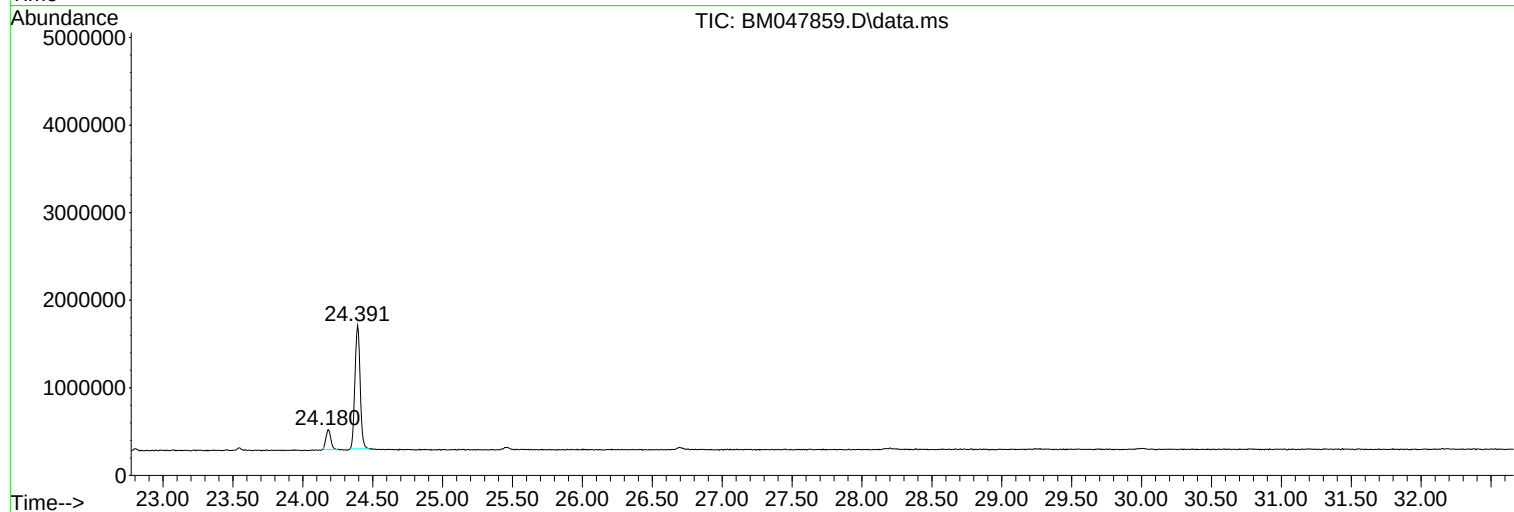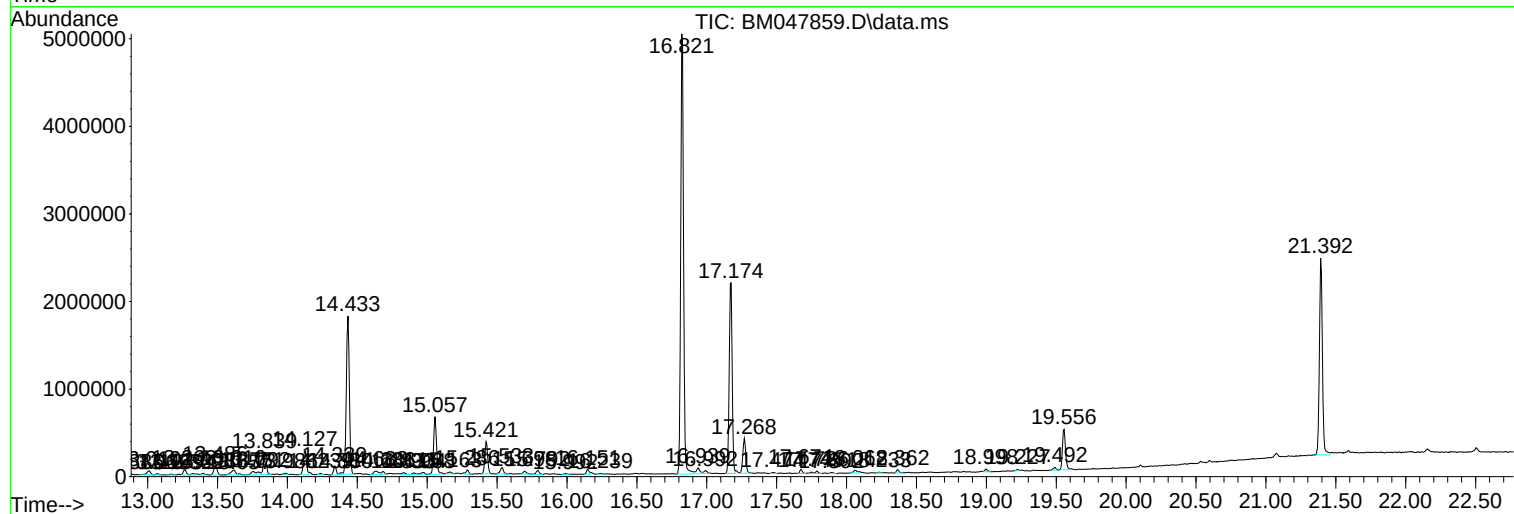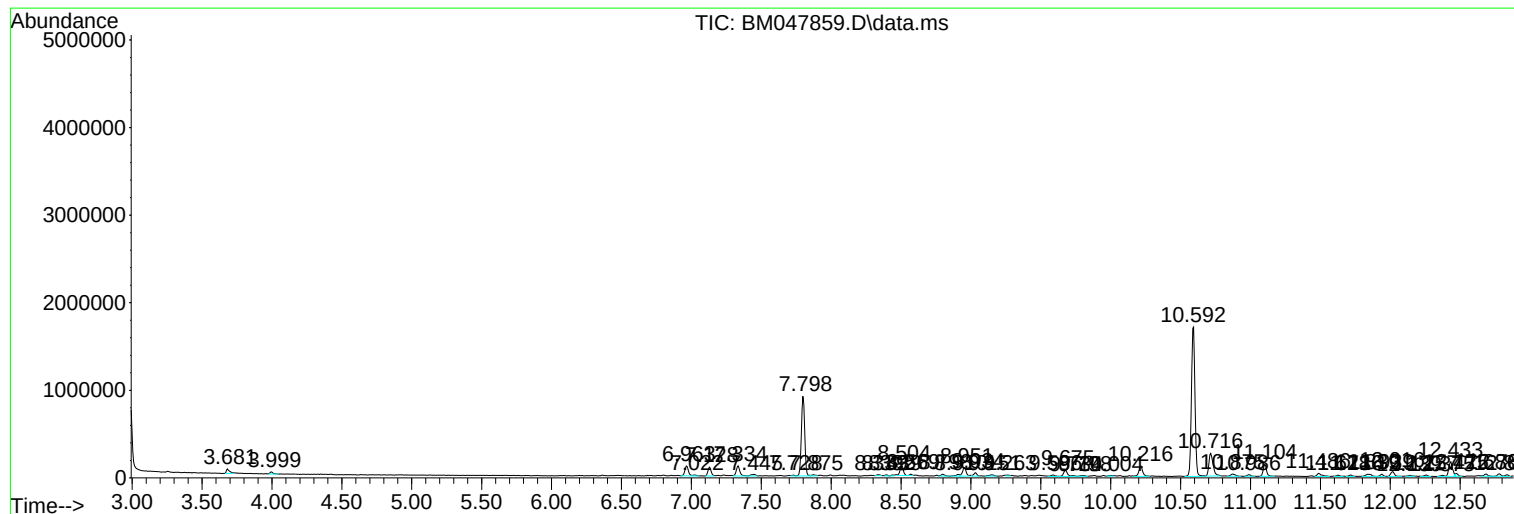

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047859.D
Acq On : 05 Oct 2024 02:13
Operator : RC/JU
Sample : P4017-11MEDL 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDC86MEDL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.433	2.10 ng/ul	311686	Naphthalene-d8	10.592

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Methyl-4-decanone	170	C11H22O	006628-25-7	38	
2	5-Undecanone	170	C11H22O	033083-83-9	38	
3	5-Nonanone	142	C9H18O	000502-56-7	35	
4	5-Nonanone	142	C9H18O	000502-56-7	35	
5	Hexane, 2,4-dimethyl-	114	C8H18	000589-43-5	18	

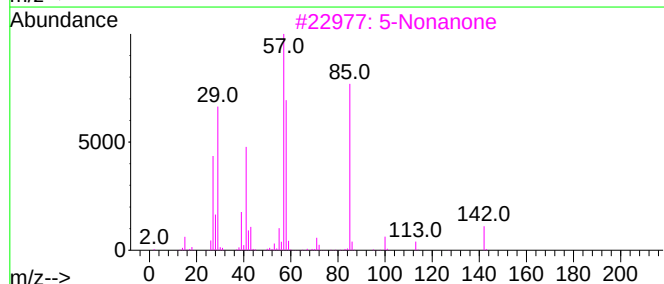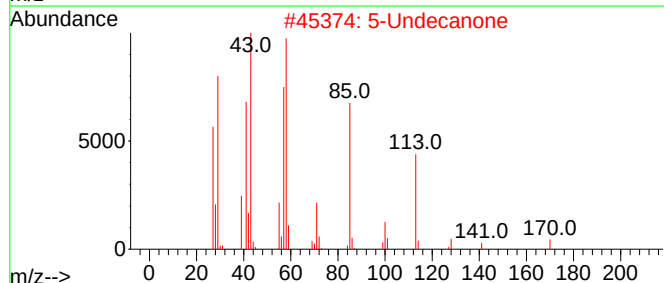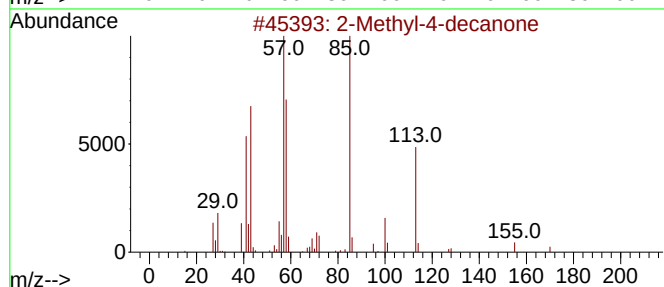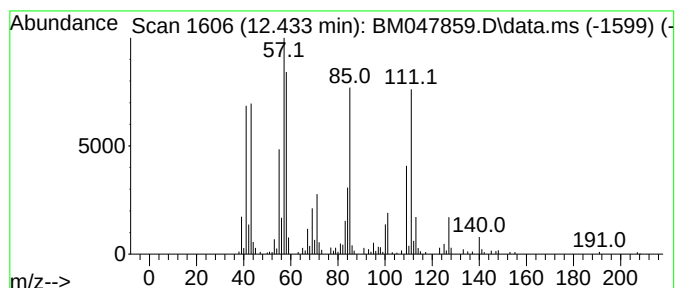

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047859.D
Acq On : 05 Oct 2024 02:13
Operator : RC/JU
Sample : P4017-11MEDL 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDC86MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	12.433	2.1	ng/ul	311686	2	10.592	2975500	20.0