

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047864.D
 Acq On : 05 Oct 2024 06:12
 Operator : RC/JU
 Sample : PB163918BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK918

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	41	45	52	rVB	70060	90449	2.31%	0.204%
2	3.663	111	115	134	rBV	840800	1293074	33.01%	2.916%
3	3.993	169	171	175	rVB4	11493	13129	0.34%	0.030%
4	5.622	446	448	452	rVB4	5413	6176	0.16%	0.014%
5	6.963	669	676	689	rBV	859245	1344339	34.32%	3.032%
6	7.128	697	704	715	rBV	705420	1098747	28.05%	2.478%
7	7.334	732	739	749	rBV	858816	1380455	35.24%	3.113%
8	7.798	811	818	827	rBV	654432	1039252	26.53%	2.344%
9	8.504	931	938	952	rBV	987855	1617665	41.30%	3.649%
10	8.951	1006	1014	1029	rBV	775091	1290032	32.94%	2.910%
11	9.675	1129	1137	1145	rBV	582995	966094	24.67%	2.179%
12	10.210	1221	1228	1241	rBV	942458	1583824	40.44%	3.572%
13	10.592	1285	1293	1301	rBV	844285	1432684	36.58%	3.231%
14	10.722	1308	1315	1337	rBV	938653	1667452	42.57%	3.761%
15	11.739	1484	1488	1491	rBV6	2733	4394	0.11%	0.010%
16	12.192	1558	1565	1572	rBV4	9818	20466	0.52%	0.046%
17	13.839	1839	1845	1855	rBV	1598658	2181020	55.68%	4.919%
18	14.127	1887	1894	1903	rBV	1840622	2733084	69.78%	6.164%
19	14.433	1939	1946	1957	rBV	1234807	1803505	46.05%	4.068%
20	14.621	1972	1978	1995	rBV	609209	976430	24.93%	2.202%
21	15.421	2107	2114	2123	rBV	2339503	3281695	83.79%	7.402%
22	15.533	2127	2133	2141	rBV	532122	755254	19.28%	1.703%
23	15.662	2151	2155	2161	rVB6	11577	17392	0.44%	0.039%
24	16.057	2218	2222	2223	rVB3	4888	4300	0.11%	0.010%
25	16.098	2223	2229	2230	rBV6	3281	5274	0.13%	0.012%
26	16.198	2243	2246	2251	rBV6	3211	5470	0.14%	0.012%
27	17.168	2403	2411	2418	rBV	1453450	2014614	51.44%	4.544%
28	17.268	2422	2428	2440	rVV	2475321	3443323	87.91%	7.766%
29	18.004	2548	2553	2555	rVB6	3608	4142	0.11%	0.009%
30	18.074	2561	2565	2568	rVB5	5047	3943	0.10%	0.009%
31	19.121	2740	2743	2748	rVB5	25970	36998	0.94%	0.083%
32	19.192	2752	2755	2760	rVB2	23506	29831	0.76%	0.067%
33	19.556	2811	2817	2829	rBV	3064030	3916766	100.00%	8.834%
34	21.392	3124	3129	3136	rBV	1413370	2073100	52.93%	4.676%
35	24.185	3596	3604	3619	rVB	1580634	3762865	96.07%	8.487%
36	24.385	3631	3638	3652	rVB	901956	2440527	62.31%	5.504%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047864.D
Acq On : 05 Oct 2024 06:12
Operator : RC/JU
Sample : PB163918BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK918

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 44337765

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047864.D
Acq On : 05 Oct 2024 06:12
Operator : RC/JU
Sample : PB163918BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK918

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

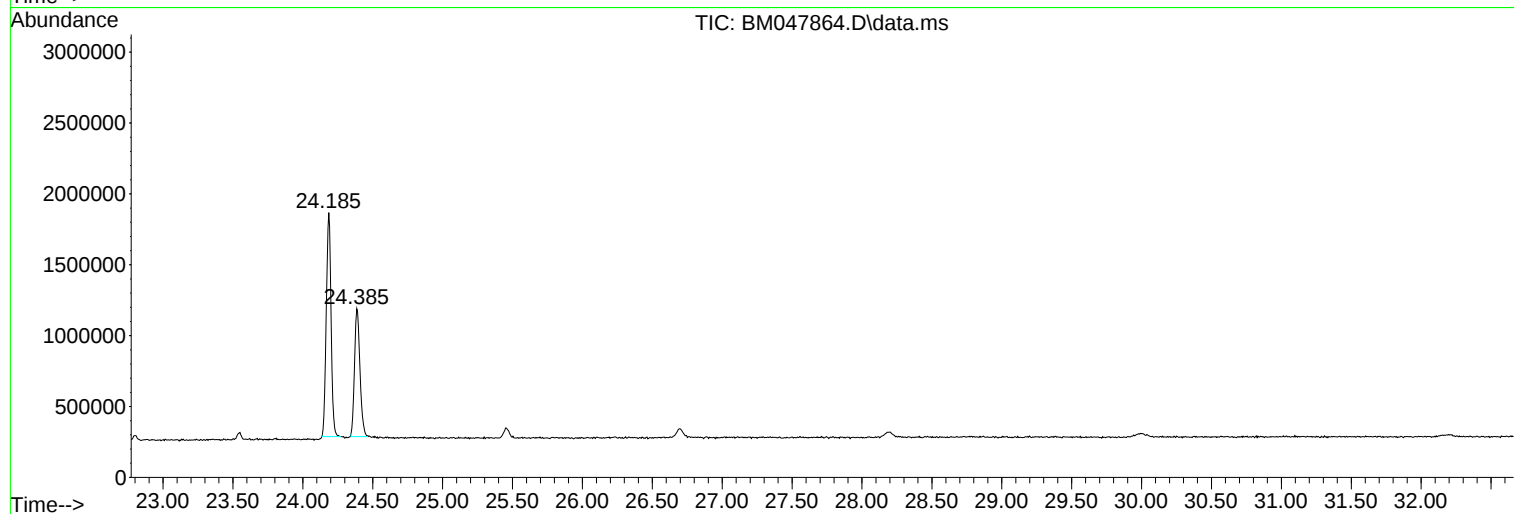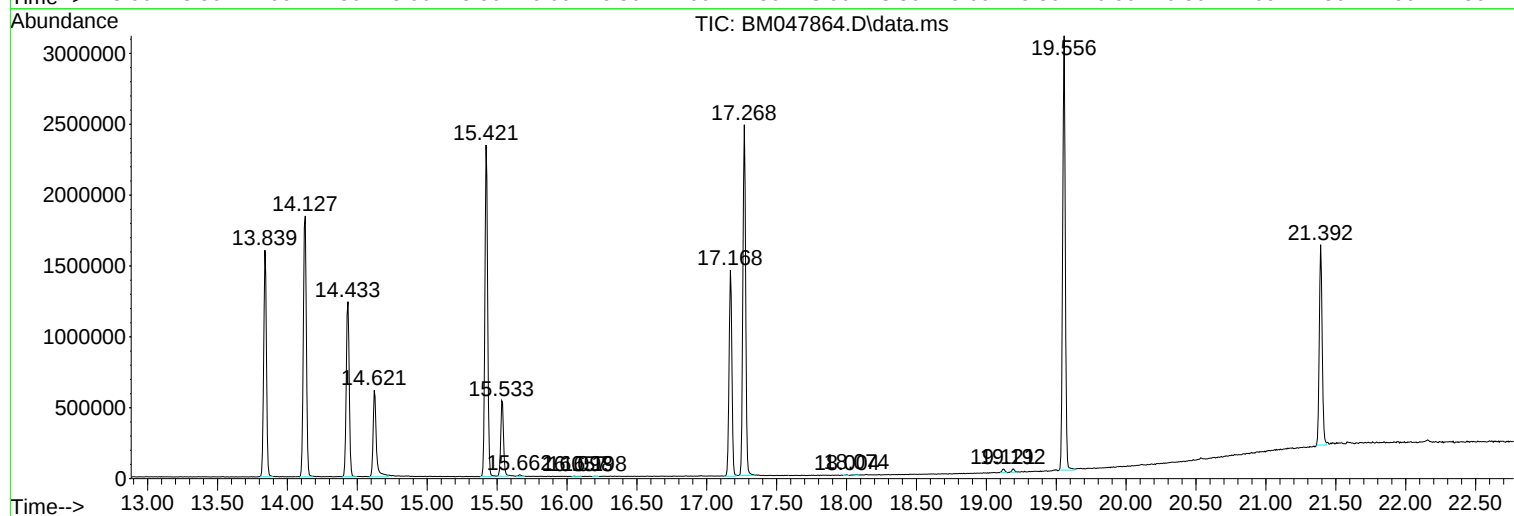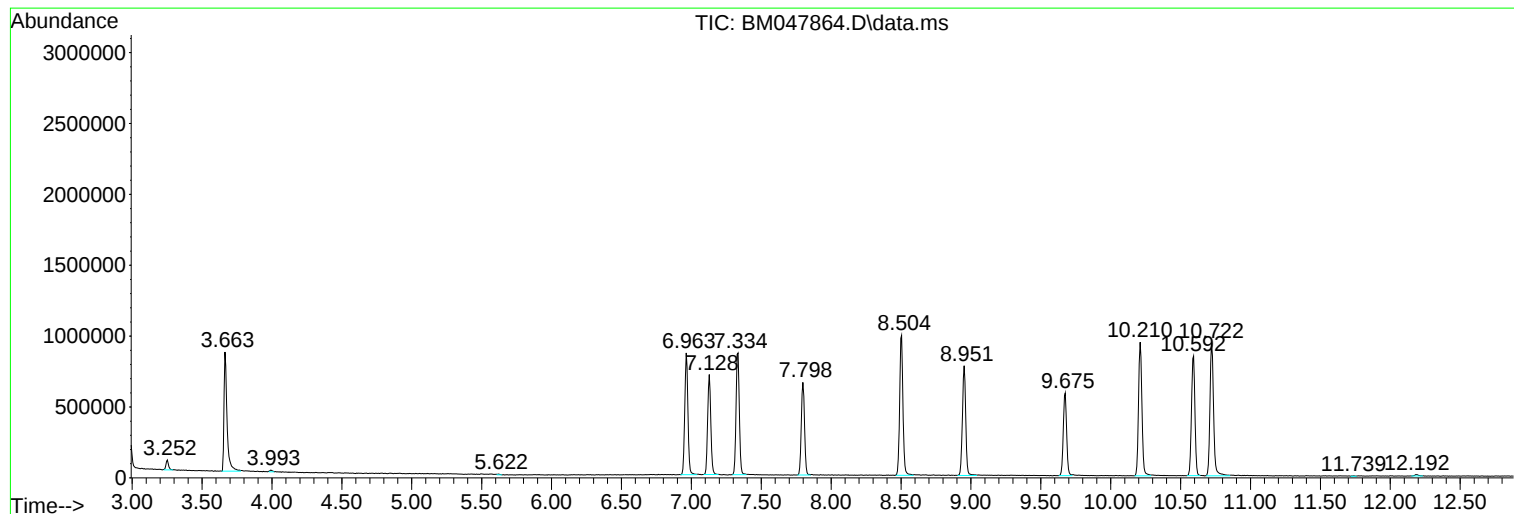

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047864.D
Acq On : 05 Oct 2024 06:12
Operator : RC/JU
Sample : PB163918BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK918

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047864.D
Acq On : 05 Oct 2024 06:12
Operator : RC/JU
Sample : PB163918BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK918

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc