

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
 Data File : BM047867.D
 Acq On : 05 Oct 2024 08:10
 Operator : RC/JU
 Sample : P4020-05MEDL 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCF9MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.675	114	117	130	rBV	76073	133080	3.49%	0.646%
2	3.993	168	171	178	rVB2	25005	33602	0.88%	0.163%
3	6.057	520	522	526	rBV3	4878	4761	0.12%	0.023%
4	6.963	670	676	683	rBV	88501	147435	3.87%	0.716%
5	7.128	698	704	711	rBV	77974	129661	3.40%	0.630%
6	7.334	732	739	747	rBV	93575	156540	4.10%	0.760%
7	7.798	811	818	826	rBV	722215	1150500	30.16%	5.588%
8	8.504	932	938	945	rBV	100209	174803	4.58%	0.849%
9	8.951	1005	1014	1024	rBV	79446	147161	3.86%	0.715%
10	9.675	1131	1137	1145	rBV3	49122	91264	2.39%	0.443%
11	9.957	1183	1185	1191	rVB5	3342	5412	0.14%	0.026%
12	10.210	1222	1228	1237	rBV2	85827	169616	4.45%	0.824%
13	10.592	1285	1293	1303	rBV	932364	1596012	41.84%	7.752%
14	10.728	1308	1316	1329	rBV2	85585	186138	4.88%	0.904%
15	13.839	1839	1845	1854	rBV	200000	300419	7.88%	1.459%
16	14.121	1885	1893	1903	rBV2	222164	348631	9.14%	1.693%
17	14.433	1939	1946	1956	rBV	1347096	2029362	53.21%	9.857%
18	14.633	1973	1980	1988	rBV3	23712	56765	1.49%	0.276%
19	15.057	2048	2052	2058	rBV5	21756	36779	0.96%	0.179%
20	15.421	2108	2114	2122	rBV	297425	436310	11.44%	2.119%
21	15.533	2127	2133	2140	rBV2	41716	64651	1.70%	0.314%
22	15.786	2169	2176	2181	rBV	30780	44511	1.17%	0.216%
23	16.821	2346	2352	2367	rBV	2793923	3814134	100.00%	18.526%
24	17.168	2405	2411	2421	rBV	1757059	2380689	62.42%	11.563%
25	17.268	2422	2428	2438	rVB	322191	474589	12.44%	2.305%
26	17.786	2511	2516	2524	rBV5	27858	41548	1.09%	0.202%
27	18.062	2558	2563	2567	rBV5	21768	34662	0.91%	0.168%
28	19.192	2753	2755	2758	rBV4	8181	8576	0.22%	0.042%
29	19.550	2811	2816	2824	rBV	385366	553177	14.50%	2.687%
30	21.392	3124	3129	3140	rBV	1753269	2498647	65.51%	12.136%
31	24.180	3598	3603	3615	rVB	203741	489409	12.83%	2.377%
32	24.391	3630	3639	3653	rVB	1070748	2849505	74.71%	13.840%




Sum of corrected areas: 20588349

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047867.D
Acq On : 05 Oct 2024 08:10
Operator : RC/JU
Sample : P4020-05MEDL 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCF9MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

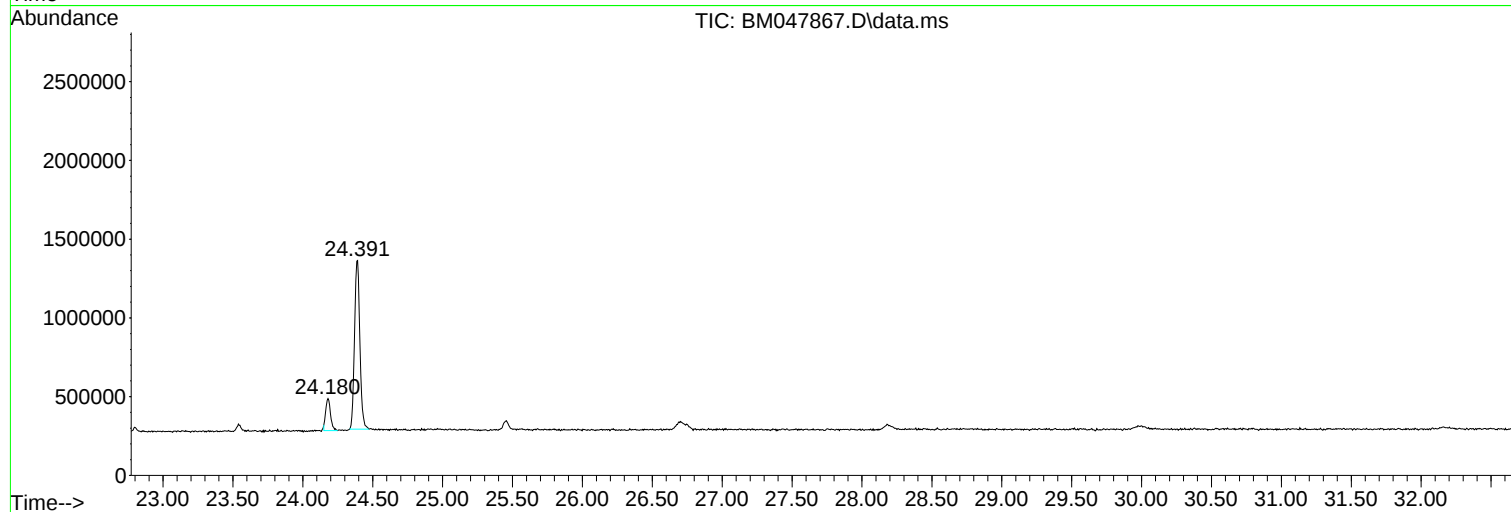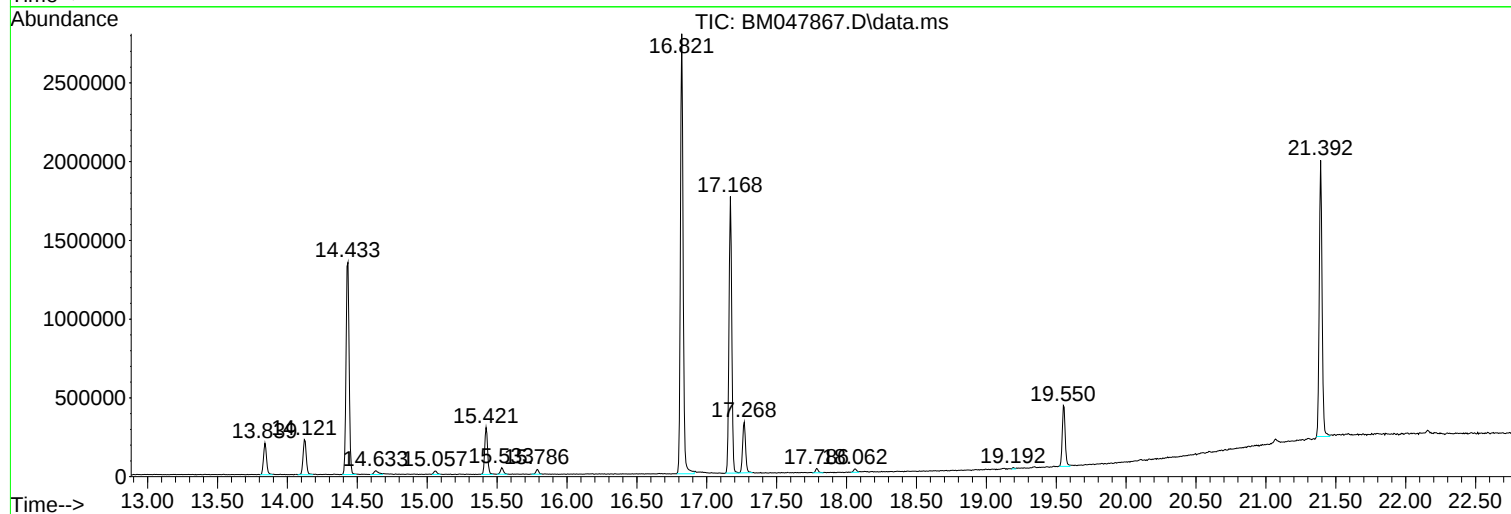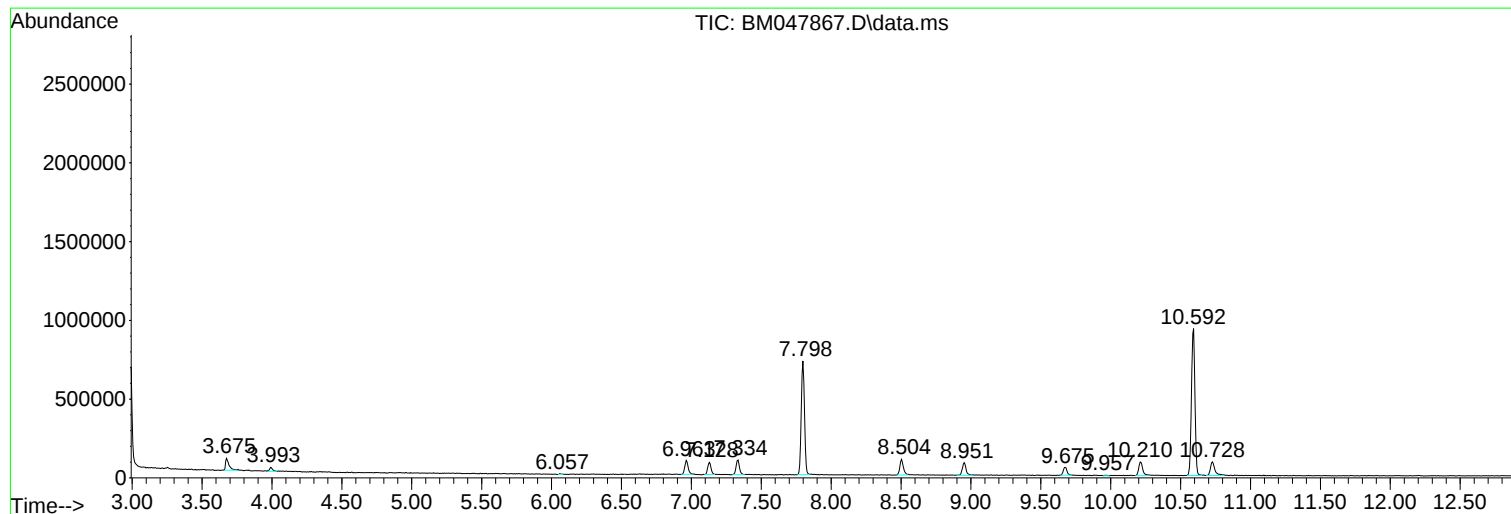

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047867.D
Acq On : 05 Oct 2024 08:10
Operator : RC/JU
Sample : P4020-05MEDL 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCF9MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100324\
Data File : BM047867.D
Acq On : 05 Oct 2024 08:10
Operator : RC/JU
Sample : P4020-05MEDL 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCF9MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------