

Data Path : Z:\HPCHEM1\BNA_M\Data\BM100416\
 Data File : BM007651.D
 Acq On : 04 Oct 2016 12:09
 Operator : UM/SJ
 Sample : PB93759BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK59

Quant Time: Oct 04 13:08:57 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 04 13:03:57 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	137282	20.00	ng/ul	0.00
18) Naphthalene-d8	10.55	136	656460	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	536354	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	1249848	20.00	ng/ul	0.00
75) Chrysene-d12	21.33	240	1515898	20.00	ng/ul	0.00
83) Perylene-d12	23.59	264	1319926	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	20434	7.32	ng/uL	0.00
5) Phenol-d5	6.95	99	383285	31.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.11	67	239425	36.55	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	299155	33.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	332060	31.92	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	162648	34.66	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	177824	33.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	340816	32.08	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	389498	34.92	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	1372972	35.19	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	1597530	35.29	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	172446	25.04	ng/ul	0.00
57) Fluorene-d10	15.40	176	1230700	35.97	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	199100	26.11	ng/ul	0.00
70) Anthracene-d10	17.24	188	2101732	36.59	ng/ul	0.00
76) Pyrene-d10	19.54	212	2559407	42.55	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.44	264	2095952	35.89	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.47	70	9224	1.15 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM100416\
Data File : BM007651.D
Acq On : 04 Oct 2016 12:09
Operator : UM/SJ
Sample : PB93759BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK59

Quant Time: Oct 04 13:08:57 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 04 13:03:57 2016
Response via : Initial Calibration

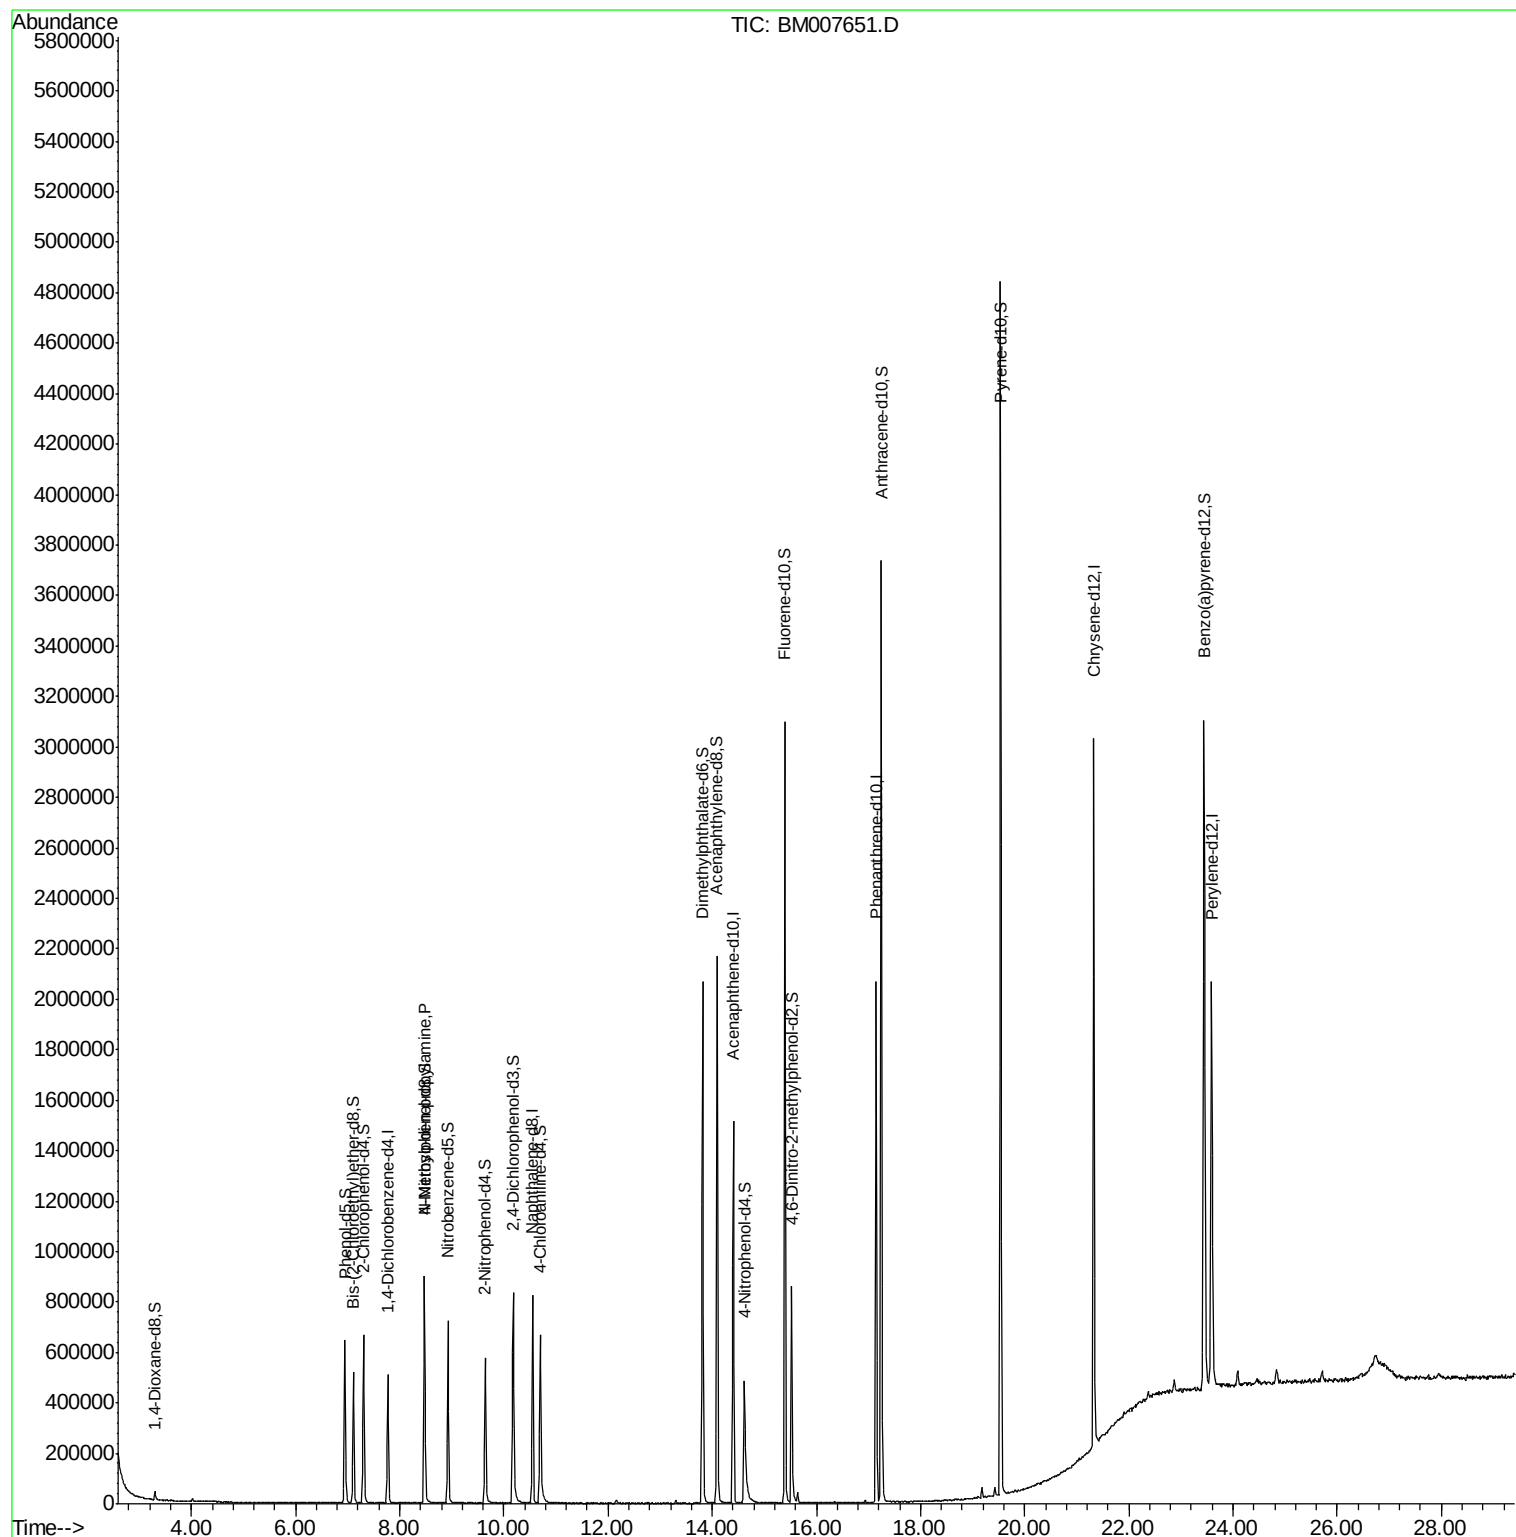

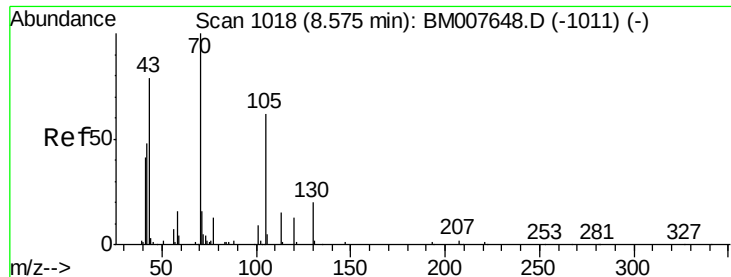

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.15 ng/ul
 RT: 8.47 min Scan# 1001
 Delta R.T. -0.10 min
 Lab File: BM007651.D
 Acq: 04 Oct 2016 12:09

Instrument :
 BNA_M
 ClientSampleId :
 SBLK59

Tgt Ion: 70 Resp: 9224
 Ion Ratio Lower Upper
 70 100
 42 323.4 43.4 65.2#
 101 0.0 7.8 11.6#
 130 0.0 16.2 24.4#

