

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100417\
 Data File : BM011910.D
 Acq On : 05 Oct 2017 03:07
 Operator : SJ/JU
 Sample : I5406-11
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B0BC4

Quant Time: Oct 05 07:18:38 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 05 07:08:17 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	320796	20.00	ng/ul	0.00
18) Naphthalene-d8	10.68	136	1453126	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.52	164	915276	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.26	188	2146595	20.00	ng/ul	0.00
75) Chrysene-d12	21.43	240	1979556	20.00	ng/ul	0.00
83) Perylene-d12	23.76	264	1691693	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.29	96	21280	3.14	ng/uL	0.00
5) Phenol-d5	7.03	99	443301	16.06	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.20	67	287359	17.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.40	132	399130	18.03	ng/ul	0.00
13) 4-Methylphenol-d8	8.57	113	312786	13.11	ng/ul	0.00
19) Nitrobenzene-d5	9.04	128	201724	19.49	ng/ul	0.00
22) 2-Nitrophenol-d4	9.76	143	224290	19.24	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.30	165	420081	17.83	ng/ul	0.00
29) 4-Chloroaniline-d4	10.82	131	456209	17.75	ng/ul	0.00
43) Dimethylphthalate-d6	13.92	166	1475720	18.60	ng/ul	0.00
46) Acenaphthylene-d8	14.21	160	1731606	18.58	ng/ul	0.00
51) 4-Nitrophenol-d4	14.72	143	167537	12.09	ng/ul	0.00
57) Fluorene-d10	15.51	176	1281102	18.30	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.63	200	157276	10.89	ng/ul	0.00
70) Anthracene-d10	17.36	188	1966364	18.59	ng/ul	0.00
76) Pyrene-d10	19.65	212	2187061	24.49	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.61	264	1464579	18.00	ng/ul	0.00
Target Compounds						
44) Dimethylphthalate	13.97	163	365388	4.788	ng/ul	0.00


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100417\
Data File : BM011910.D
Acq On : 05 Oct 2017 03:07
Operator : SJ/JU
Sample : I5406-11
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B0BC4

Quant Time: Oct 05 07:18:38 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 05 07:08:17 2017
Response via : Initial Calibration

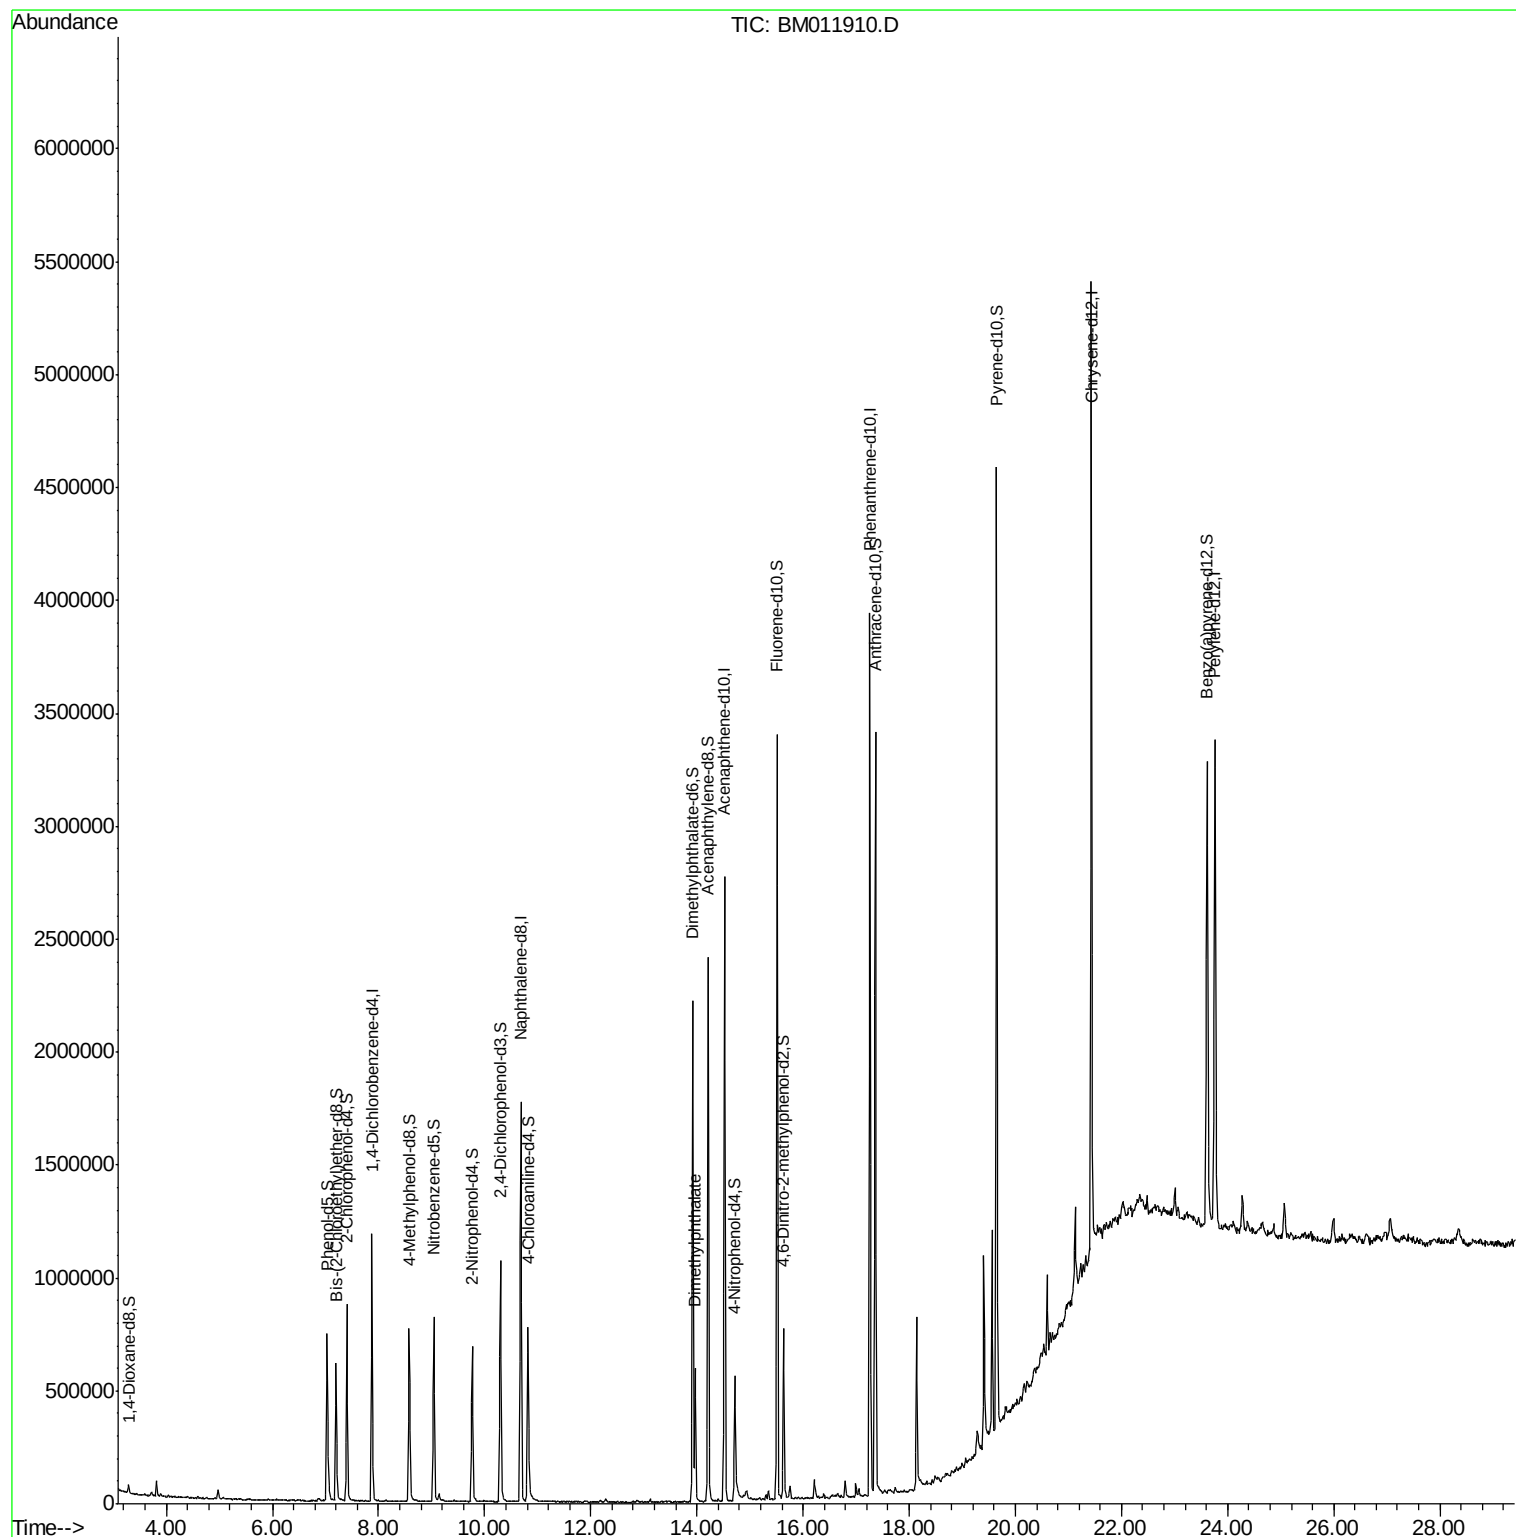

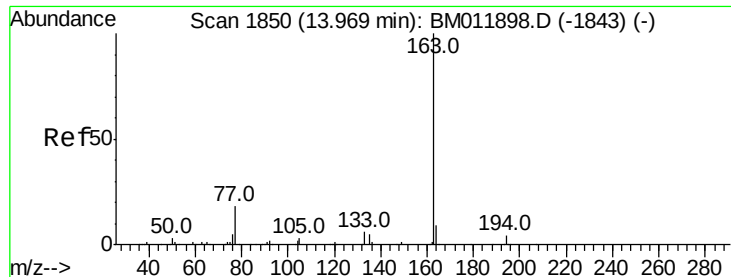

#44

Dimethylphthalate

Concen: 4.788 ng/ul

RT: 13.97 min Scan# 1850

Delta R.T. -0.00 min

Lab File: BM011910.D

Acq: 05 Oct 2017 03:07

Instrument :

BNA_M

ClientSampleId :

B0BC4


Tot Ion:163 Resp: 365388

Ion Ratio Lower Upper

163 100

194 3.7 3.5 5.3

164 8.9 8.2 12.4

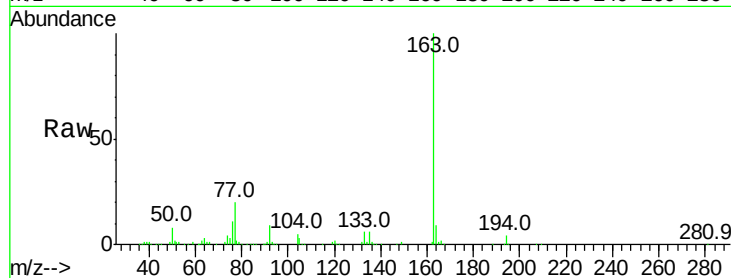

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

