

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100417\
 Data File : BM011912.D
 Acq On : 05 Oct 2017 04:20
 Operator : SJ/JU
 Sample : I5406-14
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B0BD1

Quant Time: Oct 05 07:18:57 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 05 07:08:17 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	439841	20.00	ng/ul	0.00
18) Naphthalene-d8	10.68	136	1980446	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.52	164	1225646	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.26	188	2706333	20.00	ng/ul	0.00
75) Chrysene-d12	21.43	240	2093131	20.00	ng/ul	0.00
83) Perylene-d12	23.76	264	1886039	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.29	96	31056	3.34	ng/uL	0.00
5) Phenol-d5	7.03	99	746437	19.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.20	67	463899	20.71	ng/ul	0.00
9) 2-Chlorophenol-d4	7.40	132	656310	21.62	ng/ul	0.00
13) 4-Methylphenol-d8	8.57	113	564203	17.25	ng/ul	0.00
19) Nitrobenzene-d5	9.04	128	328410	23.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.76	143	377815	23.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.30	165	694518	21.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.82	131	736328	21.02	ng/ul	0.00
43) Dimethylphthalate-d6	13.92	166	2320361	21.84	ng/ul	0.00
46) Acenaphthylene-d8	14.21	160	2741982	21.97	ng/ul	0.00
51) 4-Nitrophenol-d4	14.71	143	289174	15.58	ng/ul	0.00
57) Fluorene-d10	15.51	176	1982317	21.14	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.63	200	217585	11.95	ng/ul	0.00
70) Anthracene-d10	17.36	188	2948259	22.11	ng/ul	0.00
76) Pyrene-d10	19.65	212	2974837	31.51	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.61	264	1901522	20.96	ng/ul	0.01
Target Compounds						
6) Phenol	7.06	94	46795	1.250	ng/ul#	86
44) Dimethylphthalate	13.97	163	599508	5.866	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100417\
Data File : BM011912.D
Acq On : 05 Oct 2017 04:20
Operator : SJ/JU
Sample : I5406-14
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B0BD1

Quant Time: Oct 05 07:18:57 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 05 07:08:17 2017
Response via : Initial Calibration

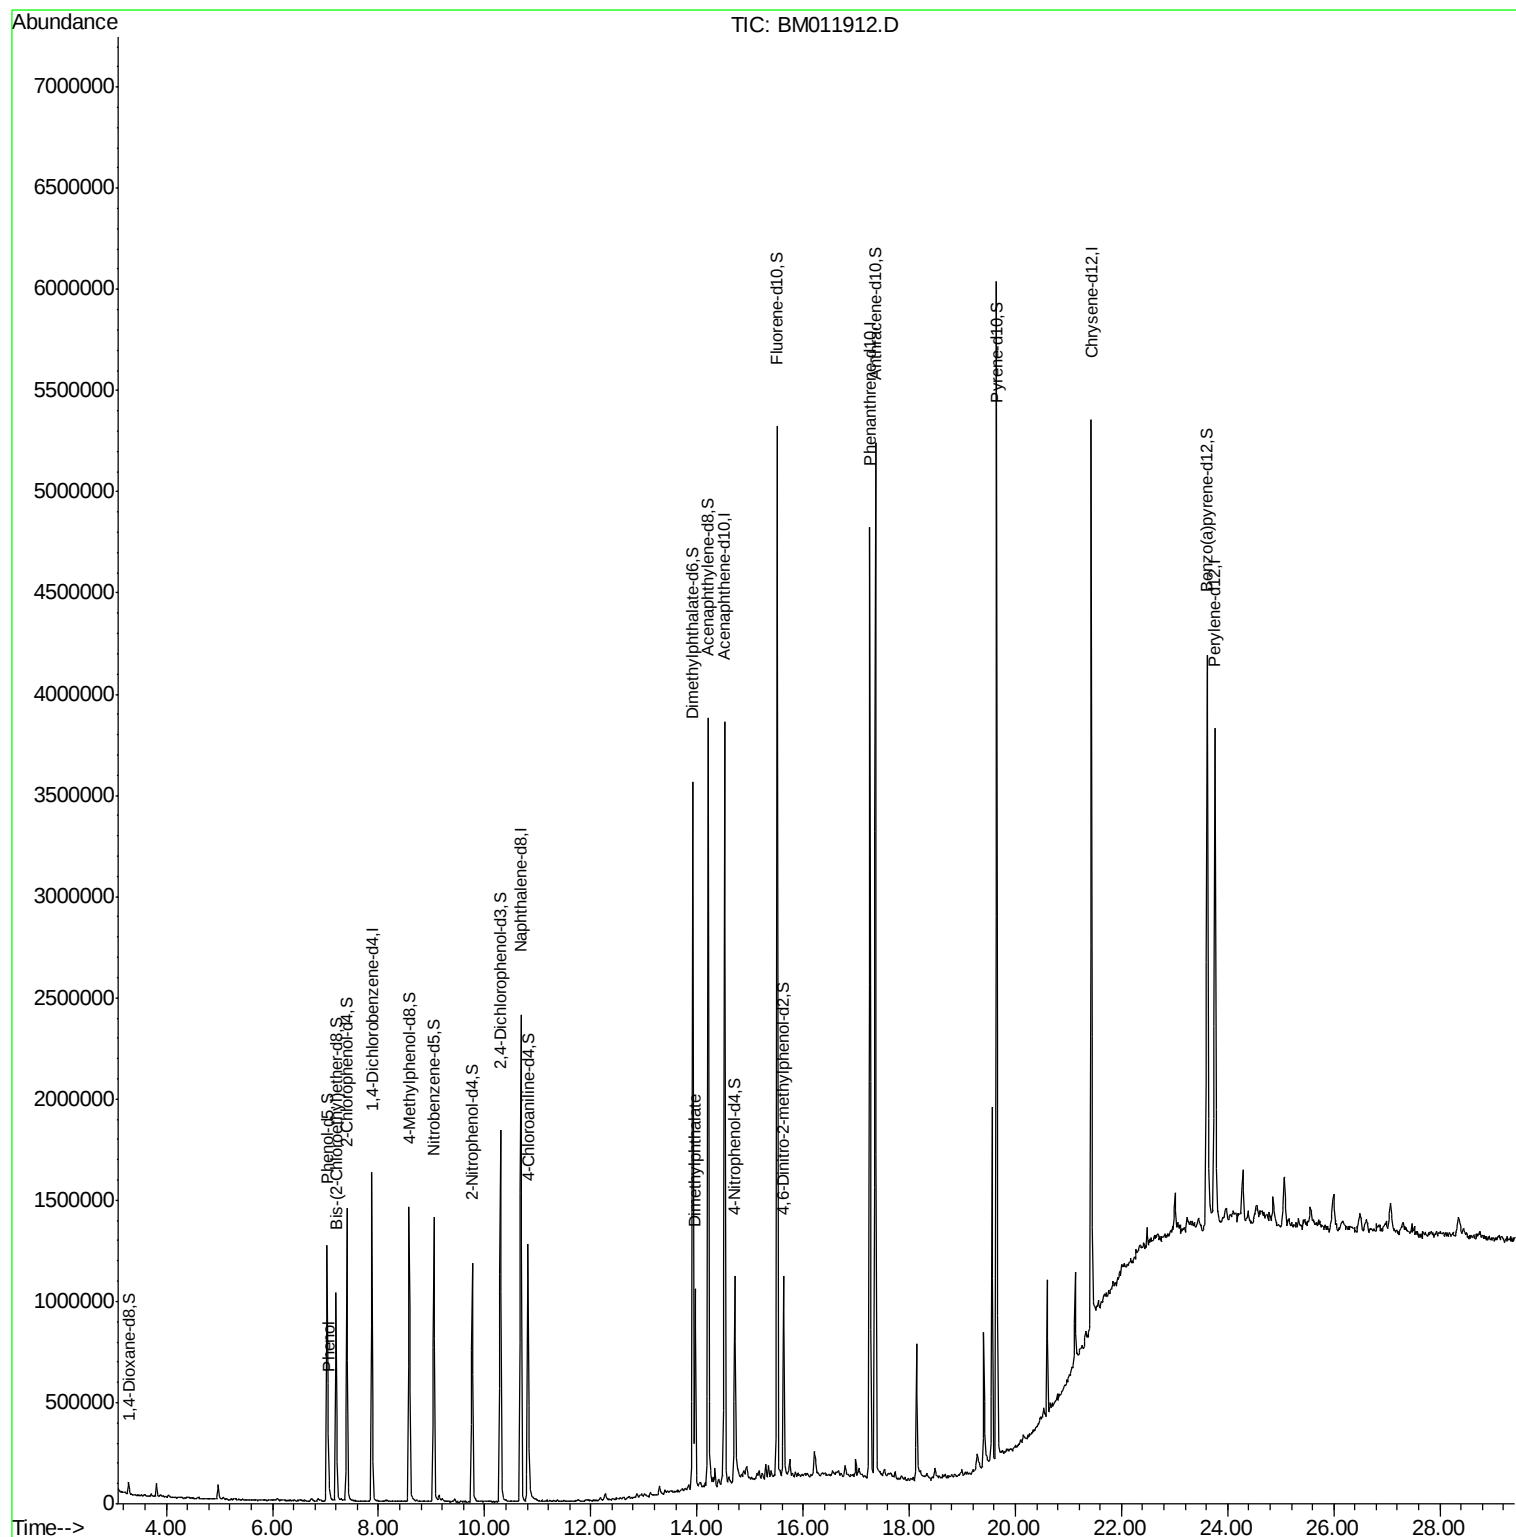

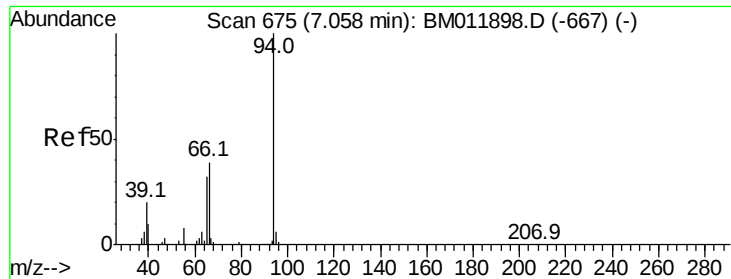

#6

Phenol

Concen: 1.250 ng/ul

RT: 7.06 min Scan# 675

Delta R.T. -0.00 min

Lab File: BM011912.D

Acq: 05 Oct 2017 04:20

Instrument :

BNA_M

ClientSampleId :

B0BD1


Tot Ion: 94 Resp: 46795

Ion Ratio Lower Upper

94 100

65 30.1 28.2 42.4




66 46.7 47.2 70.8#

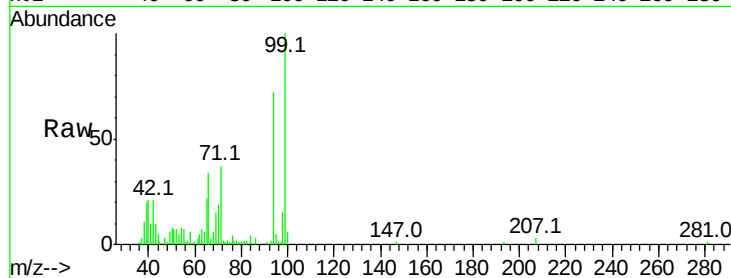

Abundance Ion 94.00 (93.70 to 94.70): BM011898.D (-667) (-)

Ion 65.00 (64.70 to 65.70): BM011898.D (-667) (-)

Ion 66.00 (65.70 to 66.70): BM011898.D (-667) (-)

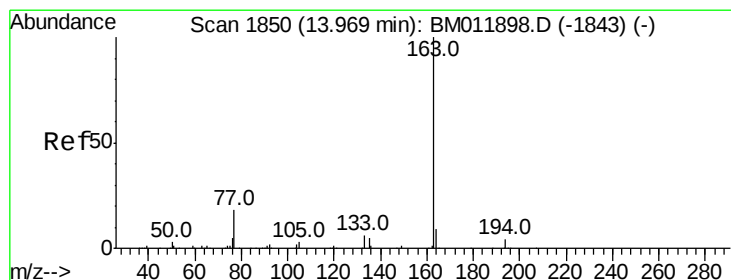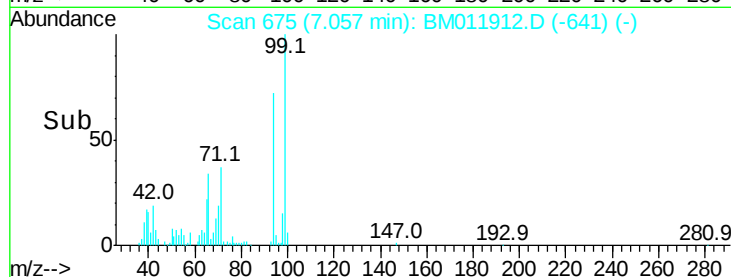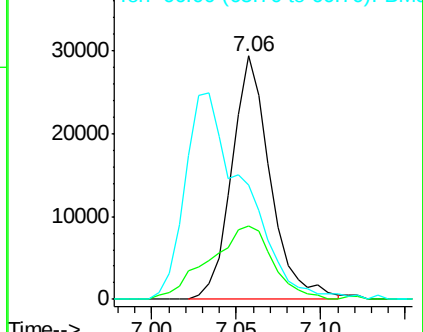

#44

Dimethylphthalate

Concen: 5.866 ng/ul

RT: 13.97 min Scan# 1850

Delta R.T. -0.00 min

Lab File: BM011912.D

Acq: 05 Oct 2017 04:20


Tgt Ion:163 Resp: 599508

Ion Ratio Lower Upper

163 100

194 4.2 3.5 5.3

164 10.4 8.2 12.4

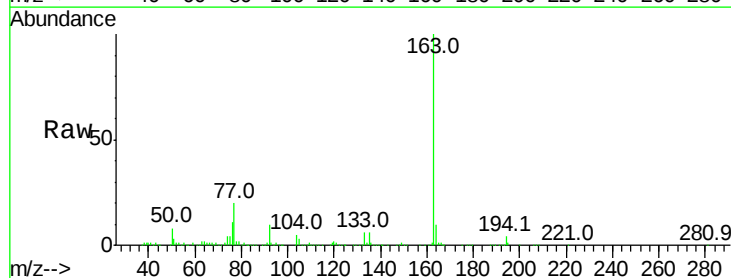

Abundance Ion 163.00 (162.70 to 163.70): BM011898.D (-1843) (-)

Ion 194.00 (193.70 to 194.70): BM011898.D (-1843) (-)

Ion 164.00 (163.70 to 164.70): BM011898.D (-1843) (-)

