

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
 Data File : BM017004.D
 Acq On : 04 Oct 2018 17:48
 Operator : MJ/SJ
 Sample : J5157-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA0

Quant Time: Oct 04 18:25:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 04 15:26:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	198505	20.00	ng/ul	0.00
18) Naphthalene-d8	10.47	136	838750	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.34	164	456975	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.09	188	1033402	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	1139210	20.00	ng/ul	0.00
86) Perylene-d12	23.50	264	1204867	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	13067	3.27	ng/uL	0.00
5) Phenol-d5	6.87	99	313912	18.92	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.04	67	205806	20.45	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	260956	18.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	282998	21.77	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	136363	22.25	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	144029	23.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	281771	21.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	450454	29.22	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	1271535	35.07	ng/ul	0.00
47) Acenaphthylene-d8	14.03	160	1426881	30.79	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	199895	29.18	ng/ul	0.00
58) Fluorene-d10	15.33	176	1105492	34.23	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.46	200	154243	25.31	ng/ul	0.00
71) Anthracene-d10	17.19	188	1882086	38.13	ng/ul	0.00
79) Pyrene-d10	19.48	212	2309751	44.94	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.36	264	2825024	45.80	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.80	163	577244	16.079	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
Data File : BM017004.D
Acq On : 04 Oct 2018 17:48
Operator : MJ/SJ
Sample : J5157-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA0

Quant Time: Oct 04 18:25:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 04 15:26:45 2018
Response via : Initial Calibration

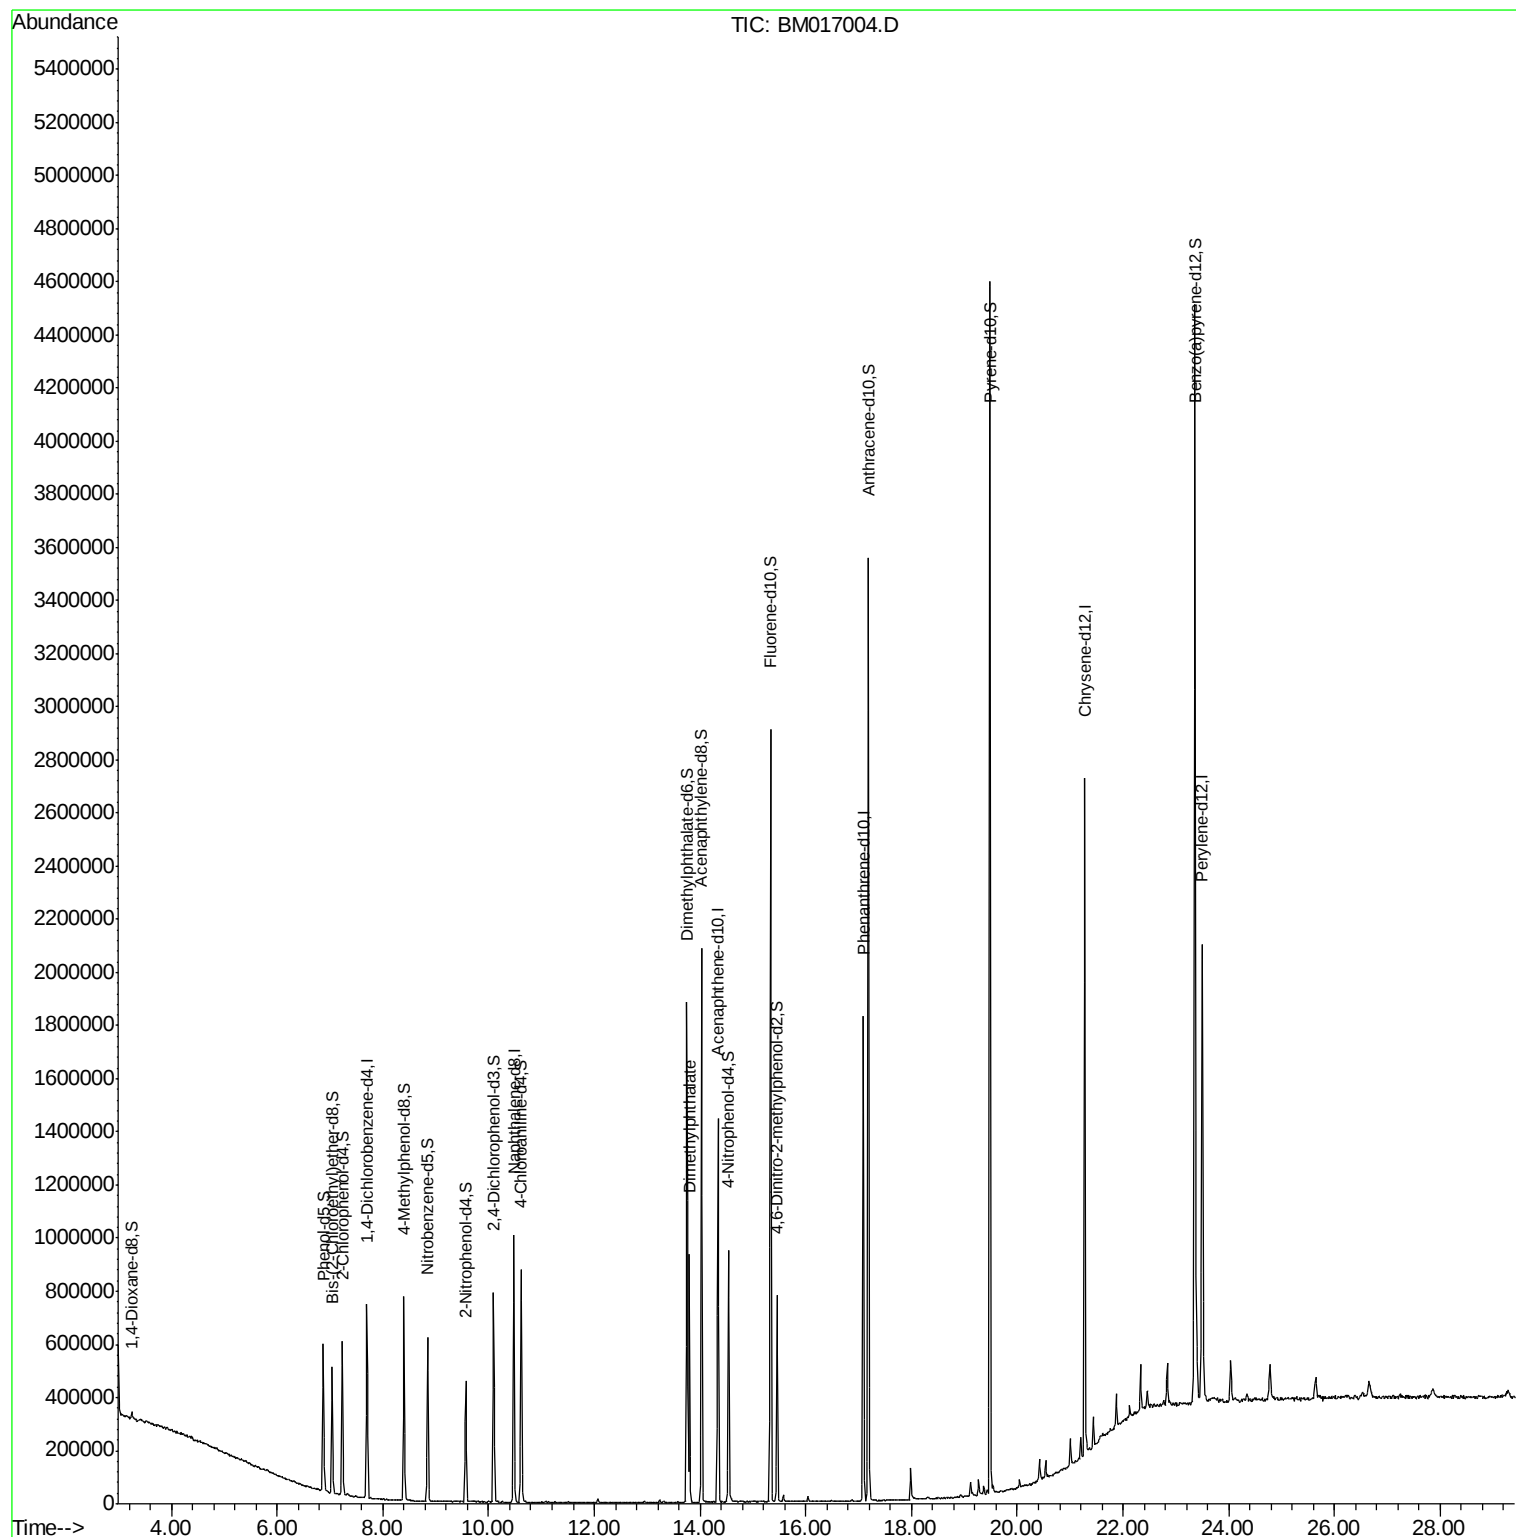

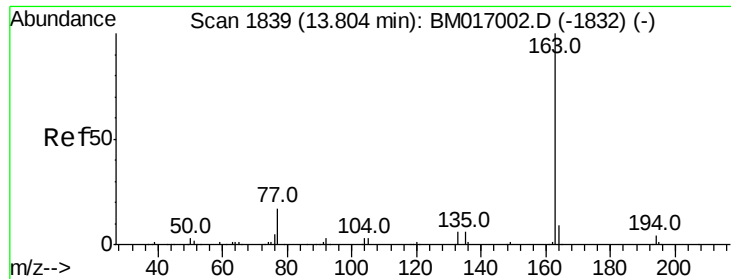

#45

Dimethylphthalate

Concen: 16.079 ng/ul

RT: 13.80 min Scan# 1838

Delta R.T. -0.01 min

Lab File: BM017004.D

Acq: 04 Oct 2018 17:48

Instrument :

BNA_M

ClientSampleId :

C0AA0


Tot Ion:163 Resp: 577244

Ion Ratio Lower Upper

163 100

194 4.0 3.3 4.9

164 10.0 8.0 12.0

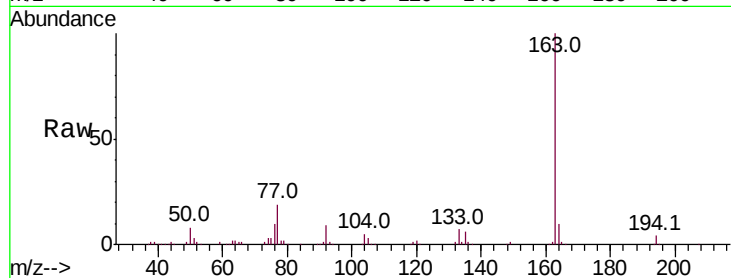

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

