

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
 Data File : BM017008.D
 Acq On : 04 Oct 2018 20:12
 Operator : MJ/SJ
 Sample : J5157-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC7

Quant Time: Oct 05 05:00:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 05 04:50:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	211095	20.00	ng/ul	0.00
18) Naphthalene-d8	10.47	136	918550	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.34	164	495169	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.09	188	1097344	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	1183530	20.00	ng/ul	0.00
86) Perylene-d12	23.50	264	1227240	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	21759	5.12	ng/uL	0.00
5) Phenol-d5	6.87	99	483930	27.42	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.04	67	312055	29.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	415379	28.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	394391	28.52	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	200792	29.91	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	204091	29.88	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	391540	27.86	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	564560	33.44	ng/ul	0.00
44) Dimethylphthalate-d6	13.75	166	1209462	30.79	ng/ul	0.00
47) Acenaphthylene-d8	14.03	160	1548632	30.84	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	148930	20.06	ng/ul	0.00
58) Fluorene-d10	15.33	176	1073190	30.67	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.46	200	108367	16.75	ng/ul	0.00
71) Anthracene-d10	17.19	188	1608797	30.69	ng/ul	0.00
79) Pyrene-d10	19.48	212	1744311	32.67	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.36	264	1955469	31.12	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.90	94	33059	1.873	ng/ul	98
45) Dimethylphthalate	13.80	163	754322	19.390	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
Data File : BM017008.D
Acq On : 04 Oct 2018 20:12
Operator : MJ/SJ
Sample : J5157-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Quant Time: Oct 05 05:00:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 05 04:50:45 2018
Response via : Initial Calibration

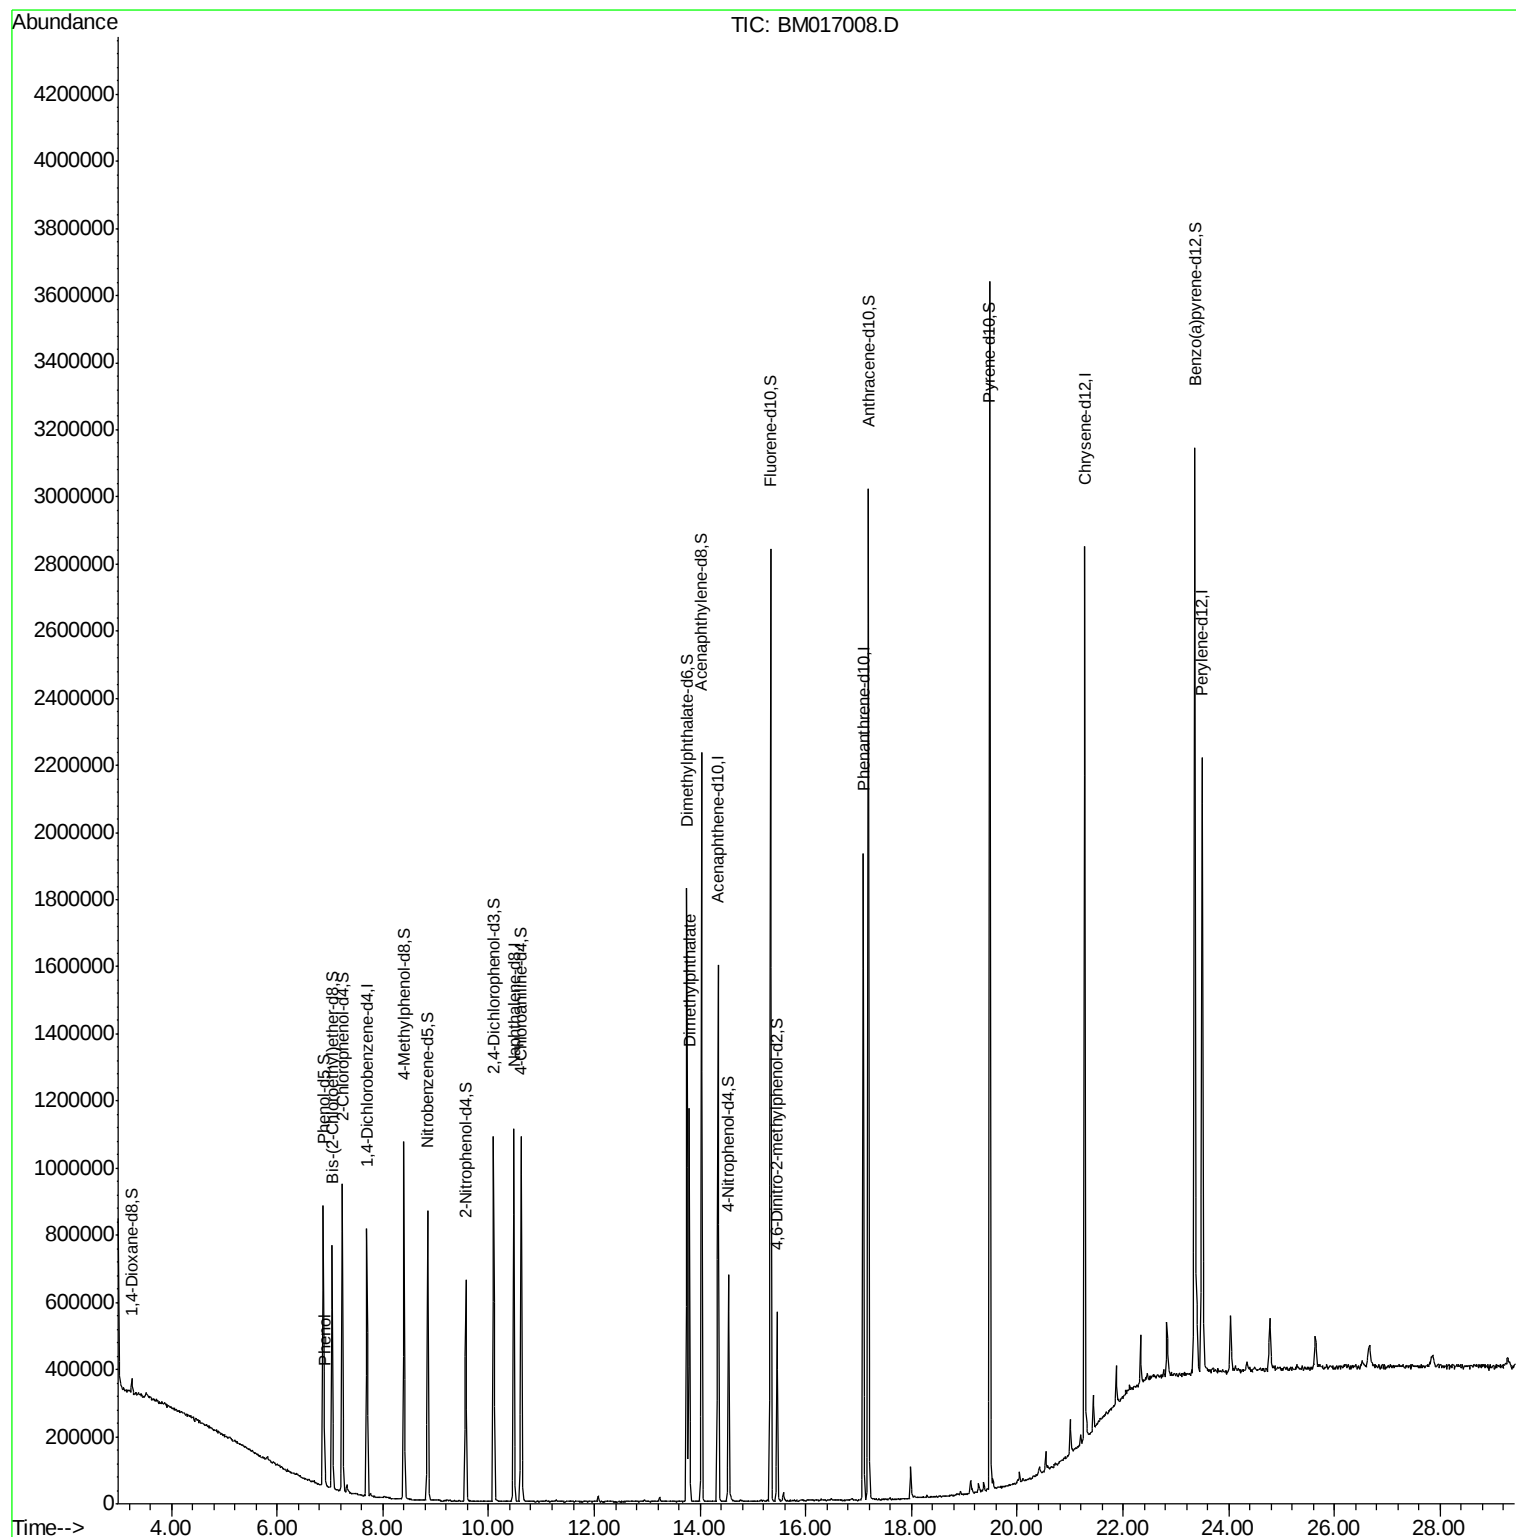

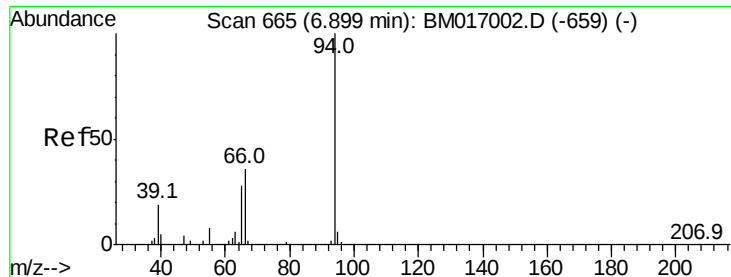

#6

Phenol

Concen: 1.873 ng/ul

RT: 6.90 min Scan# 665

Delta R.T. -0.00 min

Lab File: BM017008.D

Acq: 04 Oct 2018 20:12

Instrument :

BNA_M

ClientSampleId :

C0AC7





Tot Ion: 94 Resp: 33059

Ion Ratio Lower Upper

94 100

65 28.3 22.8 34.2

66 39.0 29.5 44.3

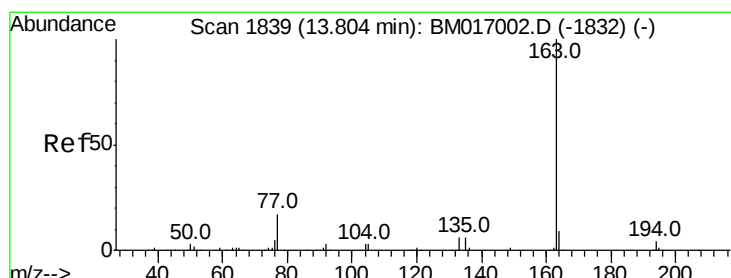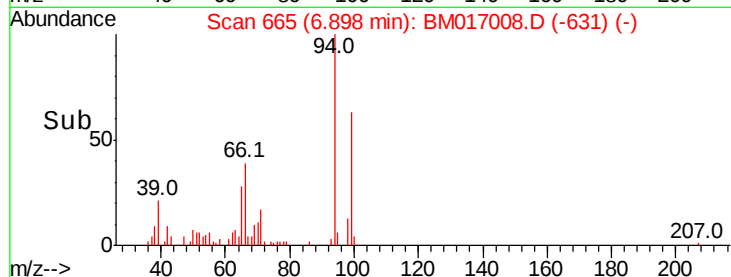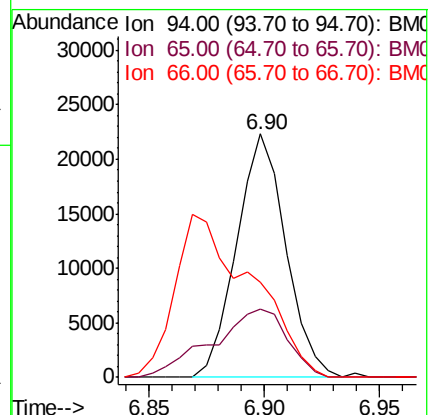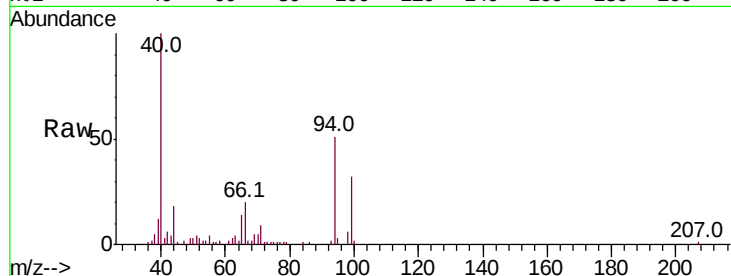

#45

Dimethylphthalate

Concen: 19.390 ng/ul

RT: 13.80 min Scan# 1838

Delta R.T. -0.01 min

Lab File: BM017008.D

Acq: 04 Oct 2018 20:12

Tgt Ion:163 Resp: 754322

Ion Ratio Lower Upper

163 100

194 4.0 3.3 4.9

164 10.3 8.0 12.0

