

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
 Data File : BM017024.D
 Acq On : 05 Oct 2018 05:51
 Operator : MJ/SJ
 Sample : J5157-20
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE2

Quant Time: Oct 05 08:22:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 05 05:34:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	251938	20.00	ng/ul	0.00
18) Naphthalene-d8	10.47	136	1123423	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.34	164	604641	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.09	188	1317703	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	1288707	20.00	ng/ul	0.00
86) Perylene-d12	23.50	264	1307562	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	21213	4.19	ng/uL	0.00
5) Phenol-d5	6.87	99	490018	23.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.04	67	316661	24.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	419058	23.93	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	402371	24.38	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	204828	24.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	207261	24.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	406027	23.62	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	575626	27.87	ng/ul	0.00
44) Dimethylphthalate-d6	13.75	166	1223900	25.51	ng/ul	0.00
47) Acenaphthylene-d8	14.03	160	1598136	26.06	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	151211	16.68	ng/ul	0.00
58) Fluorene-d10	15.33	176	1094928	25.63	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.46	200	106434	13.70	ng/ul	0.00
71) Anthracene-d10	17.19	188	1595960	25.36	ng/ul	0.00
79) Pyrene-d10	19.48	212	1670199	28.73	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.36	264	1755787	26.23	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.90	94	26146	1.241	ng/ul	93
45) Dimethylphthalate	13.80	163	269975	5.683	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
Data File : BM017024.D
Acq On : 05 Oct 2018 05:51
Operator : MJ/SJ
Sample : J5157-20
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE2

Quant Time: Oct 05 08:22:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 05 05:34:09 2018
Response via : Initial Calibration

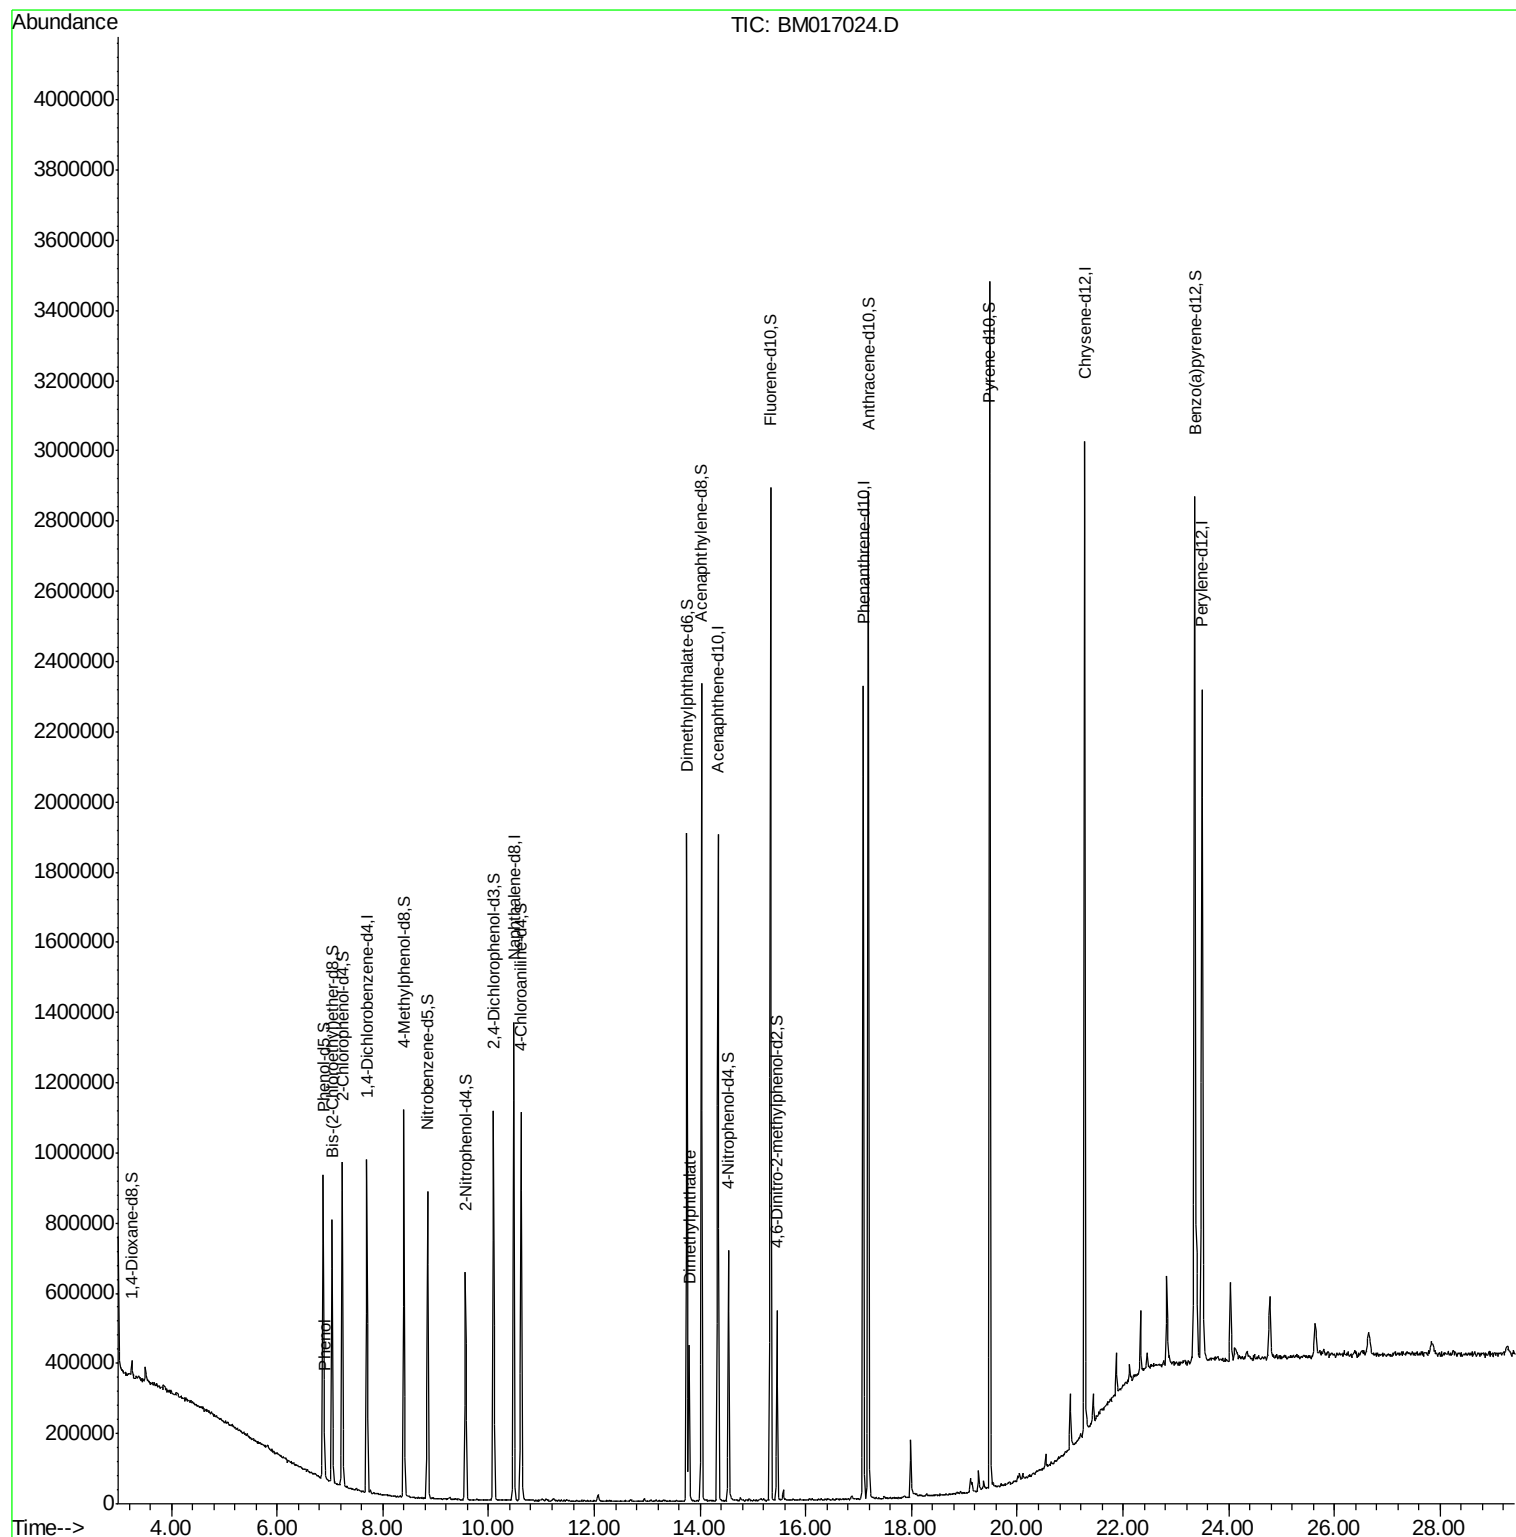

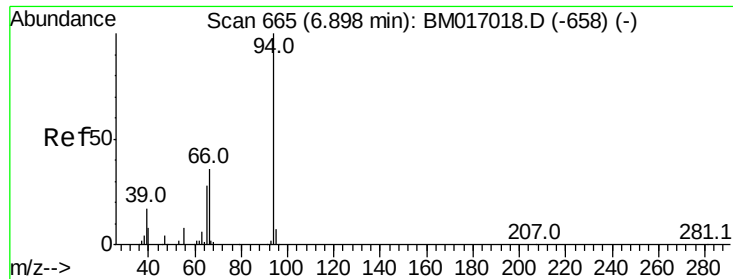

#6

Phenol

Concen: 1.241 ng/ul

RT: 6.90 min Scan# 665

Delta R.T. -0.00 min

Lab File: BM017024.D

Acq: 05 Oct 2018 05:51

Instrument :

BNA_M

ClientSampleId :

C0AE2





Tot Ion: 94 Resp: 26146

Ion Ratio Lower Upper

94 100

65 29.8 22.8 34.2

66 43.4 29.5 44.3

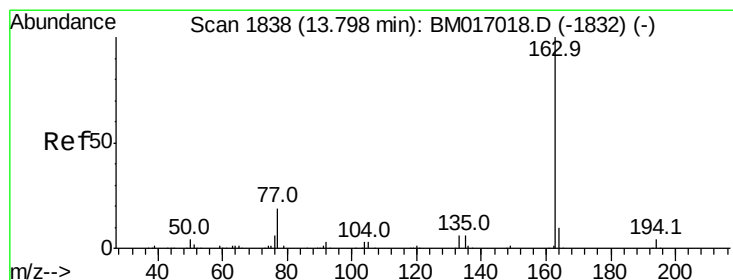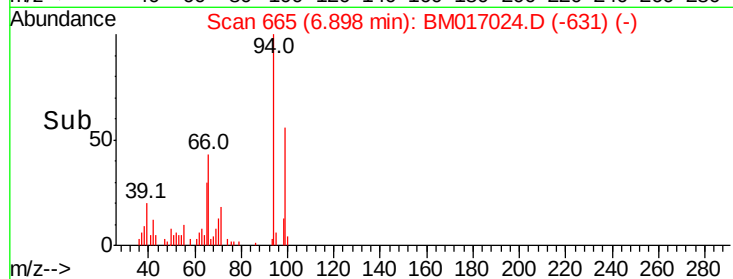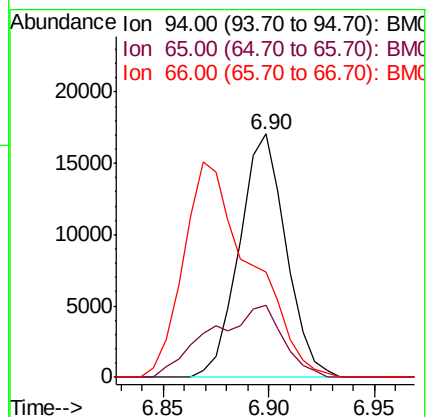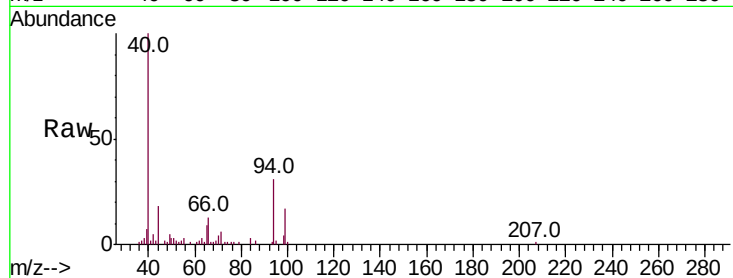

#45

Dimethylphthalate

Concen: 5.683 ng/ul

RT: 13.80 min Scan# 1838

Delta R.T. -0.00 min

Lab File: BM017024.D

Acq: 05 Oct 2018 05:51

Tgt Ion: 163 Resp: 269975

Ion Ratio Lower Upper

163 100

194 4.2 3.3 4.9

164 9.8 8.0 12.0

