

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
 Data File : BM017001.D
 Acq On : 04 Oct 2018 15:59
 Operator : MJ/SJ
 Sample : PB113373BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK73

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.875	654	661	670	rVB	682295	1069342	24.52%	2.219%
2	7.040	683	689	698	rVB	587866	871919	19.99%	1.810%
3	7.234	716	722	729	rVB	739774	1122248	25.73%	2.329%
4	7.698	795	801	810	rVB	872827	1375274	31.53%	2.854%
5	8.398	914	920	933	rVB	840124	1329330	30.48%	2.759%
6	8.851	990	997	1007	rBV	681391	1088607	24.96%	2.259%
7	9.569	1111	1119	1128	rBV	522087	834364	19.13%	1.732%
8	10.098	1202	1209	1218	rBV	860324	1366899	31.34%	2.837%
9	10.481	1265	1274	1281	rBV	1208008	2017320	46.25%	4.187%
10	10.616	1290	1297	1309	rBV	854925	1435055	32.90%	2.978%
11	12.069	1540	1544	1550	rVB	13021	21172	0.49%	0.044%
12	13.751	1824	1830	1839	rVB	1494341	2102222	48.19%	4.363%
13	14.027	1871	1877	1887	rBV	1779590	2577764	59.10%	5.350%
14	14.339	1923	1930	1941	rBV2	1820475	2673358	61.29%	5.548%
15	14.539	1958	1964	1976	rBV	647060	902027	20.68%	1.872%
16	15.333	2093	2099	2106	rBV	2319722	3259540	74.73%	6.765%
17	15.457	2115	2120	2128	rBV	530166	702703	16.11%	1.458%
18	15.574	2136	2140	2144	rBV3	20420	27507	0.63%	0.057%
19	16.874	2356	2361	2366	rVB2	9209	11407	0.26%	0.024%
20	17.086	2391	2397	2404	rBV2	2349158	3162609	72.50%	6.564%
21	17.186	2408	2414	2428	rBV	2583927	3473818	79.64%	7.210%
22	19.115	2738	2742	2747	rBV	28170	37061	0.85%	0.077%
23	19.374	2782	2786	2789	rVB	18206	21130	0.48%	0.044%
24	19.486	2798	2805	2811	rBV	2972221	4015402	92.06%	8.334%
25	21.274	3104	3109	3116	rBV	2995856	3843062	88.10%	7.976%
26	22.839	3372	3375	3381	rVB	138199	180775	4.14%	0.375%
27	23.362	3457	3464	3470	rBV	2345008	4361957	100.00%	9.053%
28	23.503	3481	3488	3499	rVB	2129050	3944296	90.42%	8.186%
29	24.038	3576	3579	3588	rVB	197575	353729	8.11%	0.734%


Sum of corrected areas: 48181897

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
Data File : BM017001.D
Acq On : 04 Oct 2018 15:59
Operator : MJ/SJ
Sample : PB113373BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK73

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

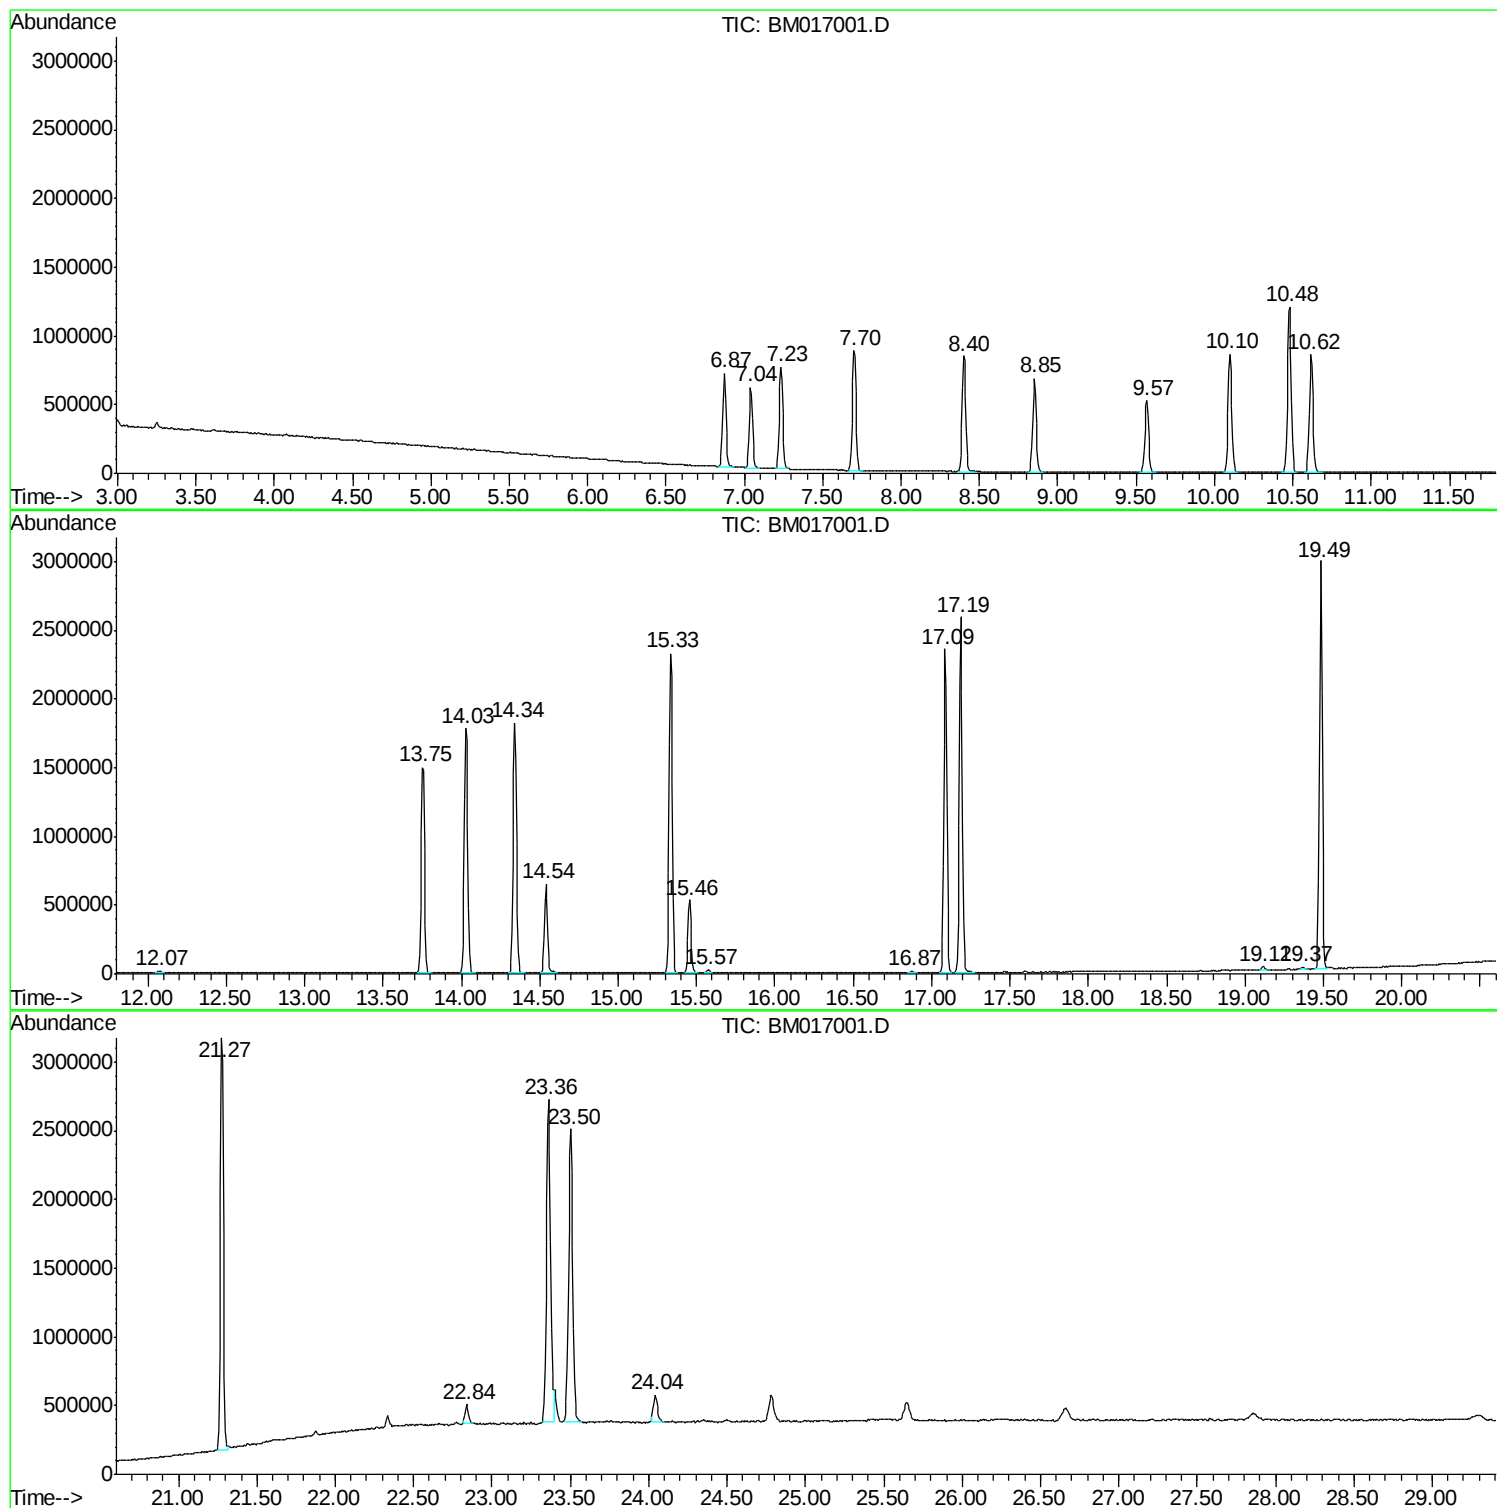

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100418\
Data File : BM017001.D
Acq On : 04 Oct 2018 15:59
Operator : MJ/SJ
Sample : PB113373BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK73

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100418\
Data File : BM017001.D
Acq On : 04 Oct 2018 15:59
Operator : MJ/SJ
Sample : PB113373BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK73

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc