

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
 Data File : BM017007.D
 Acq On : 04 Oct 2018 19:36
 Operator : MJ/SJ
 Sample : J5157-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.875	654	661	672	rVB	973874	1664014	27.33%	2.659%
2	7.040	683	689	702	rVB	856447	1283909	21.09%	2.052%
3	7.234	716	722	730	rVB	1081490	1651730	27.13%	2.640%
4	7.310	732	735	741	rBV3	24367	40180	0.66%	0.064%
5	7.699	795	801	808	rVB	828672	1292975	21.24%	2.066%
6	7.763	808	812	819	rVB4	14256	22156	0.36%	0.035%
7	8.398	911	920	938	rVB	1256784	2003554	32.91%	3.202%
8	8.851	990	997	1006	rVB	1008445	1599793	26.28%	2.557%
9	9.569	1110	1119	1132	rVB	785150	1254385	20.61%	2.005%
10	10.098	1201	1209	1221	rBV	1270713	2059795	33.84%	3.292%
11	10.475	1266	1273	1280	rBV	1128871	1896157	31.15%	3.030%
12	10.616	1290	1297	1308	rBV	1294584	2095868	34.43%	3.349%
13	12.069	1537	1544	1550	rBV3	20105	34755	0.57%	0.056%
14	12.945	1687	1693	1696	rVB3	5630	7157	0.12%	0.011%
15	13.239	1737	1743	1749	rVB4	15196	22594	0.37%	0.036%
16	13.751	1824	1830	1835	rBV	2067582	3005528	49.37%	4.803%
17	13.798	1835	1838	1846	rVB	1472279	1907626	31.34%	3.049%
18	14.028	1867	1877	1885	rBV	2540967	3775683	62.02%	6.034%
19	14.339	1923	1930	1939	rBV2	1596846	2439241	40.07%	3.898%
20	14.539	1957	1964	1976	rBV	860606	1176405	19.32%	1.880%
21	14.763	1999	2002	2007	rVB4	8053	10958	0.18%	0.018%
22	15.145	2064	2067	2071	rBV3	4908	7456	0.12%	0.012%
23	15.333	2092	2099	2107	rBV	3214537	4631503	76.08%	7.402%
24	15.457	2114	2120	2131	rVB	728590	969139	15.92%	1.549%
25	15.574	2135	2140	2145	rBV	36992	45919	0.75%	0.073%
26	16.486	2290	2295	2299	rVB3	7078	9393	0.15%	0.015%
27	16.874	2356	2361	2365	rBV4	7746	11255	0.18%	0.018%
28	17.086	2390	2397	2405	rBV	2024728	2811207	46.18%	4.493%
29	17.186	2407	2414	2424	rBV2	3466888	4832744	79.39%	7.723%
30	17.986	2546	2550	2559	rBV	90279	125408	2.06%	0.200%
31	18.063	2560	2563	2566	rVB3	6760	8485	0.14%	0.014%
32	18.921	2707	2709	2713	rVB3	8783	9019	0.15%	0.014%
33	19.115	2738	2742	2745	rBV	43643	62830	1.03%	0.100%
34	19.145	2745	2747	2753	rVB	20217	24908	0.41%	0.040%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
 Data File : BM017007.D
 Acq On : 04 Oct 2018 19:36
 Operator : MJ/SJ
 Sample : J5157-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Title : SVOA CALIBRATION

35	19.274	2765	2769	2774	rBV5	36721	48475	0.80%	0.077%
36	19.368	2781	2785	2790	rBV	29057	40669	0.67%	0.065%
37	19.480	2798	2804	2812	rBV	4009292	5606468	92.10%	8.960%
38	19.539	2812	2814	2820	rVB4	28909	42126	0.69%	0.067%
39	20.039	2897	2899	2904	rVB4	27825	34953	0.57%	0.056%
40	20.233	2930	2932	2936	rVB4	17474	17261	0.28%	0.028%
41	20.539	2981	2984	2987	rVB	50090	50008	0.82%	0.080%
42	21.004	3059	3063	3070	rBV	134002	182292	2.99%	0.291%
43	21.203	3094	3097	3100	rBV2	54227	62473	1.03%	0.100%
44	21.274	3104	3109	3114	rBV	2769289	3424538	56.26%	5.473%
45	21.439	3134	3137	3142	rVB2	88991	91264	1.50%	0.146%
46	21.874	3208	3211	3215	rVB	86063	94559	1.55%	0.151%
47	22.127	3251	3254	3258	rBV	95301	115814	1.90%	0.185%
48	22.333	3286	3289	3293	rVB	127544	159689	2.62%	0.255%
49	22.833	3371	3374	3381	rVB	149944	229928	3.78%	0.367%
50	23.362	3457	3464	3477	rVB	3174555	6087516	100.00%	9.729%
51	23.497	3480	3487	3496	rBV2	1818356	3491401	57.35%	5.580%


Sum of corrected areas: 62573163

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
Data File : BM017007.D
Acq On : 04 Oct 2018 19:36
Operator : MJ/SJ
Sample : J5157-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

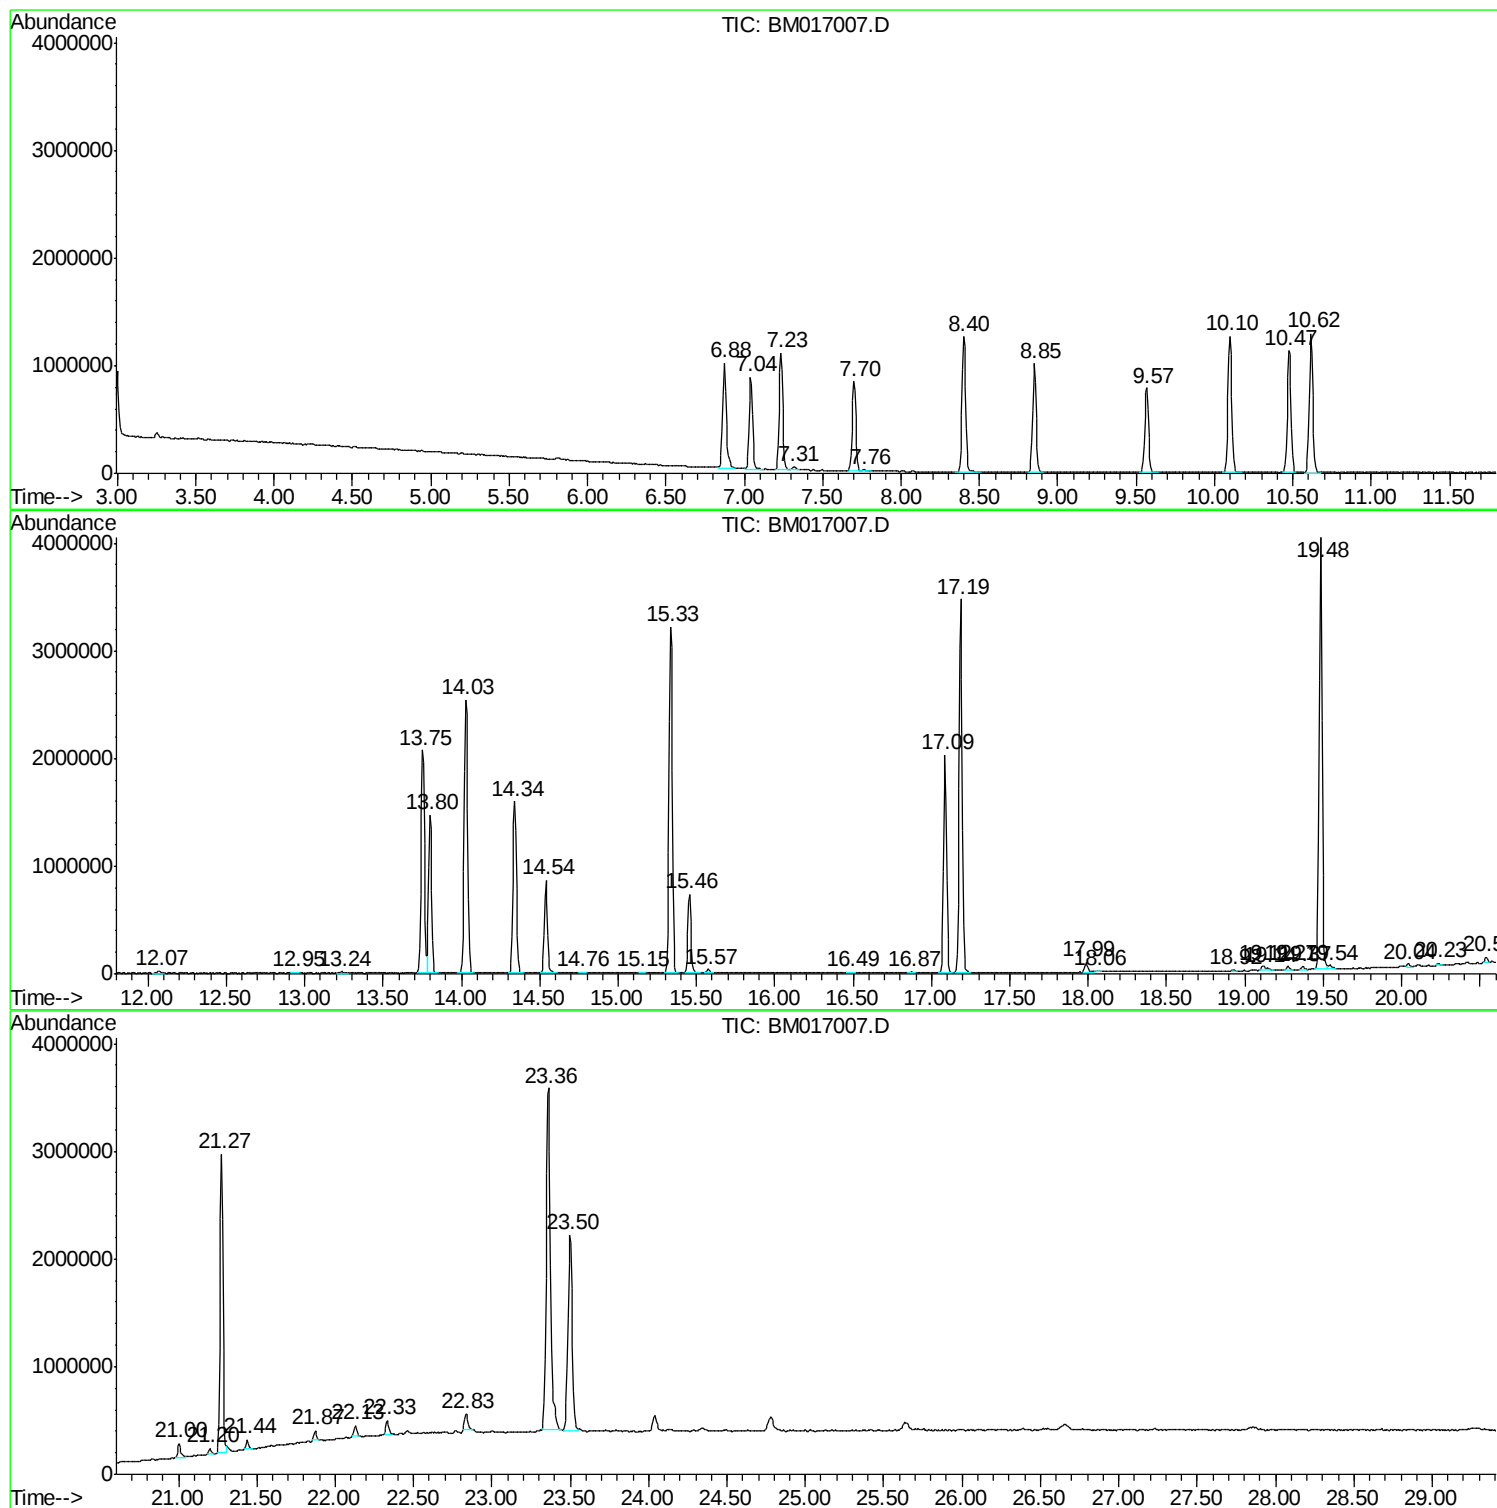

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100418\
Data File : BM017007.D
Acq On : 04 Oct 2018 19:36
Operator : MJ/SJ
Sample : J5157-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100418\
Data File : BM017007.D
Acq On : 04 Oct 2018 19:36
Operator : MJ/SJ
Sample : J5157-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc