

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
 Data File : BM017008.D
 Acq On : 04 Oct 2018 20:12
 Operator : MJ/SJ
 Sample : J5157-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.875	654	661	670	rVB	835468	1421165	26.84%	2.568%
2	7.039	683	689	701	rVB	726708	1099629	20.77%	1.987%
3	7.234	716	722	732	rVB	919483	1415984	26.74%	2.559%
4	7.316	732	736	742	rVB3	21576	35475	0.67%	0.064%
5	7.698	795	801	808	rVV	796533	1247299	23.56%	2.254%
6	7.763	808	812	817	rVB3	10887	16800	0.32%	0.030%
7	8.398	912	920	931	rBV	1064879	1696516	32.04%	3.066%
8	8.851	989	997	1005	rVB	864743	1369327	25.86%	2.475%
9	9.269	1064	1068	1073	rVB3	3875	5763	0.11%	0.010%
10	9.569	1112	1119	1130	rBV	657613	1046823	19.77%	1.892%
11	10.098	1202	1209	1222	rBV	1088475	1763441	33.30%	3.187%
12	10.475	1266	1273	1283	rVB	1110256	1833412	34.62%	3.313%
13	10.616	1288	1297	1312	rVB	1087800	1808120	34.15%	3.268%
14	11.080	1371	1376	1379	rBV4	3537	5898	0.11%	0.011%
15	11.269	1403	1408	1411	rVB4	4073	5659	0.11%	0.010%
16	12.069	1539	1544	1551	rVB2	18565	28997	0.55%	0.052%
17	12.945	1687	1693	1696	rBV3	5728	7935	0.15%	0.014%
18	13.239	1738	1743	1747	rVB3	14482	21123	0.40%	0.038%
19	13.751	1824	1830	1834	rBV	1828108	2530272	47.78%	4.573%
20	13.798	1834	1838	1846	rVB	1170494	1623127	30.65%	2.933%
21	14.027	1868	1877	1885	rBV	2230726	3208879	60.60%	5.799%
22	14.339	1923	1930	1939	rBV2	1597313	2359569	44.56%	4.264%
23	14.539	1956	1964	1978	rBV	677271	991069	18.72%	1.791%
24	14.762	1997	2002	2006	rBV4	5801	8463	0.16%	0.015%
25	15.151	2064	2068	2071	rBV2	4015	6914	0.13%	0.012%
26	15.198	2074	2076	2080	rVB3	4502	5409	0.10%	0.010%
27	15.333	2093	2099	2106	rBV	2835289	3947483	74.55%	7.134%
28	15.457	2114	2120	2131	rVB	561858	756220	14.28%	1.367%
29	15.574	2135	2140	2144	rBV2	26713	38371	0.72%	0.069%
30	16.480	2290	2294	2300	rVV4	6850	11103	0.21%	0.020%
31	16.874	2357	2361	2365	rVB3	5774	10196	0.19%	0.018%
32	17.086	2391	2397	2406	rBV2	1926767	2704439	51.07%	4.888%
33	17.186	2407	2414	2427	rVB	3011452	4131580	78.03%	7.467%
34	17.986	2545	2550	2557	rBV2	93955	129068	2.44%	0.233%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
 Data File : BM017008.D
 Acq On : 04 Oct 2018 20:12
 Operator : MJ/SJ
 Sample : J5157-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Title : SVOA CALIBRATION

35	18.286	2599	2601	2605	rBV4	7089	7664	0.14%	0.014%
36	18.927	2707	2710	2713	rVB4	8329	7796	0.15%	0.014%
37	19.121	2738	2743	2747	rBV	39277	65197	1.23%	0.118%
38	19.274	2765	2769	2774	rBV4	28323	42014	0.79%	0.076%
39	19.368	2781	2785	2792	rBV	25774	34954	0.66%	0.063%
40	19.427	2792	2795	2798	rBV4	9078	13318	0.25%	0.024%
41	19.480	2799	2804	2811	rVV	3598197	4770450	90.09%	8.621%
42	19.539	2811	2814	2820	rVB3	28040	46284	0.87%	0.084%
43	20.045	2897	2900	2904	rVB3	30027	29617	0.56%	0.054%
44	20.539	2981	2984	2988	rBV2	54607	60559	1.14%	0.109%
45	21.003	3059	3063	3071	rBV	106147	155447	2.94%	0.281%
46	21.274	3104	3109	3114	rBV	2657092	3256799	61.51%	5.886%
47	21.439	3134	3137	3141	rBV2	98477	105343	1.99%	0.190%
48	21.868	3208	3210	3216	rVB2	101661	101481	1.92%	0.183%
49	22.333	3286	3289	3294	rVB	133525	160563	3.03%	0.290%
50	22.833	3371	3374	3386	rVB3	163150	281496	5.32%	0.509%
51	23.356	3457	3463	3478	rVB	2752340	5295168	100.00%	9.570%
52	23.497	3481	3487	3502	rVB	1828671	3327793	62.85%	6.014%
53	24.038	3576	3579	3586	rVB3	162987	280146	5.29%	0.506%


Sum of corrected areas: 55333617

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
Data File : BM017008.D
Acq On : 04 Oct 2018 20:12
Operator : MJ/SJ
Sample : J5157-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

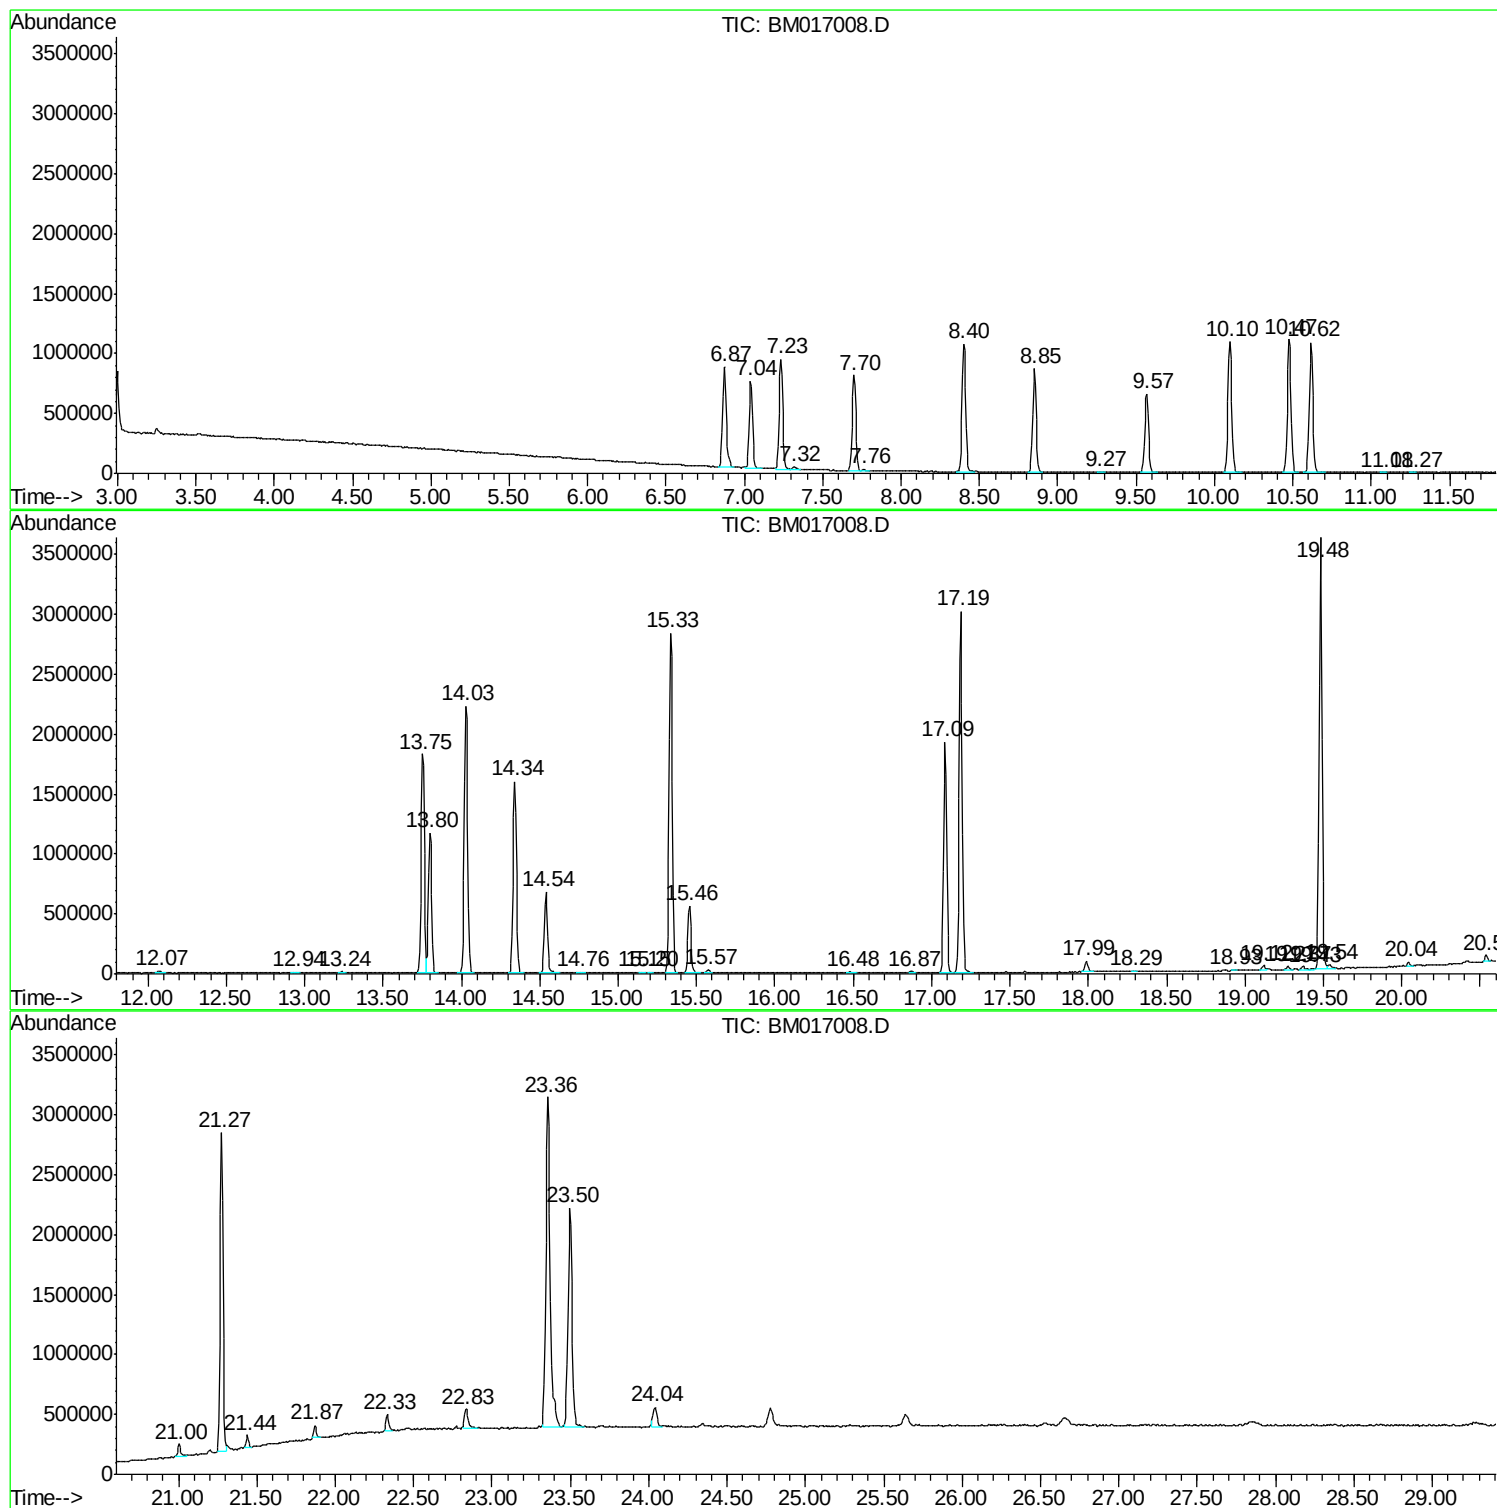

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100418\
Data File : BM017008.D
Acq On : 04 Oct 2018 20:12
Operator : MJ/SJ
Sample : J5157-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100418\
Data File : BM017008.D
Acq On : 04 Oct 2018 20:12
Operator : MJ/SJ
Sample : J5157-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc