

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
 Data File : BM017012.D
 Acq On : 04 Oct 2018 22:37
 Operator : MJ/SJ
 Sample : J5157-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.875	654	661	673	rVB	1090599	1785190	27.11%	2.689%
2	7.039	683	689	702	rVB	943966	1405714	21.35%	2.118%
3	7.234	715	722	730	rVB	1203238	1819628	27.64%	2.741%
4	7.698	794	801	808	rVV	841093	1304015	19.81%	1.965%
5	7.757	809	811	824	rVB3	11491	20423	0.31%	0.031%
6	8.016	851	855	862	rVB5	4791	7687	0.12%	0.012%
7	8.398	914	920	928	rBV	1386732	2167251	32.92%	3.265%
8	8.851	990	997	1006	rVB	1107077	1778558	27.01%	2.679%
9	9.269	1063	1068	1071	rBV4	4854	8156	0.12%	0.012%
10	9.569	1111	1119	1129	rBV	849888	1370864	20.82%	2.065%
11	10.098	1202	1209	1216	rBV	1409929	2283682	34.69%	3.440%
12	10.474	1265	1273	1282	rBV	1178476	1931716	29.34%	2.910%
13	10.616	1289	1297	1308	rBV	1387817	2319021	35.22%	3.494%
14	12.068	1539	1544	1550	rVB3	24313	37048	0.56%	0.056%
15	12.939	1688	1692	1697	rVB4	6180	8564	0.13%	0.013%
16	13.233	1735	1742	1748	rBV2	13388	20896	0.32%	0.031%
17	13.751	1823	1830	1835	rBV	2326322	3312725	50.31%	4.991%
18	13.798	1835	1838	1845	rVV	1105674	1457041	22.13%	2.195%
19	14.027	1870	1877	1887	rVB	2950988	4205552	63.88%	6.336%
20	14.339	1923	1930	1942	rVB2	1664342	2471854	37.54%	3.724%
21	14.539	1956	1964	1977	rBV	879313	1210102	18.38%	1.823%
22	14.762	1999	2002	2006	rVB3	10372	14600	0.22%	0.022%
23	15.145	2063	2067	2071	rBV3	4610	7609	0.12%	0.011%
24	15.204	2074	2077	2081	rVB5	5818	8169	0.12%	0.012%
25	15.333	2092	2099	2108	rBV	3648899	5155743	78.31%	7.767%
26	15.457	2112	2120	2132	rBV	750859	1003344	15.24%	1.512%
27	15.574	2135	2140	2146	rBV	42190	55904	0.85%	0.084%
28	16.062	2219	2223	2228	rBV6	5050	8540	0.13%	0.013%
29	16.480	2289	2294	2298	rBV5	13308	18258	0.28%	0.028%
30	16.862	2355	2359	2367	rVB4	7907	14211	0.22%	0.021%
31	17.086	2391	2397	2404	rBV	2019761	2829594	42.98%	4.263%
32	17.186	2407	2414	2425	rVV	3913142	5316587	80.75%	8.010%
33	17.986	2546	2550	2560	rBV	135251	207848	3.16%	0.313%
34	18.292	2599	2602	2604	rBV4	7134	6606	0.10%	0.010%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
Data File : BM017012.D
Acq On : 04 Oct 2018 22:37
Operator : MJ/SJ
Sample : J5157-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD2

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Title : SVOA CALIBRATION

35	18.862	2695	2699	2706	rBV6	20689	40495	0.62%	0.061%
36	18.927	2707	2710	2716	rVB4	13087	18217	0.28%	0.027%
37	19.115	2738	2742	2746	rBV	52448	78924	1.20%	0.119%
38	19.274	2765	2769	2774	rBV4	42459	60705	0.92%	0.091%
39	19.368	2782	2785	2792	rVB	35001	47893	0.73%	0.072%
40	19.480	2798	2804	2812	rBV	4415249	6147006	93.36%	9.261%
41	19.539	2812	2814	2819	rVB3	33280	46067	0.70%	0.069%
42	20.039	2897	2899	2904	rVB2	36935	42446	0.64%	0.064%
43	20.539	2981	2984	2987	rVB	79392	80436	1.22%	0.121%
44	21.003	3059	3063	3070	rBV	176064	238231	3.62%	0.359%
45	21.274	3104	3109	3114	rBV	2694017	3356570	50.98%	5.057%
46	21.438	3134	3137	3140	rBV	141050	135923	2.06%	0.205%
47	21.868	3208	3210	3220	rVB	123541	162727	2.47%	0.245%
48	22.333	3286	3289	3293	rVB	133561	151029	2.29%	0.228%
49	22.833	3371	3374	3379	rVB	163329	210728	3.20%	0.317%
50	23.362	3456	3464	3479	rBV	3452871	6584017	100.00%	9.919%
51	23.497	3481	3487	3500	rVB	1861450	3404167	51.70%	5.128%


Sum of corrected areas: 66378281

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
Data File : BM017012.D
Acq On : 04 Oct 2018 22:37
Operator : MJ/SJ
Sample : J5157-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

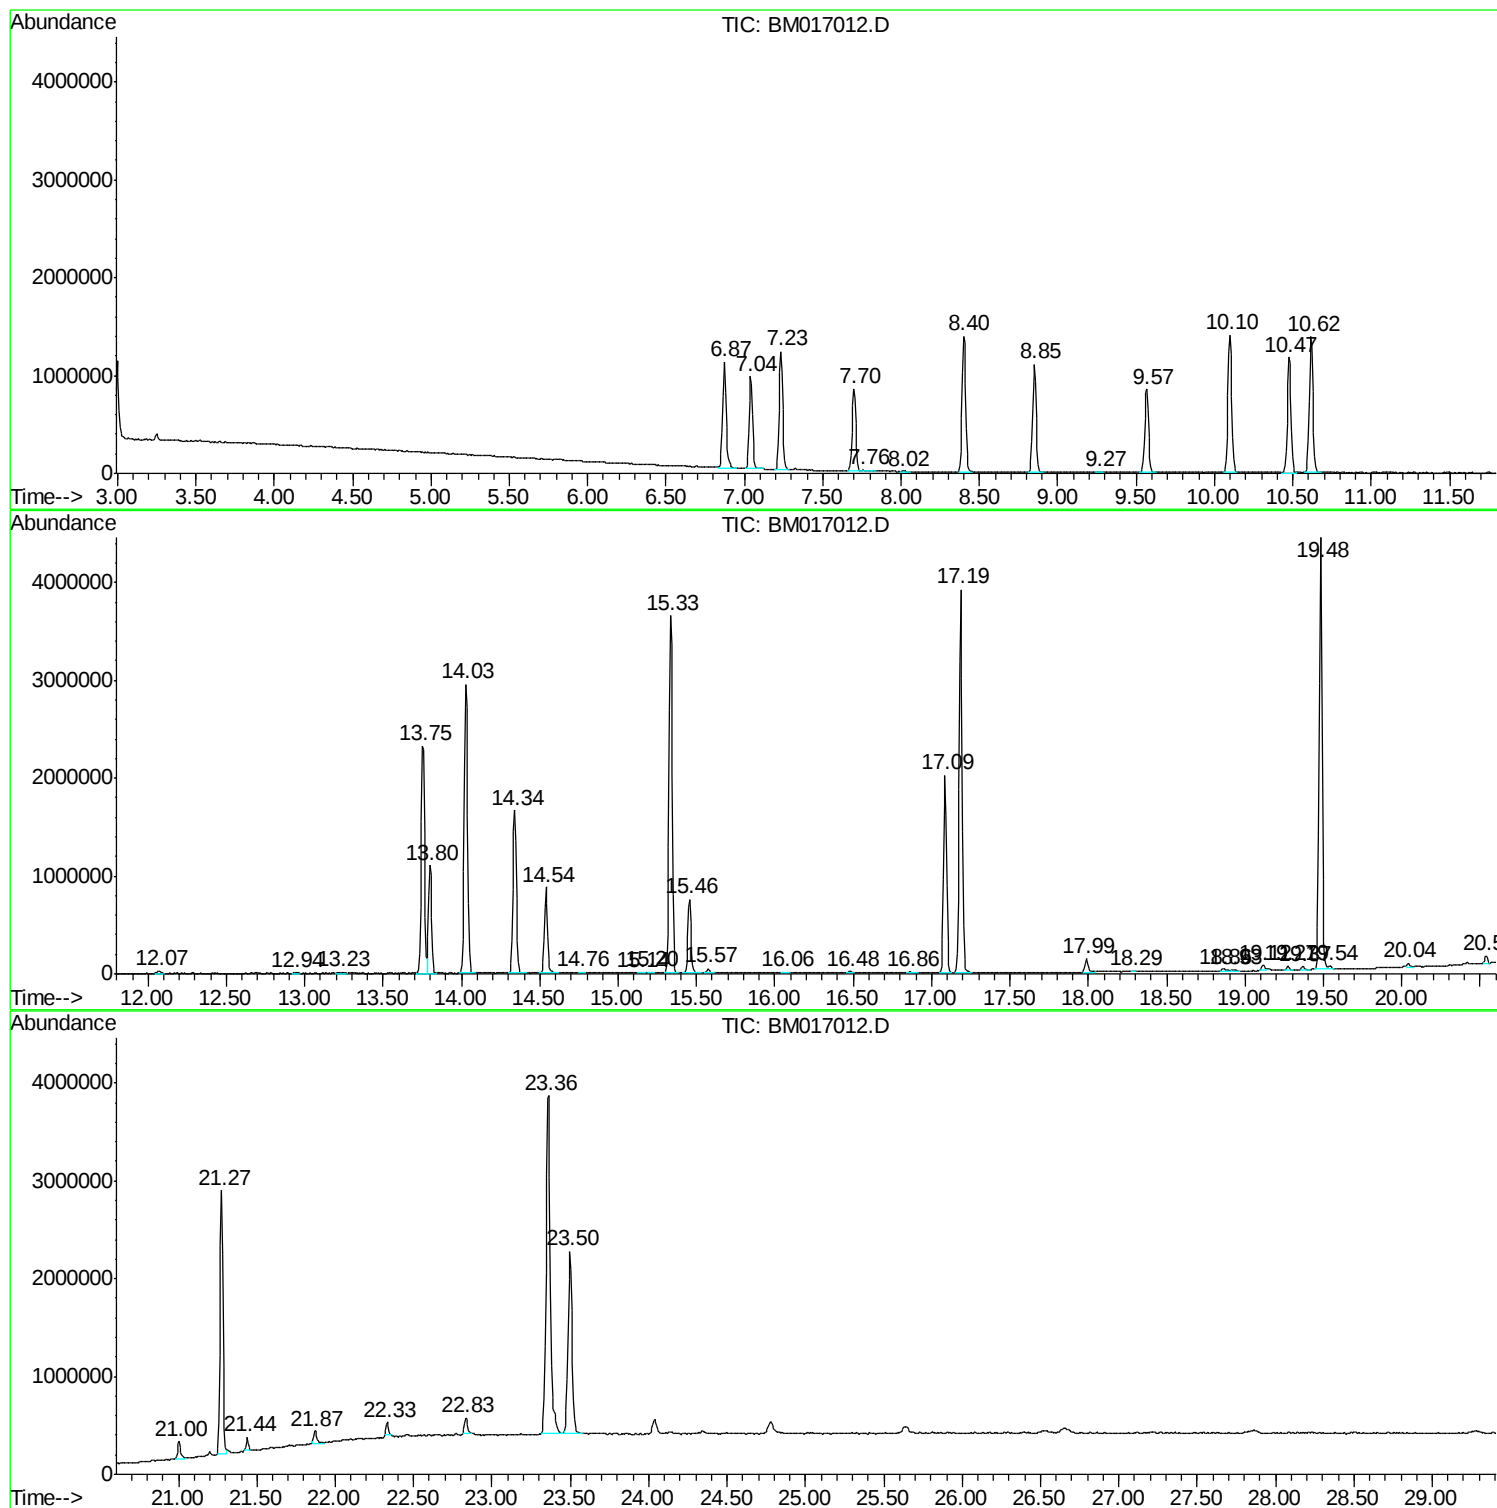

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100418\
Data File : BM017012.D
Acq On : 04 Oct 2018 22:37
Operator : MJ/SJ
Sample : J5157-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100418\
Data File : BM017012.D
Acq On : 04 Oct 2018 22:37
Operator : MJ/SJ
Sample : J5157-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc