

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
 Data File : BM017013.D
 Acq On : 04 Oct 2018 23:13
 Operator : MJ/SJ
 Sample : J5157-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.869	654	660	674	rVB	831981	1399612	24.69%	2.490%
2	7.039	683	689	703	rVB	729696	1081276	19.07%	1.924%
3	7.234	716	722	733	rVB	912951	1387592	24.47%	2.468%
4	7.698	795	801	808	rBV	865161	1361501	24.01%	2.422%
5	7.763	809	812	817	rVB3	8551	12591	0.22%	0.022%
6	8.398	914	920	930	rBV	984442	1564358	27.59%	2.783%
7	8.851	988	997	1005	rBV	841750	1329367	23.45%	2.365%
8	9.269	1062	1068	1073	rVB4	4748	8014	0.14%	0.014%
9	9.569	1111	1119	1126	rBV	627945	1003469	17.70%	1.785%
10	10.098	1202	1209	1218	rBV	1045107	1693550	29.87%	3.013%
11	10.475	1266	1273	1281	rBV	1201026	2015771	35.55%	3.586%
12	10.616	1287	1297	1309	rBV	939991	1577541	27.82%	2.806%
13	12.069	1538	1544	1552	rVB2	17032	29464	0.52%	0.052%
14	12.945	1688	1693	1697	rBV3	5507	9049	0.16%	0.016%
15	13.239	1738	1743	1747	rBV3	11066	18249	0.32%	0.032%
16	13.751	1824	1830	1834	rBV	1790885	2476341	43.68%	4.405%
17	13.798	1834	1838	1845	rVB	1066323	1413331	24.93%	2.514%
18	14.027	1867	1877	1886	rBV	2156323	3097038	54.62%	5.510%
19	14.339	1923	1930	1937	rBV2	1721760	2541337	44.82%	4.521%
20	14.539	1956	1964	1976	rBV	597640	836392	14.75%	1.488%
21	14.704	1988	1992	1995	rVB4	5456	7012	0.12%	0.012%
22	14.763	1998	2002	2009	rVB5	29475	42196	0.74%	0.075%
23	15.145	2061	2067	2068	rBV4	5698	6389	0.11%	0.011%
24	15.168	2068	2071	2075	rVV2	14632	18829	0.33%	0.033%
25	15.333	2092	2099	2108	rBV	2776197	3896604	68.72%	6.932%
26	15.457	2114	2120	2131	rVB	535176	706465	12.46%	1.257%
27	15.574	2135	2140	2145	rBV2	29304	38342	0.68%	0.068%
28	16.068	2221	2224	2227	rVB4	5032	6089	0.11%	0.011%
29	16.486	2289	2295	2299	rBV6	8928	14093	0.25%	0.025%
30	16.857	2354	2358	2359	rBV3	6021	7089	0.13%	0.013%
31	16.874	2359	2361	2365	rVB2	7442	7971	0.14%	0.014%
32	17.086	2391	2397	2404	rBV2	2085239	2910588	51.33%	5.178%
33	17.186	2407	2414	2426	rVV	2950923	4088811	72.11%	7.274%
34	17.474	2458	2463	2464	rBV3	4400	6179	0.11%	0.011%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
 Data File : BM017013.D
 Acq On : 04 Oct 2018 23:13
 Operator : MJ/SJ
 Sample : J5157-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
 Title : SVOA CALIBRATION

35	17.862	2527	2529	2534	rVV4	5040	5885	0.10%	0.010%
36	17.986	2545	2550	2560	rBV2	147311	233018	4.11%	0.415%
37	18.503	2635	2638	2644	rBV5	12227	19559	0.34%	0.035%
38	18.803	2686	2689	2691	rBV4	5800	7052	0.12%	0.013%
39	18.921	2707	2709	2713	rVB5	8512	8880	0.16%	0.016%
40	19.115	2738	2742	2745	rBV2	40047	61396	1.08%	0.109%
41	19.145	2745	2747	2756	rVB	28770	41855	0.74%	0.074%
42	19.274	2765	2769	2775	rBV3	41971	61372	1.08%	0.109%
43	19.368	2781	2785	2790	rBV2	28646	42027	0.74%	0.075%
44	19.480	2798	2804	2813	rBV	3563716	4932038	86.99%	8.774%
45	20.045	2897	2900	2903	rVB3	22374	23278	0.41%	0.041%
46	20.421	2961	2964	2967	rVB4	24561	27965	0.49%	0.050%
47	20.539	2981	2984	2987	rBV3	42904	44294	0.78%	0.079%
48	21.003	3059	3063	3070	rBV2	154158	229653	4.05%	0.409%
49	21.203	3094	3097	3101	rBV2	85988	95500	1.68%	0.170%
50	21.274	3104	3109	3122	rVV	2895600	3641499	64.23%	6.478%
51	21.439	3134	3137	3140	rBV2	88175	94230	1.66%	0.168%
52	21.868	3208	3210	3216	rVB	89839	105229	1.86%	0.187%
53	22.333	3286	3289	3293	rVB	152750	181612	3.20%	0.323%
54	22.838	3371	3375	3380	rVB	178412	262253	4.63%	0.467%
55	23.362	3457	3464	3477	rVV	2909097	5669875	100.00%	10.087%
56	23.497	3481	3487	3503	rVB2	1938370	3811390	67.22%	6.780%


Sum of corrected areas: 56212360

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM100418\
Data File : BM017013.D
Acq On : 04 Oct 2018 23:13
Operator : MJ/SJ
Sample : J5157-09
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

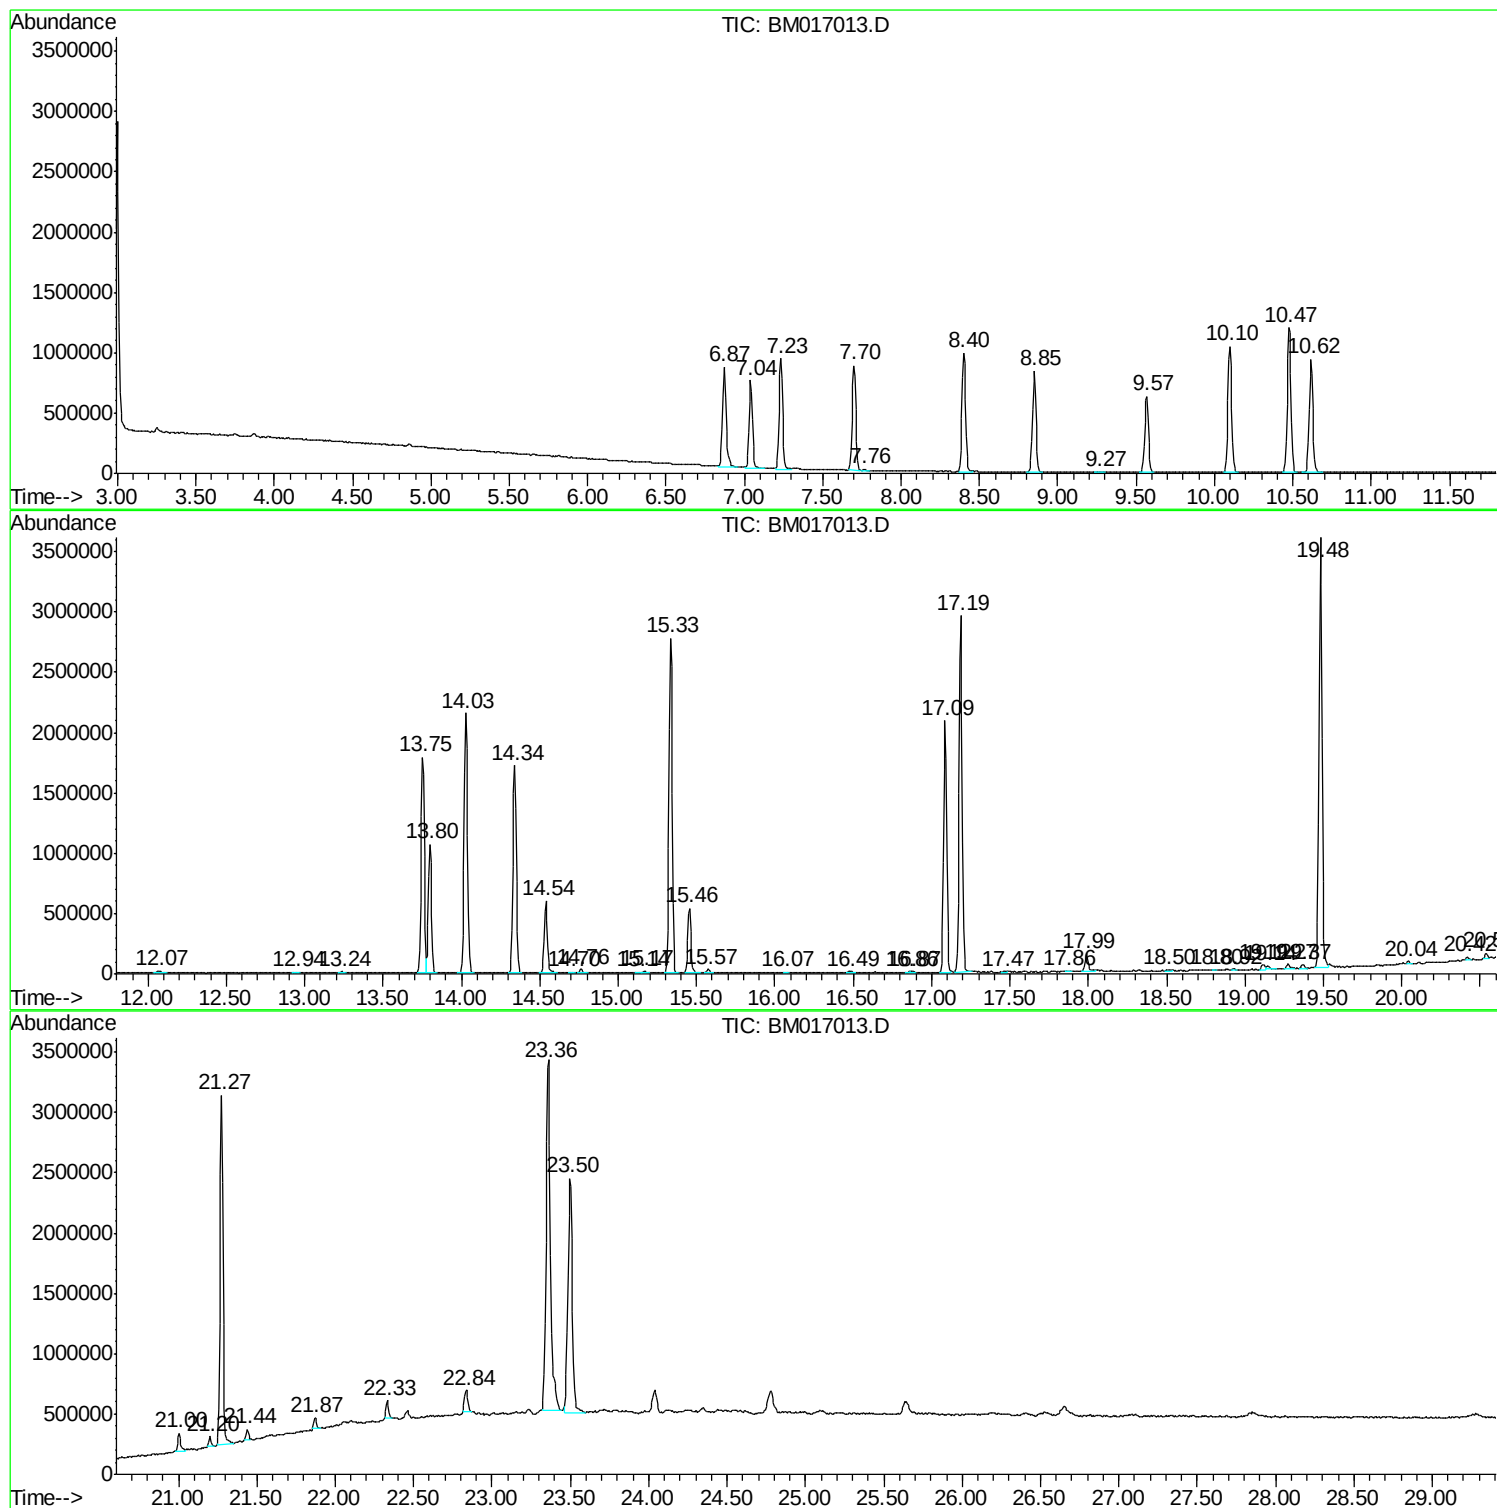

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100418\
Data File : BM017013.D
Acq On : 04 Oct 2018 23:13
Operator : MJ/SJ
Sample : J5157-09
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100418\
Data File : BM017013.D
Acq On : 04 Oct 2018 23:13
Operator : MJ/SJ
Sample : J5157-09
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM100418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc