

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100421\
 Data File : BM032318.D
 Acq On : 04 Oct 2021 10:28
 Operator : CG/JU
 Sample : PB139114BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB139114BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM032318.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.713	314	319	327	rBV	315825	425014	2.59%	0.545%
2	5.213	397	404	417	rBV	6217763	8843229	53.89%	11.342%
3	6.831	671	679	691	rBV	5441332	8962568	54.62%	11.495%
4	7.637	808	816	823	rBV	1020093	1513164	9.22%	1.941%
5	8.795	1005	1013	1022	rBV	3682918	5760708	35.11%	7.388%
6	10.430	1282	1291	1301	rBV	1320238	2080188	12.68%	2.668%
7	12.907	1704	1712	1718	rBV	8173396	12498746	76.17%	16.030%
8	14.283	1940	1946	1953	rBV	1977974	2670076	16.27%	3.424%
9	15.771	2192	2199	2214	rBV	6288053	9071423	55.28%	11.634%
10	17.012	2403	2410	2421	rBV	2356882	3213138	19.58%	4.121%
11	19.630	2849	2855	2860	rBV	11904012	16408991	100.00%	21.045%
12	20.383	2979	2983	2987	rBV	215173	247086	1.51%	0.317%
13	21.171	3113	3117	3124	rBV	2627162	3286854	20.03%	4.216%
14	23.330	3478	3484	3494	rBV	1751625	2989392	18.22%	3.834%




Sum of corrected areas: 77970577

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100421\
Data File : BM032318.D
Acq On : 04 Oct 2021 10:28
Operator : CG/JU
Sample : PB139114BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB139114BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

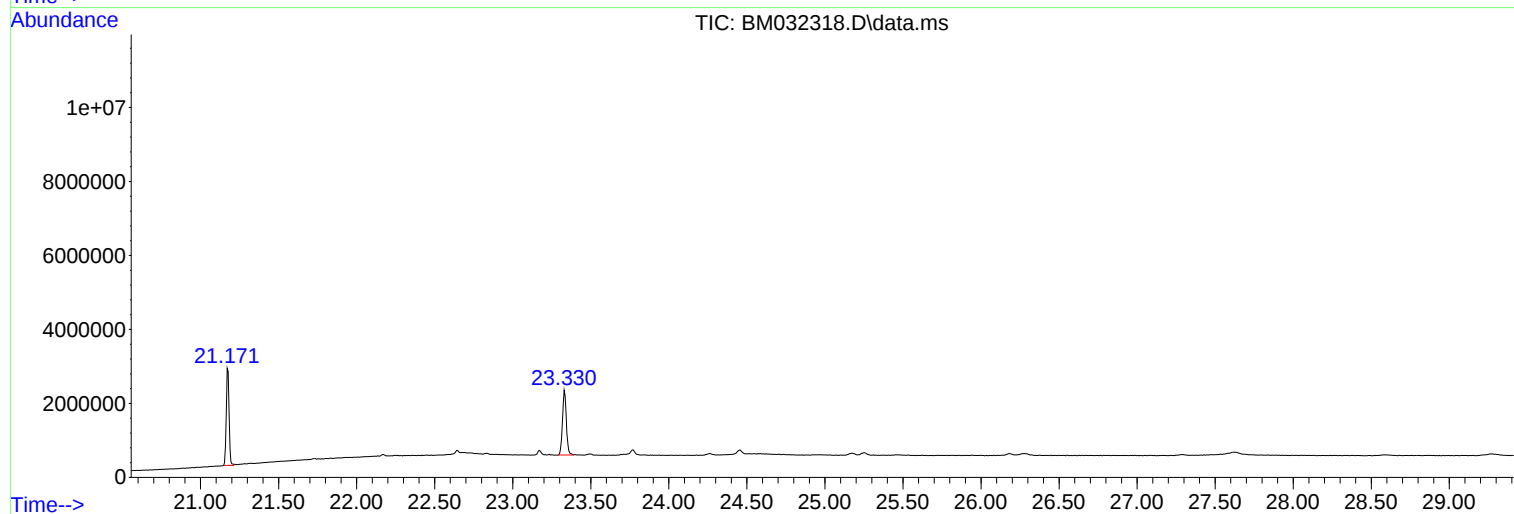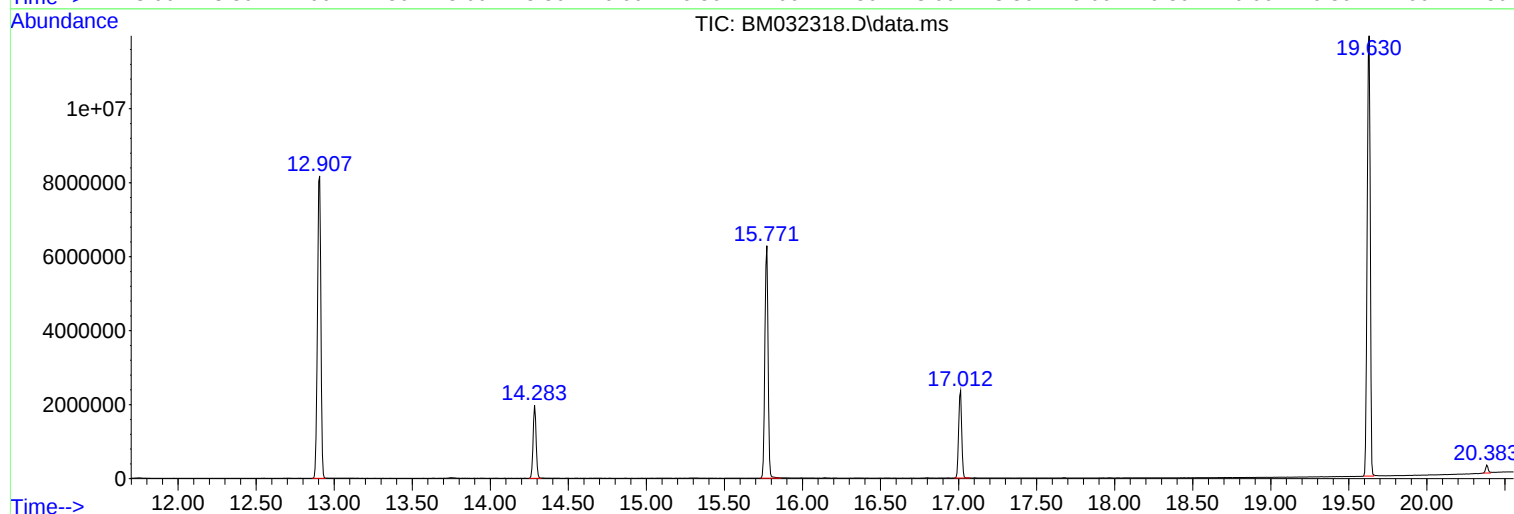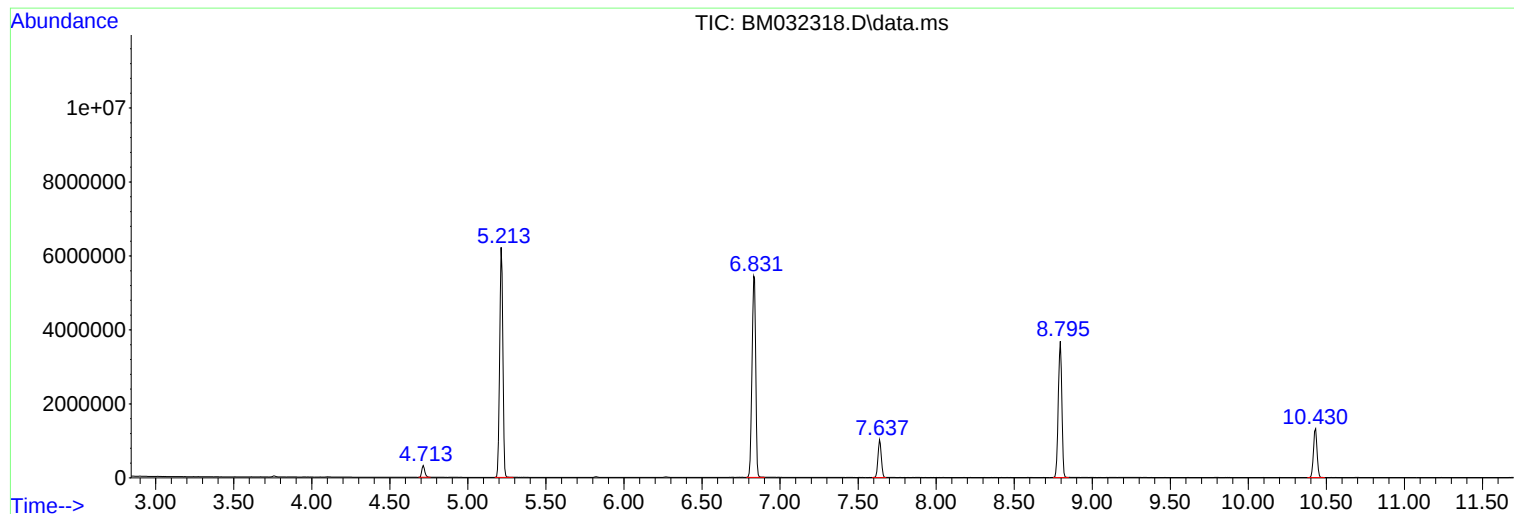

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100421\
Data File : BM032318.D
Acq On : 04 Oct 2021 10:28
Operator : CG/JU
Sample : PB139114BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB139114BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.713	5.62 ng	425014	1,4-Dichlorobenzene-d4	7.637

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	Succinic acid, heptyl 2-methoxye...	274	C14H26O5	1000325-80-7	33		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	5-Hexen-2-one	98	C6H10O	000109-49-9	9		

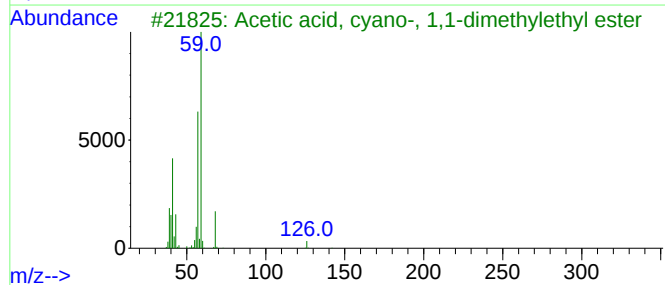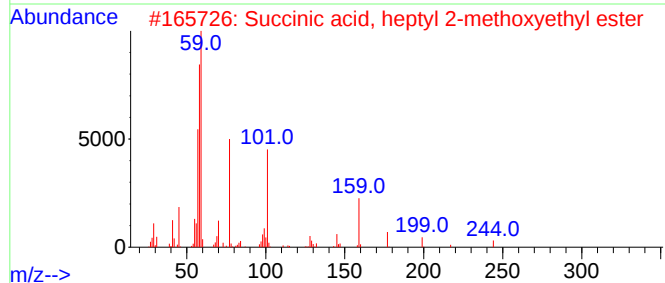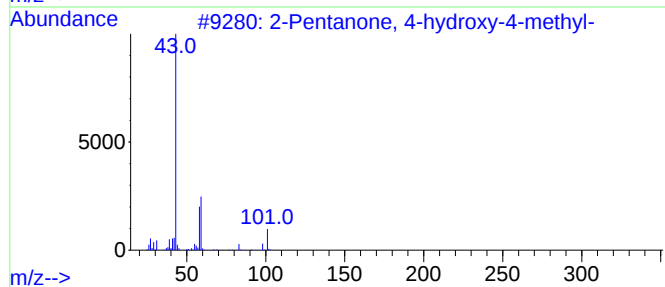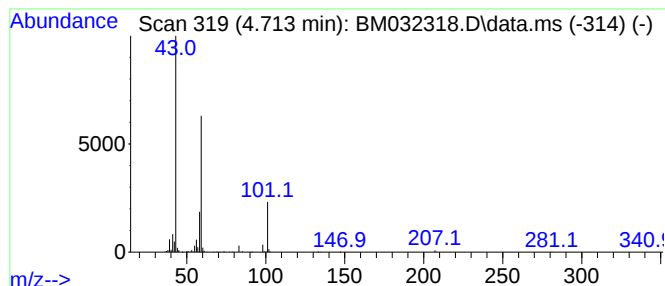

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100421\
Data File : BM032318.D
Acq On : 04 Oct 2021 10:28
Operator : CG/JU
Sample : PB139114BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB139114BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.713	5.6	ng	425014	1	7.637	1513160	20.0