


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100421\
 Data File : BM032316.D
 Acq On : 04 Oct 2021 09:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 01 18:34:58 2021

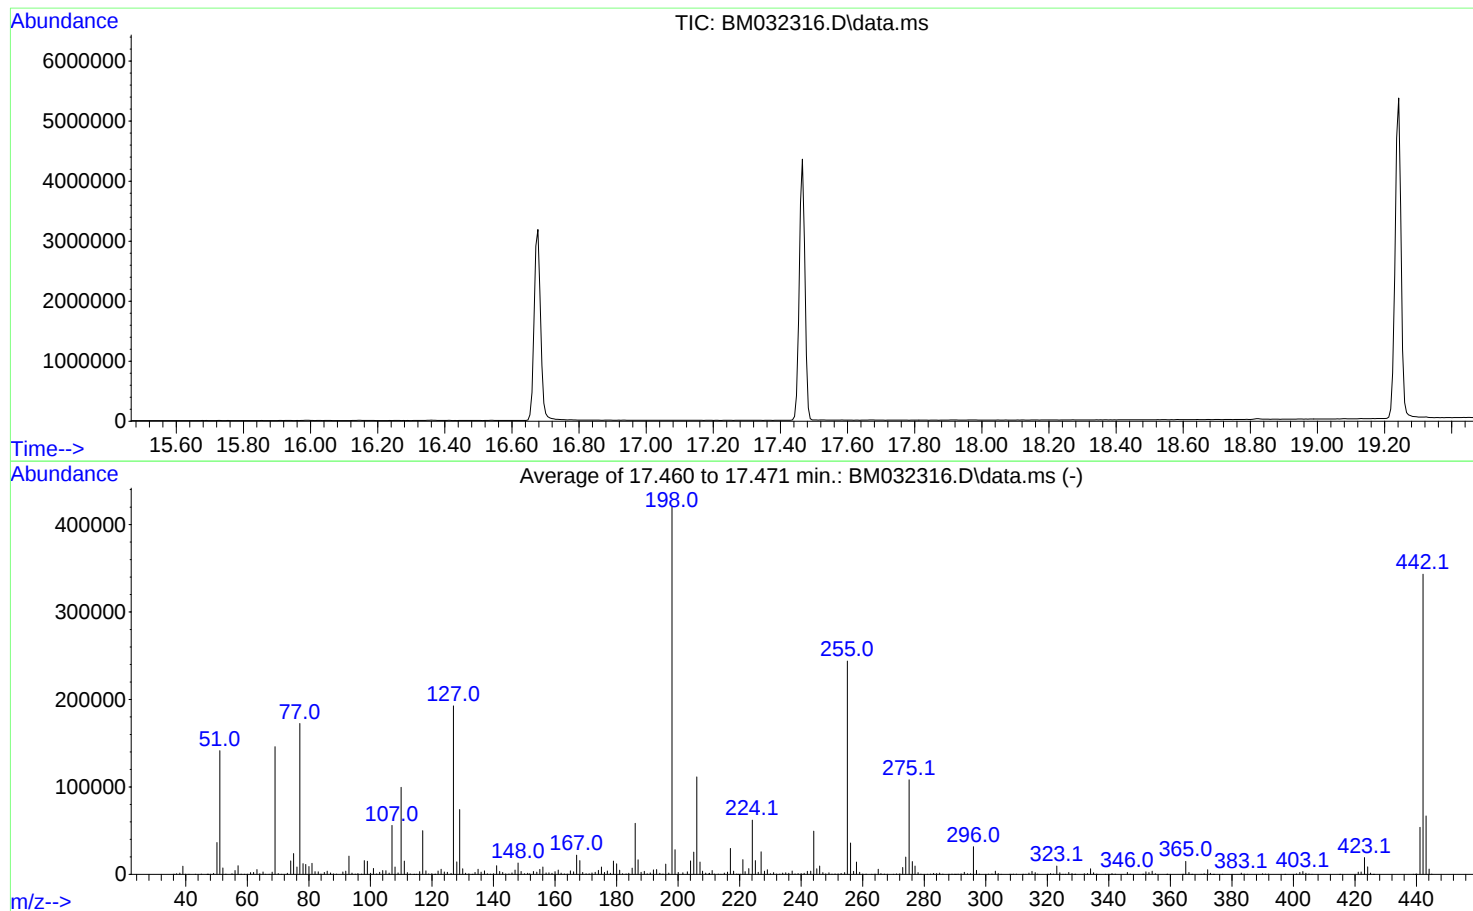




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	141411	PASS
68	69	0.00	2	1.8	2653	PASS
69	198	0.00	100	34.7	146051	PASS
70	69	0.00	2	0.6	833	PASS
127	198	10	80	45.8	192619	PASS
197	198	0.00	2	0.4	1526	PASS
198	198	100	100	100.0	420672	PASS
199	198	5	9	6.7	28248	PASS
275	198	10	60	25.7	108213	PASS
365	198	1	100	3.5	14839	PASS
441	198	0.01	100	12.8	53816	PASS
442	442	50	100	100.0	343253	PASS
443	442	15	24	19.5	66805	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100421\
Data File : BM032316.D
Acq On : 04 Oct 2021 09:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 04 10:57:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 01 18:34:58 2021
Response via : Initial Calibration

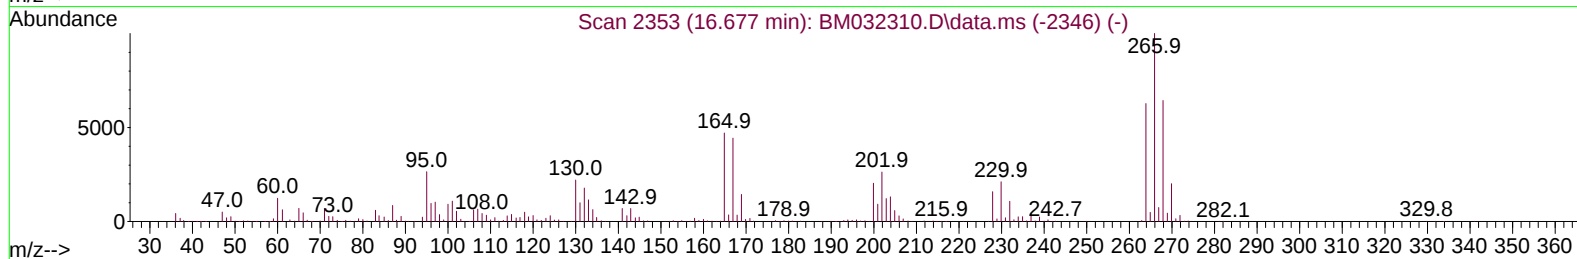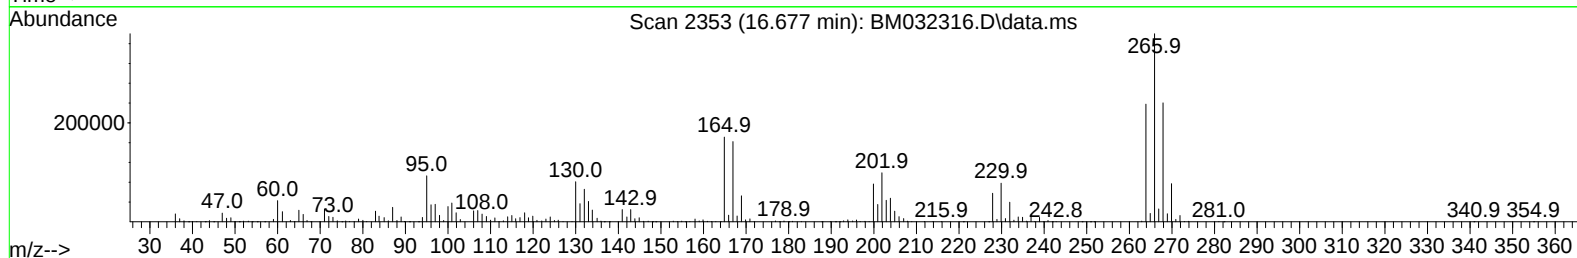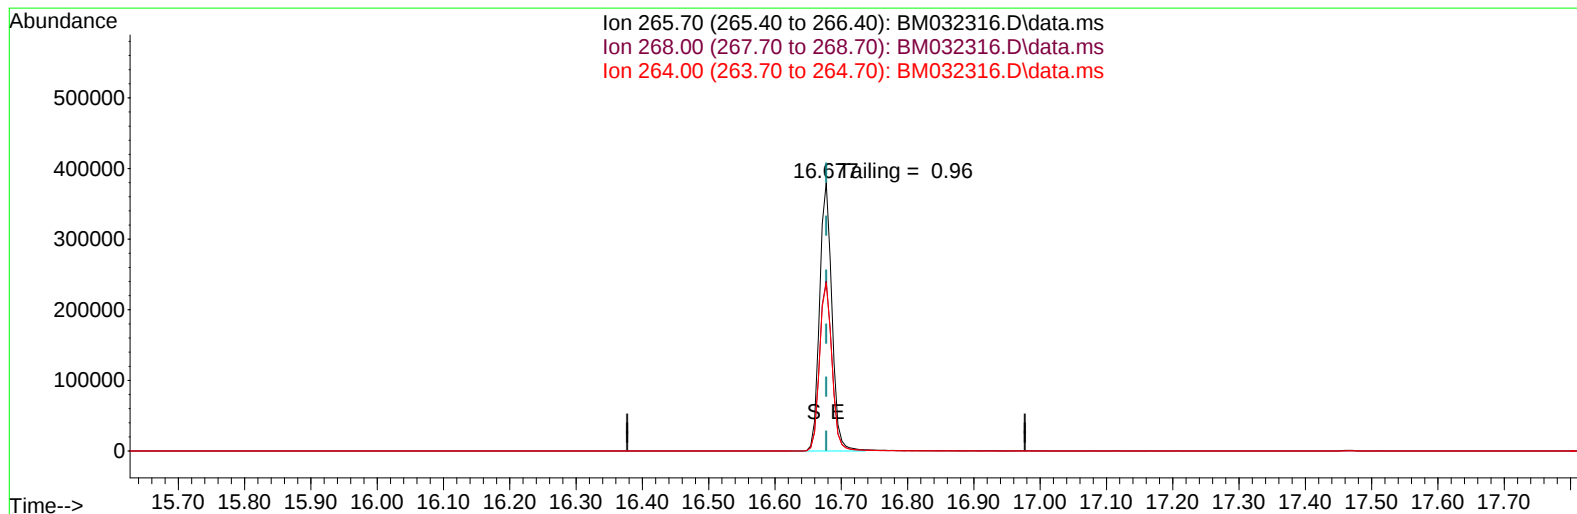

TIC: BM032316.D\data.ms

(70) Pentachlorophenol (C)

16.677min (+ 0.000) 0.00 ng




response 493174

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.24
264.00	65.10	62.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100421\
Data File : BM032316.D
Acq On : 04 Oct 2021 09:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 04 10:57:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 01 18:34:58 2021
Response via : Initial Calibration

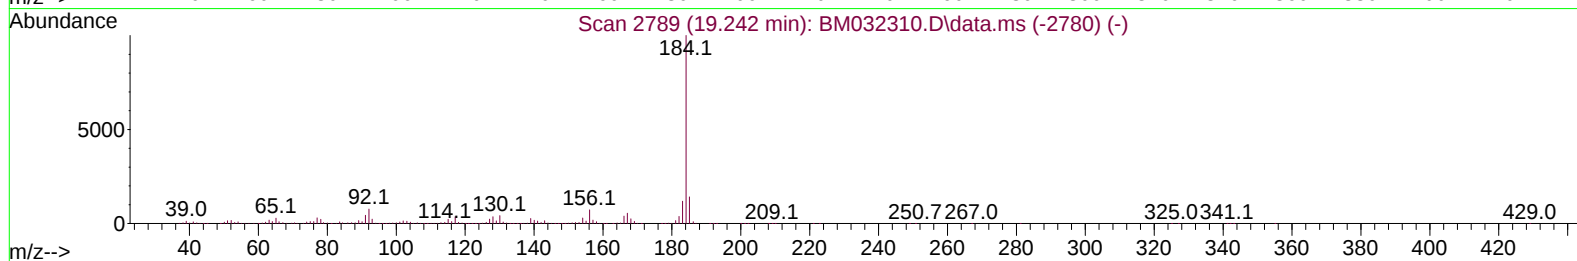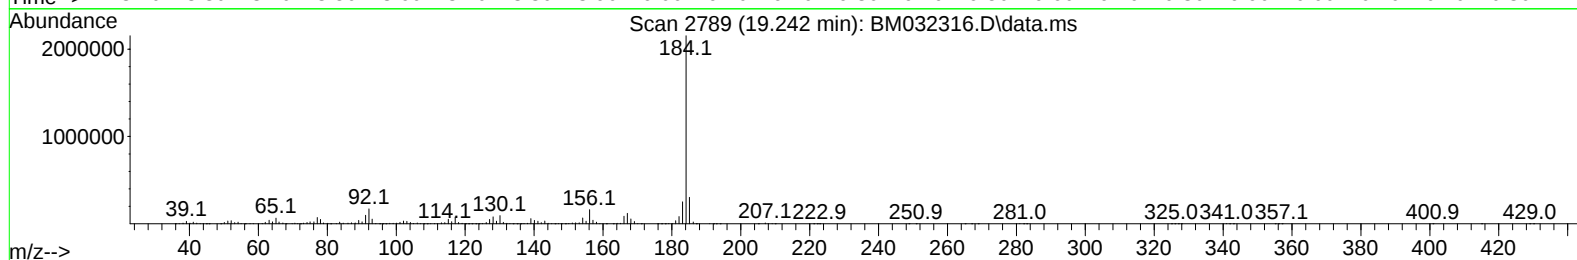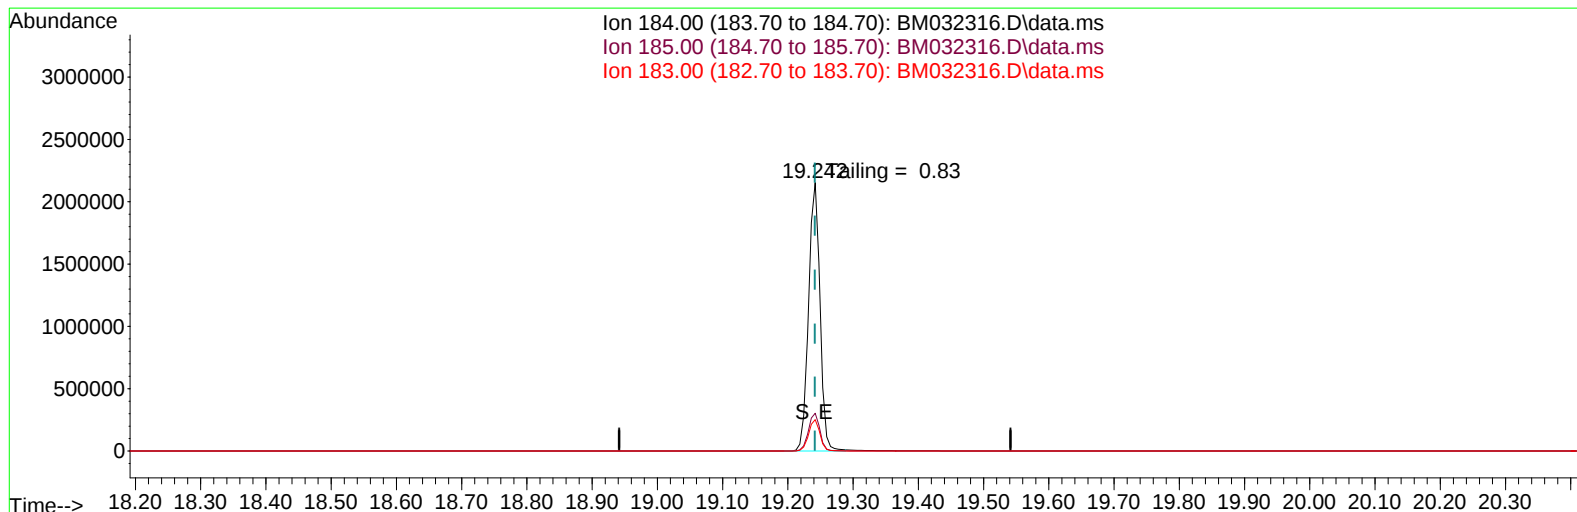

TIC: BM032316.D\data.ms

(77) Benzidine

19.242min (+ 0.000) 0.00 ng

response 2665106

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.08
183.00	11.20	11.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/4/2021	BNA_M	<u>BM032316.D</u>
Compound Name	Response	Retention Time
DDT	1324670	20.47
DDD	15629	20.04
DDE	2096	19.53
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17725	1342395	1.32

Instrument :
BNA_M
ClientSampleId :
DFTPP