


Data Path : Z:\HPCHEM1\BNA M\DATA\BM100515\
 Data File : BM002844.D
 Acq On : 05 Oct 2015 09:23
 Operator : UM/IZ
 Sample : DFTPP20
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP20

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM100515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 05 19:04:11 2015

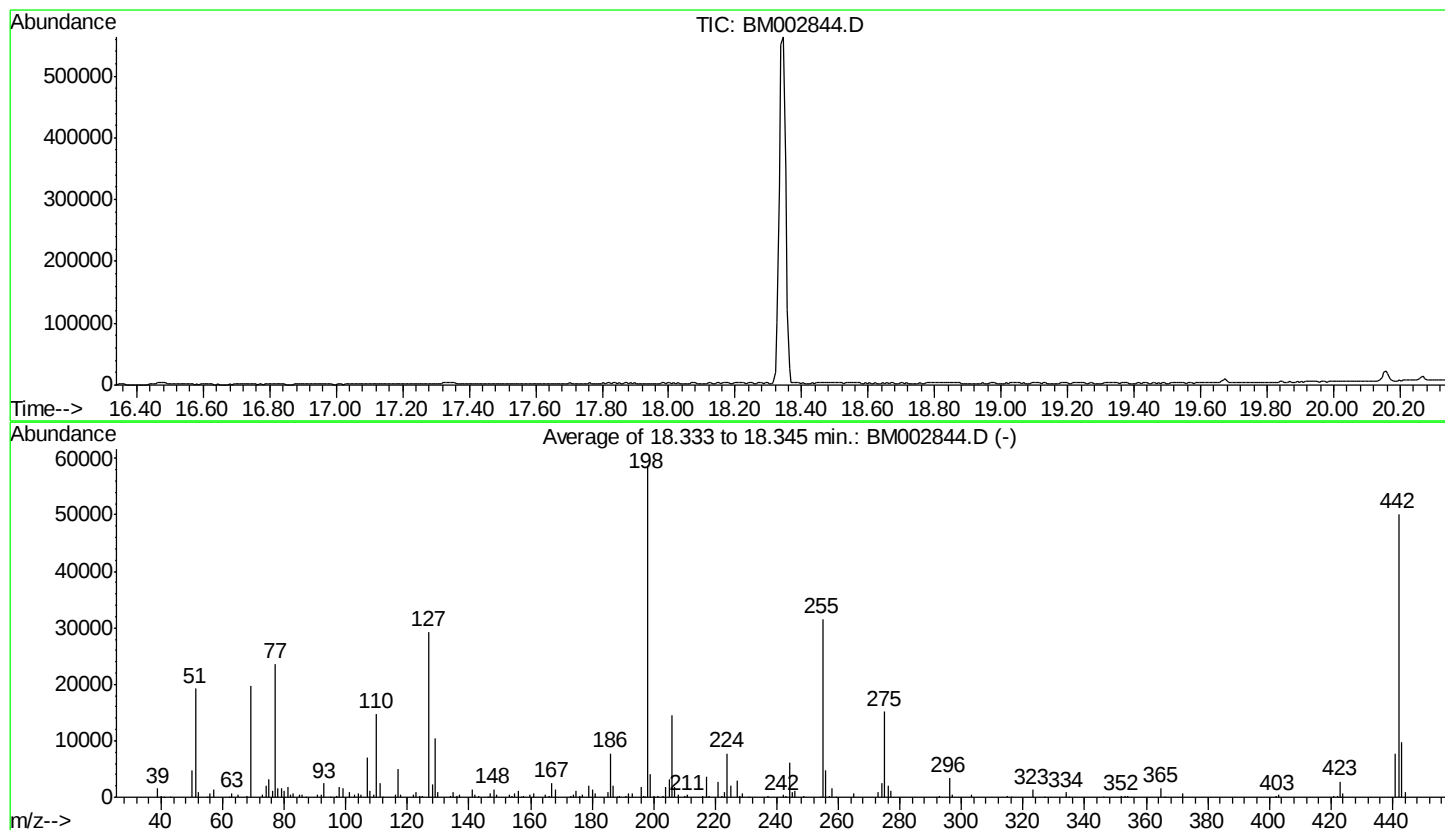

AutoFind: Scans 2592, 2593, 2594; Background Corrected with Scan 2586

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	19174	PASS
68	69	0.00	2	1.5	299	PASS
69	198	0.00	100	33.7	19803	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.9	29304	PASS
197	198	0.00	1	0.2	123	PASS
198	198	100	100	100.0	58730	PASS
199	198	5	9	6.9	4062	PASS
275	198	10	60	25.7	15113	PASS
365	198	1	100	2.8	1620	PASS
441	443	0.01	100	78.9	7739	PASS
442	198	50	100	85.5	50208	PASS
443	442	15	24	19.5	9805	PASS

Scan 2586 (18.298 min): BM002844.D
DFTPP20

m/z	Abundance
41.00	333.0
43.00	316.0
44.00	976.0
55.00	413.0
57.10	300.0
69.10	377.0
95.00	351.0
206.90	437.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

m/z	Abundance
39.00	1262.0
41.00	330.0
43.00	312.0
43.90	885.0
50.00	3697.0
51.10	15059.0
52.00	779.0
55.10	427.0
56.00	538.0
57.00	1338.0
63.00	604.0
65.00	347.0
69.00	16262.0
73.10	313.0
74.00	1622.0
75.00	2383.0
76.10	785.0
77.10	18024.0
78.00	1338.0
79.00	1249.0
79.90	812.0
81.00	1377.0
82.00	475.0
83.00	636.0
85.00	356.0
86.00	362.0
90.90	414.0
92.00	349.0
93.00	2006.0
95.00	376.0
97.00	325.0
98.00	1326.0
99.00	1291.0
101.00	650.0
102.90	360.0
103.90	459.0
105.00	388.0
107.00	5408.0
108.00	1018.0
109.00	325.0
110.00	11341.0
111.00	1927.0
115.90	307.0
117.00	3734.0
118.00	317.0
121.90	425.0
122.90	720.0
127.00	21528.0
128.00	1692.0
129.00	7487.0
130.00	761.0
135.00	772.0
137.10	431.0
141.00	1011.0
142.00	315.0
147.00	568.0
148.00	928.0
149.00	339.0
152.90	303.0
155.00	583.0
156.00	801.0
160.00	365.0
161.00	472.0
164.90	424.0
167.00	1852.0
168.00	1135.0
174.00	403.0
174.90	704.0
177.00	353.0
178.90	1504.0
180.00	1104.0
181.00	519.0
185.00	691.0
186.00	5247.0
187.00	1446.0
191.90	374.0
193.00	449.0
196.00	1068.0
198.00	39464.0
198.90	2931.0
204.00	1238.0
205.00	2187.0
206.00	9663.0
207.00	1724.0
208.00	441.0
211.10	438.0
217.00	2501.0
221.00	1794.0
223.00	477.0
224.00	5217.0
225.00	1330.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

227.00	1994.0
229.00	386.0
241.90	302.0
244.00	3882.0
245.10	580.0
246.00	765.0
255.00	20160.0
256.00	3148.0
258.00	1017.0
265.00	377.0
272.90	536.0
274.00	1560.0
275.00	9780.0
276.00	1295.0
277.00	755.0
296.00	2223.0
296.90	324.0
303.00	323.0
323.00	722.0
334.00	439.0
364.90	788.0
372.00	396.0
423.00	1427.0
424.00	412.0
441.00	3848.0
442.00	25408.0
443.00	4902.0
444.00	642.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

m/z	Abundance
39.00	1883.0
39.90	368.0
41.00	368.0
43.10	337.0
44.00	808.0
50.00	5408.0
51.10	22704.0
52.00	1103.0
55.00	438.0
56.00	843.0
57.00	2011.0
63.00	817.0
65.00	499.0
68.10	490.0
69.00	23240.0
73.00	422.0
74.00	2134.0
75.00	3841.0
76.00	1219.0
77.10	27408.0
78.10	1858.0
79.00	1754.0
80.00	1237.0
81.00	2051.0
82.00	626.0
83.00	690.0
85.00	551.0
86.00	562.0
86.90	310.0
90.90	505.0
92.00	474.0
93.00	2733.0
95.10	402.0
97.10	318.0
98.00	2052.0
99.00	1708.0
101.00	1182.0
102.90	370.0
104.00	659.0
105.00	658.0
107.00	8484.0
108.00	1408.0
109.10	499.0
110.00	17080.0
111.00	2943.0
112.00	318.0
116.00	500.0
117.00	5622.0
118.00	511.0
122.00	590.0
123.00	1035.0
123.90	462.0
125.00	433.0
127.00	33824.0
128.00	2716.0
129.00	12143.0
130.00	1035.0
134.00	367.0
135.00	1112.0
135.90	419.0
137.00	547.0
141.00	1599.0
142.00	512.0
143.00	371.0
145.90	312.0
146.90	859.0
148.00	1691.0
148.90	459.0
153.00	593.0
153.90	322.0
155.00	815.0
156.00	1221.0
157.00	314.0
157.90	308.0
159.90	380.0
161.00	735.0
164.90	646.0
166.00	487.0
167.00	2901.0
168.00	1600.0
173.00	376.0
174.00	636.0
175.00	1213.0
176.10	333.0
177.00	678.0
179.00	2320.0
180.00	1688.0
180.90	666.0
185.00	1152.0
186.00	9085.0
187.00	2478.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

188.00	355.0
188.90	477.0
191.00	315.0
192.00	738.0
193.00	809.0
196.00	2165.0
196.90	369.0
198.00	68512.0
198.90	4443.0
200.00	339.0
201.40	342.0
202.90	424.0
204.00	2146.0
205.00	3718.0
206.00	16632.0
207.00	2693.0
208.00	519.0
210.20	333.0
210.80	613.0
215.90	307.0
217.00	4160.0
218.00	454.0
221.00	3292.0
222.00	543.0
223.10	1017.0
224.00	8715.0
225.00	2388.0
227.00	3209.0
228.00	542.0
229.00	714.0
231.00	308.0
237.00	330.0
241.90	438.0
243.00	437.0
244.00	7109.0
245.00	879.0
246.00	1205.0
249.00	301.0
255.00	36240.0
256.00	5535.0
256.90	382.0
258.00	1755.0
265.00	704.0
273.00	1219.0
274.00	2894.0
275.00	16888.0
276.00	2275.0
277.00	1362.0
293.00	317.0
296.00	3770.0
297.00	627.0
303.00	640.0
314.90	391.0
316.00	318.0
323.00	1585.0
334.00	942.0
352.00	501.0
354.00	423.0
365.00	1957.0
372.00	769.0
402.00	334.0
403.00	568.0
420.90	366.0
422.00	394.0
423.00	3107.0
424.00	746.0
441.00	8785.0
442.00	55320.0
443.00	11031.0
444.00	1031.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

m/z	Abundance
39.00	1550.0
40.00	390.0
41.10	352.0
43.00	305.0
44.00	798.0
50.00	5003.0
51.10	19760.0
52.00	1142.0
55.00	483.0
56.00	680.0
57.00	1683.0
62.00	302.0
63.00	861.0
65.00	479.0
68.00	407.0
69.00	21040.0
73.00	409.0
74.00	2086.0
75.00	3207.0
76.00	1098.0
77.10	25360.0
78.00	1843.0
79.00	1593.0
80.00	1277.0
81.00	2015.0
82.00	556.0
83.00	616.0
85.00	434.0
85.90	438.0
91.00	541.0
92.00	534.0
93.00	2463.0
95.00	363.0
98.00	1924.0
99.00	1680.0
101.00	1145.0
102.90	344.0
104.00	620.0
105.00	582.0
107.00	7544.0
108.00	1263.0
109.10	515.0
110.00	15964.0
111.00	2551.0
116.00	460.0
117.00	5340.0
117.90	396.0
122.00	544.0
123.00	961.0
124.00	384.0
125.00	387.0
127.00	32560.0
128.00	2311.0
129.00	11672.0
130.00	946.0
133.90	357.0
135.00	1131.0
135.90	471.0
137.10	604.0
141.00	1427.0
142.00	570.0
143.00	365.0
147.00	792.0
148.00	1691.0
148.90	409.0
153.00	509.0
154.00	409.0
155.00	849.0
156.00	1330.0
157.90	320.0
159.90	488.0
161.00	673.0
165.00	585.0
166.00	432.0
167.00	2792.0
168.00	1379.0
173.00	443.0
173.90	650.0
175.00	1215.0
176.00	345.0
176.90	673.0
179.00	1994.0
180.00	1596.0
181.00	745.0
185.00	1132.0
186.00	8933.0
187.00	2405.0
188.90	560.0
191.00	383.0
191.90	681.0
193.00	841.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

196.00	2178.0
197.10	337.0
198.00	68216.0
199.00	4813.0
199.90	351.0
201.30	350.0
201.50	351.0
202.90	407.0
204.00	2167.0
205.00	3831.0
206.00	17256.0
207.00	2614.0
208.00	629.0
210.30	308.0
211.00	658.0
216.00	374.0
217.00	3987.0
218.00	544.0
221.00	3251.0
223.00	923.0
224.00	9403.0
225.00	2391.0
227.00	3397.0
227.90	451.0
228.90	837.0
237.00	306.0
242.00	448.0
243.00	505.0
244.00	7230.0
245.00	959.0
245.90	1288.0
248.90	306.0
254.10	317.0
255.00	38216.0
256.00	5950.0
257.00	537.0
258.00	1842.0
259.00	362.0
265.00	782.0
273.00	1162.0
274.00	3232.0
275.00	18672.0
276.00	2601.0
277.00	1390.0
292.90	346.0
296.00	4347.0
297.00	646.0
303.10	586.0
315.00	495.0
323.00	1567.0
327.00	333.0
334.10	1162.0
335.00	307.0
345.90	325.0
352.00	450.0
353.00	373.0
354.00	547.0
365.00	2115.0
365.90	339.0
372.00	964.0
402.00	378.0
403.00	589.0
420.90	631.0
422.00	496.0
423.00	3646.0
424.00	926.0
441.00	10585.0
442.00	69896.0
443.00	13484.0
444.00	1080.0

Instrument :

BNA_M

ClientSampleId :

DFTPP20