

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100520\
Quantitation Report (Not Reviewed)

Data File : BM027621.D
Acq On : 06 Oct 2020 00:38
Operator : JU/CG
Sample : L4184-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AM5

Quant Time: Oct 06 01:26:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 06 01:23:11 2020
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	1689	0.40	ng/ul	0.00
2) Naphthalene-d8	10.57	136	4835	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.42	164	3518	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.17
16) Chrysene-d12	21.34	240	9620	0.40	ng/ul	0.00
20) Perylene-d12	23.60	264	10389	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.17	152	2550	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.19	212	7661	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.56	202	3032	0.069	ng/ul#	1
23) Benzo(a)pyrene	23.46	252	3195	0.085	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM027621.D
Acq On : 06 Oct 2020 00:38
Operator : JU/CG
Sample : L4184-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AM5

Quant Time: Oct 06 01:26:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 06 01:23:11 2020
Response via : Initial Calibration




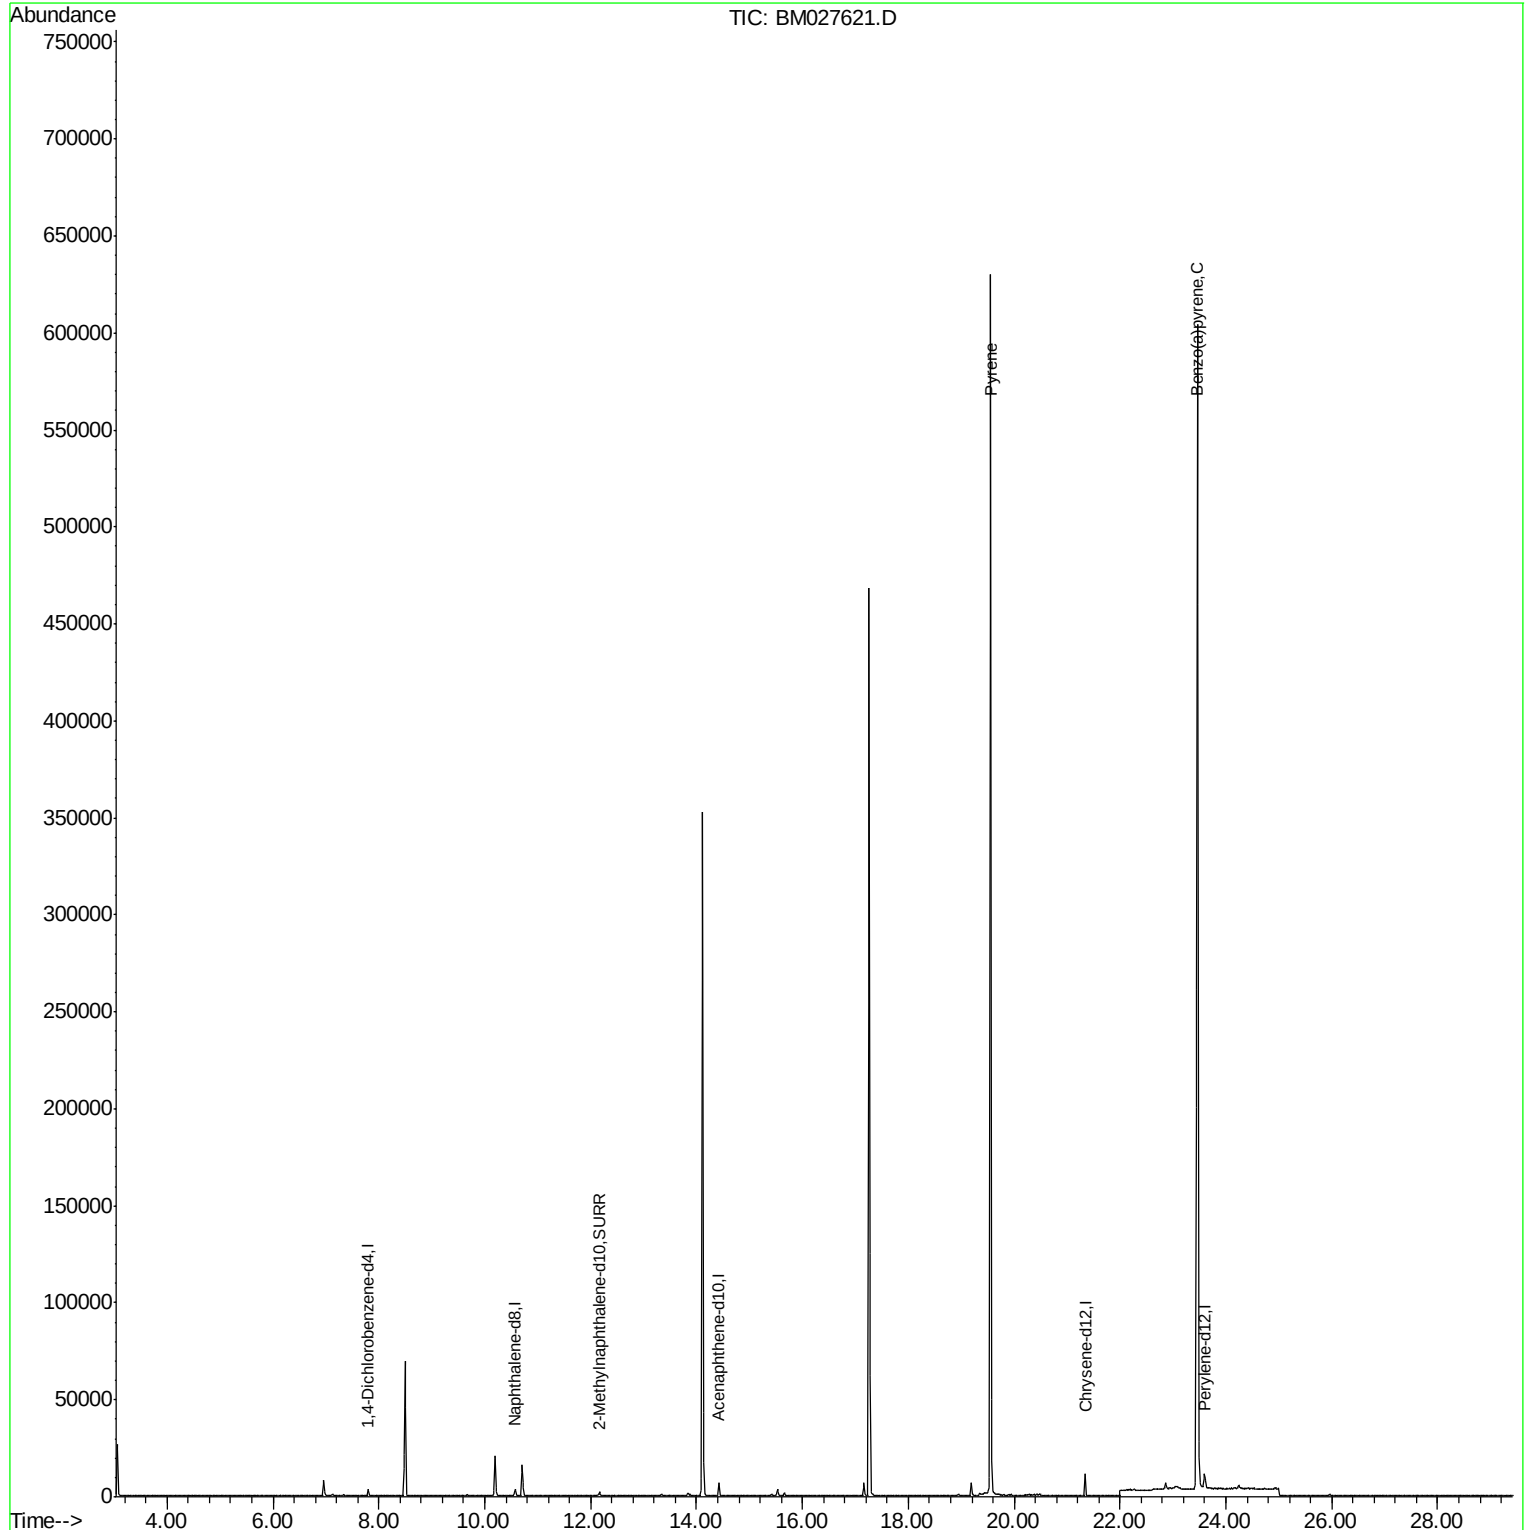


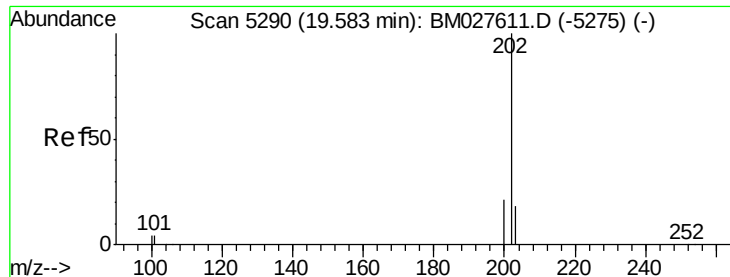

#17
Pyrene
Concen: 0.069 ng/ul
RT: 19.56 min Scan# 5283
Delta R.T. -0.03 min
Lab File: BM027621.D
Acq: 06 Oct 2020 00:38

Instrument :
BNA_M
ClientSampleId :
C0AM5

Tgt Ion:202 Resp: 3032
Ion Ratio Lower Upper
202 100
101 97.9 4.7 7.1#
100 702.7 3.9 5.9#

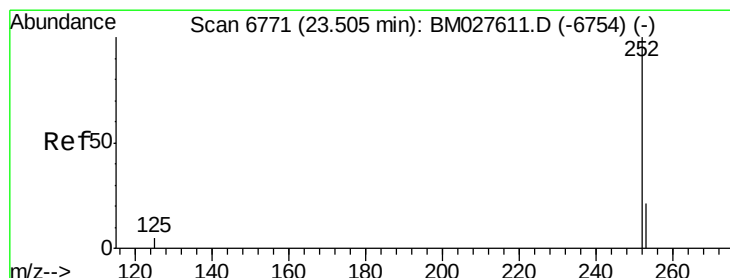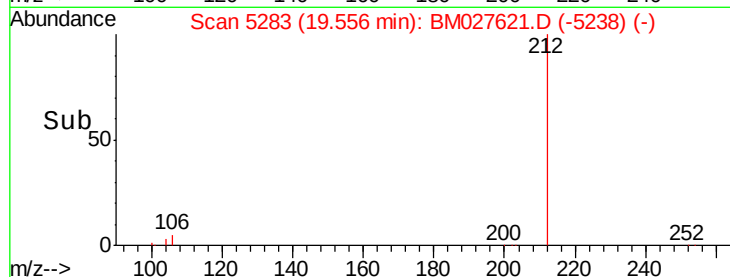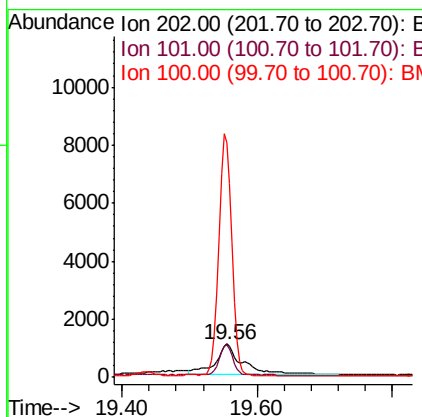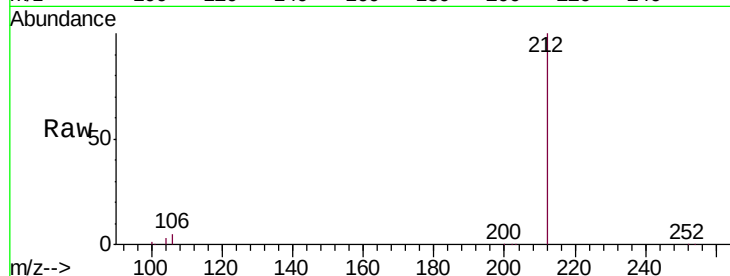

#23
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.46 min Scan# 6752
Delta R.T. -0.05 min
Lab File: BM027621.D
Acq: 06 Oct 2020 00:38

Tgt Ion:252 Resp: 3195
Ion Ratio Lower Upper
252 100
253 50.2 19.6 29.4#
125 25.8 5.0 7.6#

