


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100520\
Data File : BM027601.D
Acq On : 05 Oct 2020 11:51
Operator : JU/CG
Sample : L4185-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AR1

Manual Integrations
APPROVED

mohammad
10/6/2020 3:23:24 PM

Quant Time: Oct 05 12:23:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 10:43:07 2020
Response via : Initial Calibration

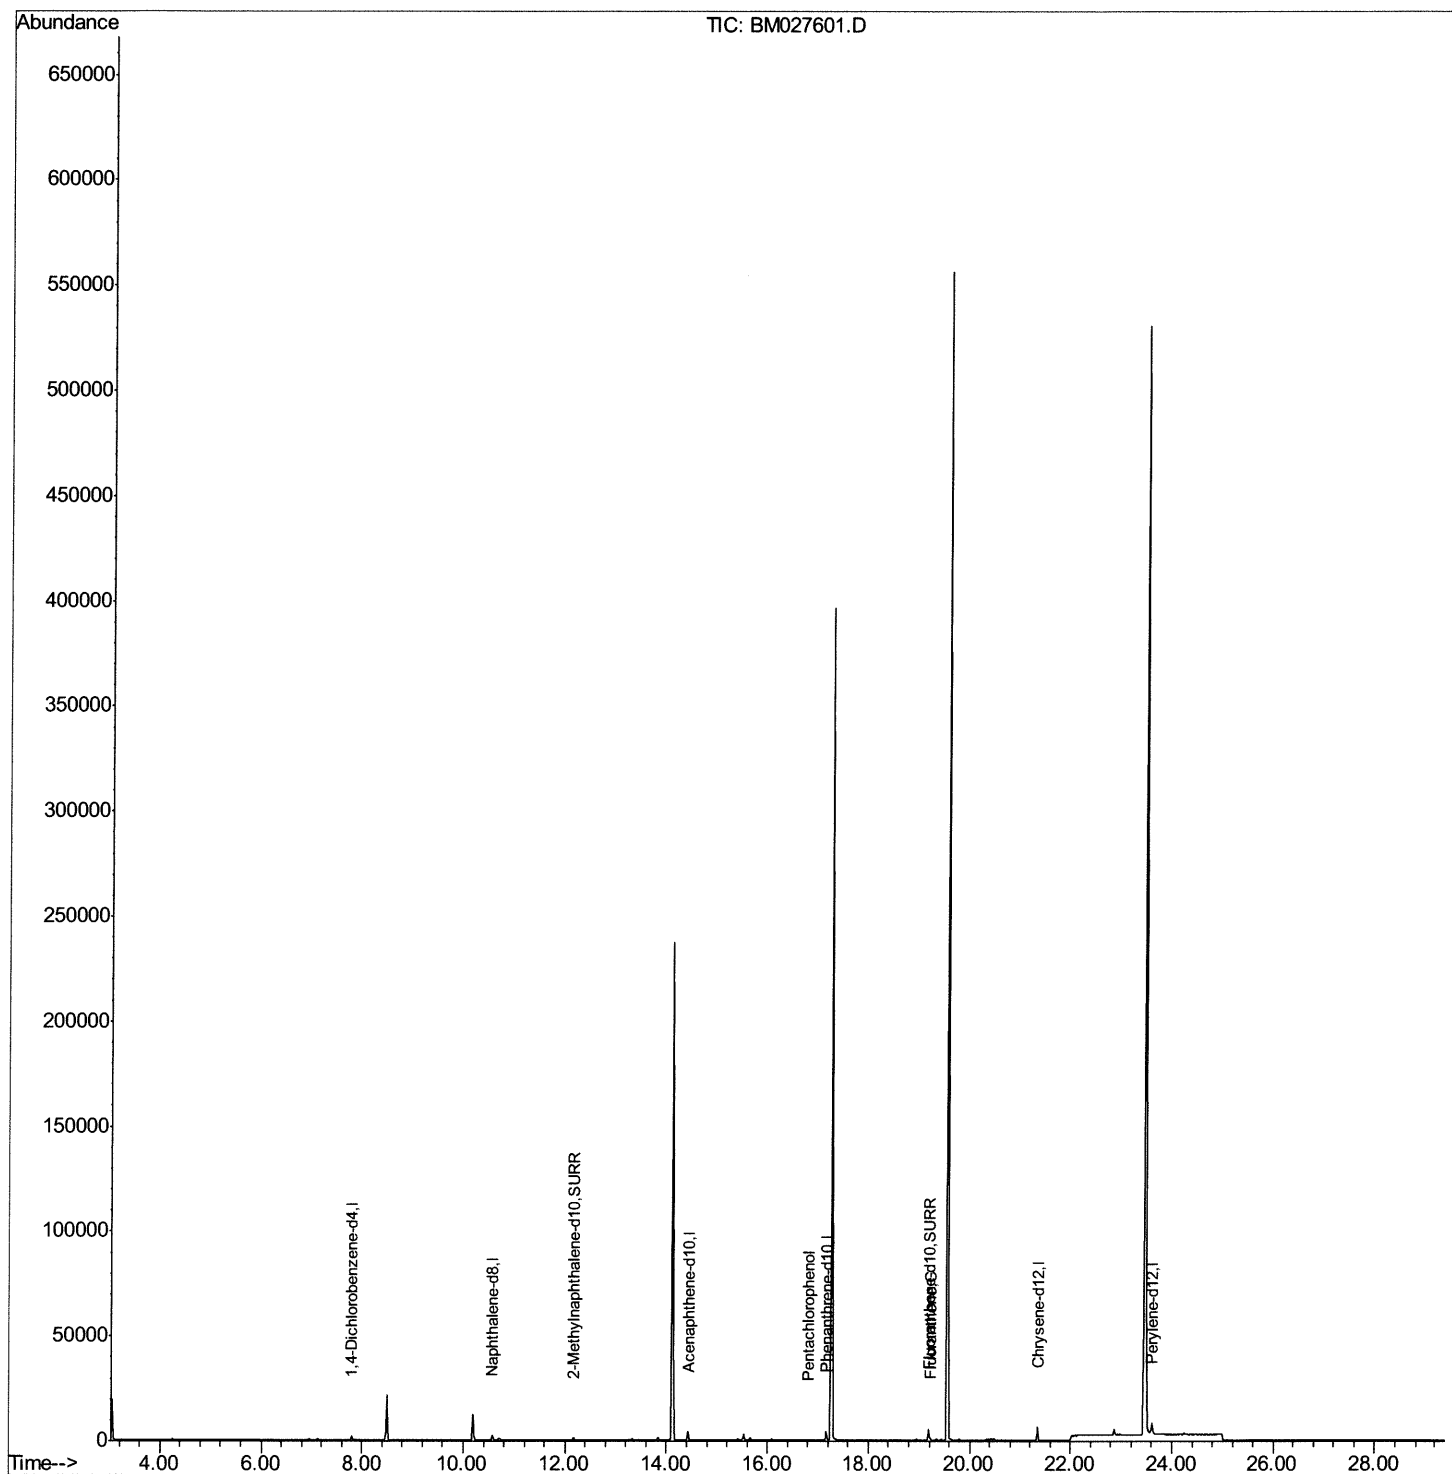

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100520\
 Data File : BM027601.D
 Acq On : 05 Oct 2020 11:51
 Operator : JU/CG
 Sample : L4185-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AR1

Manual Integrations
 APPROVED

mohammad
 10/6/2020 3:23:24 PM

Quant Time: Oct 05 12:22:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 05 10:43:07 2020
 Response via : Initial Calibration

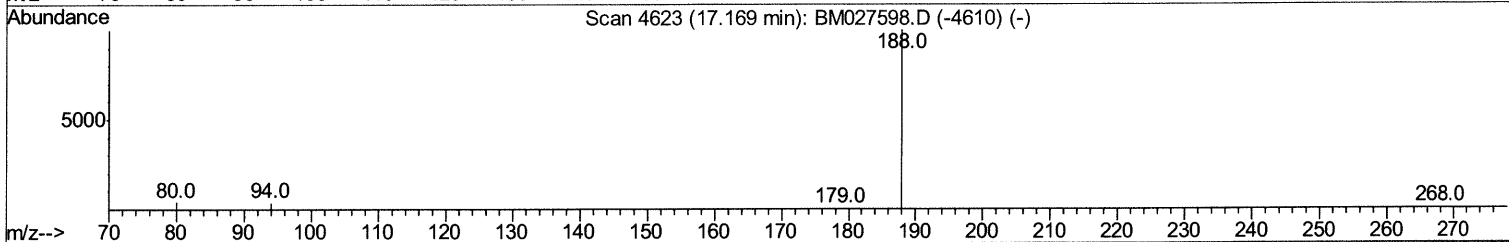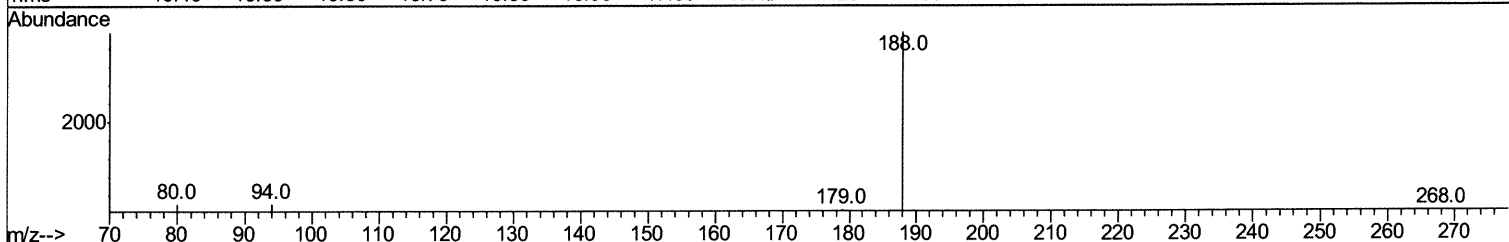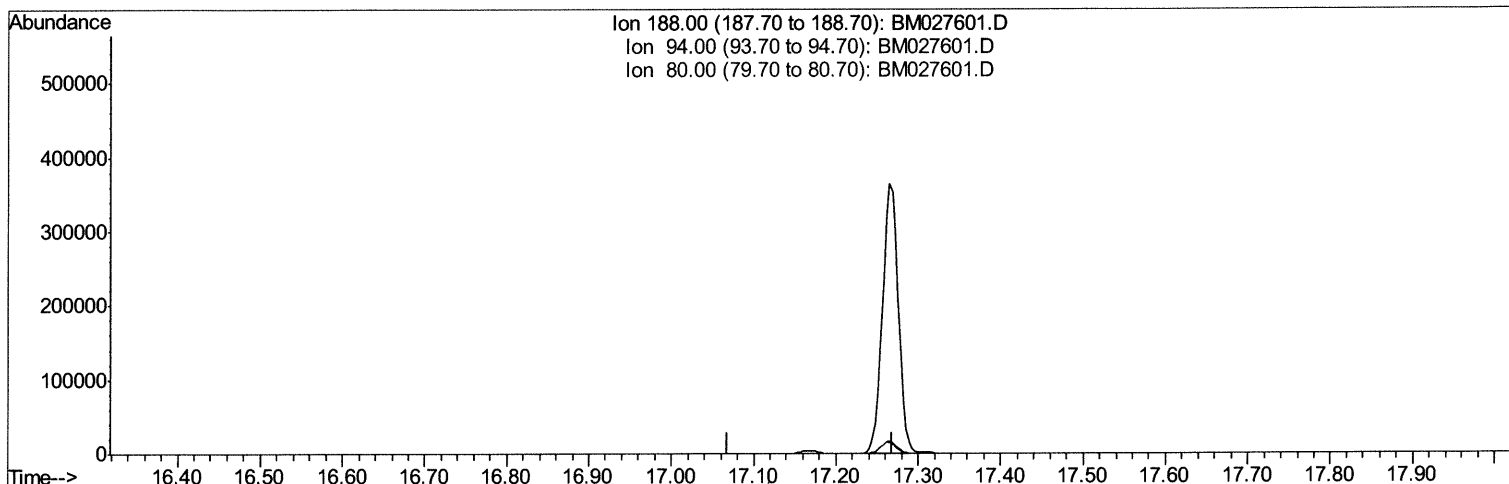

TIC: BM027601.D

(10) Phenanthrene-d10 (I)
 17.169min (-17.169) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	5.20	0.00#
80.00	6.20	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100520\
 Data File : BM027601.D
 Acq On : 05 Oct 2020 11:51
 Operator : JU/CG
 Sample : L4185-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 C0AR1

Manual Integrations
APPROVED

mohammad
 10/6/2020 3:23:24 PM

Quant Time: Oct 05 12:22:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 05 10:43:07 2020
 Response via : Initial Calibration

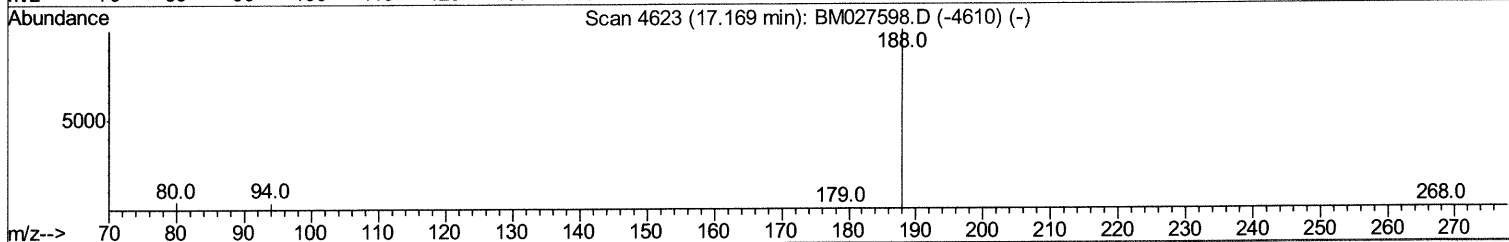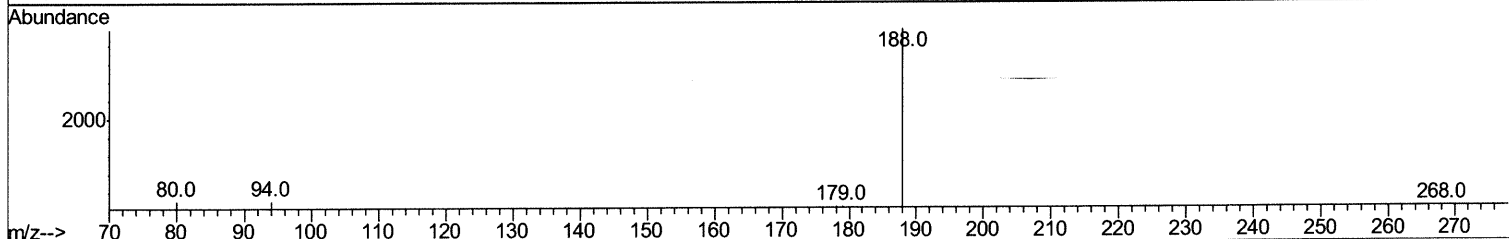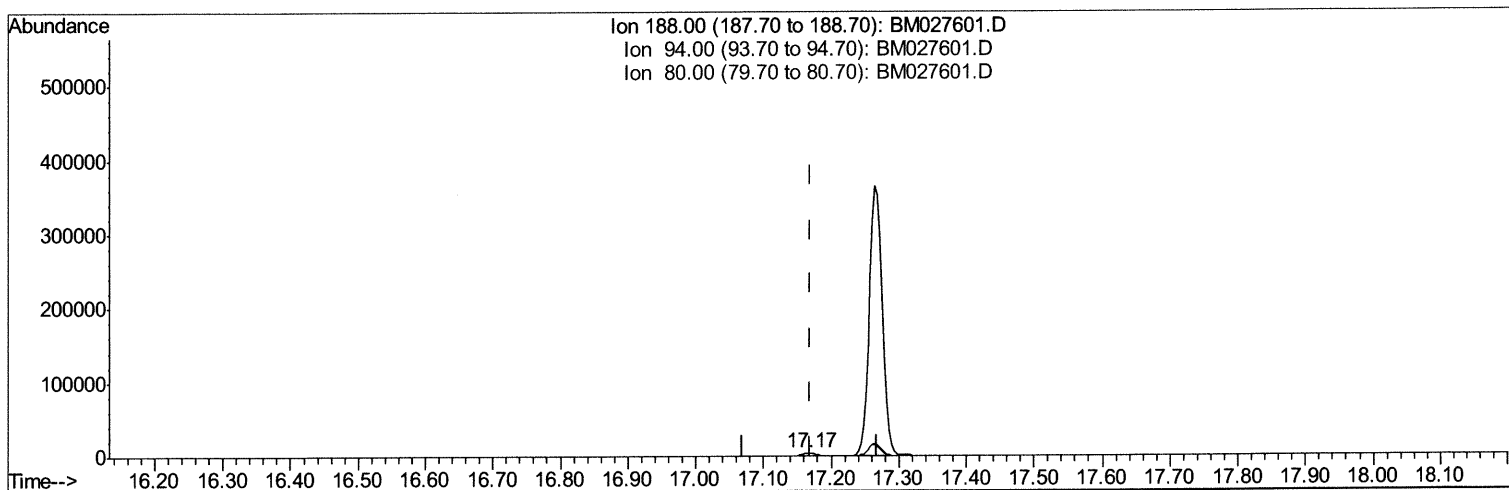

TIC: BM027601.D

(10) Phenanthrene-d10 (I)

17.168min (-0.002) 0.40ng/ul m 10/07/2020 JU

response 5445

Ion	Exp%	Act%
188.00	100	100
94.00	5.20	5.59
80.00	6.20	5.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100520\
 Data File : BM027601.D
 Acq On : 05 Oct 2020 11:51
 Operator : JU/CG
 Sample : L4185-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AR1

Manual Integrations
 APPROVED

mohammad
 10/6/2020 3:23:24 PM

Quant Time: Oct 05 12:23:41 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 05 10:43:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	990	0.40	ng/ul	0.00
2) Naphthalene-d8	10.58	136	2914	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.43	164	2203	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.17	188	5445m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.35	240	6045	0.40	ng/ul	0.00
20) Perylene-d12	23.61	264	6654	0.40	ng/ul	0.00

10/07/20 JU

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.17	152	1561	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.19	212	6469	0.43	ng/ul	0.00

Target Compounds

					Ovalue	
11) Pentachlorophenol	16.82	266	62	0.042	ng/ul#	78
15) Fluoranthene	19.22	202	703	0.035	ng/ul	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed