


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100520\
Data File : BM027603.D
Acq On : 05 Oct 2020 13:04
Operator : JU/CG
Sample : L4185-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AR6

Manual Integrations
APPROVED

mohammad
10/6/2020 3:23:29 PM

Quant Time: Oct 05 13:37:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 10:43:07 2020
Response via : Initial Calibration

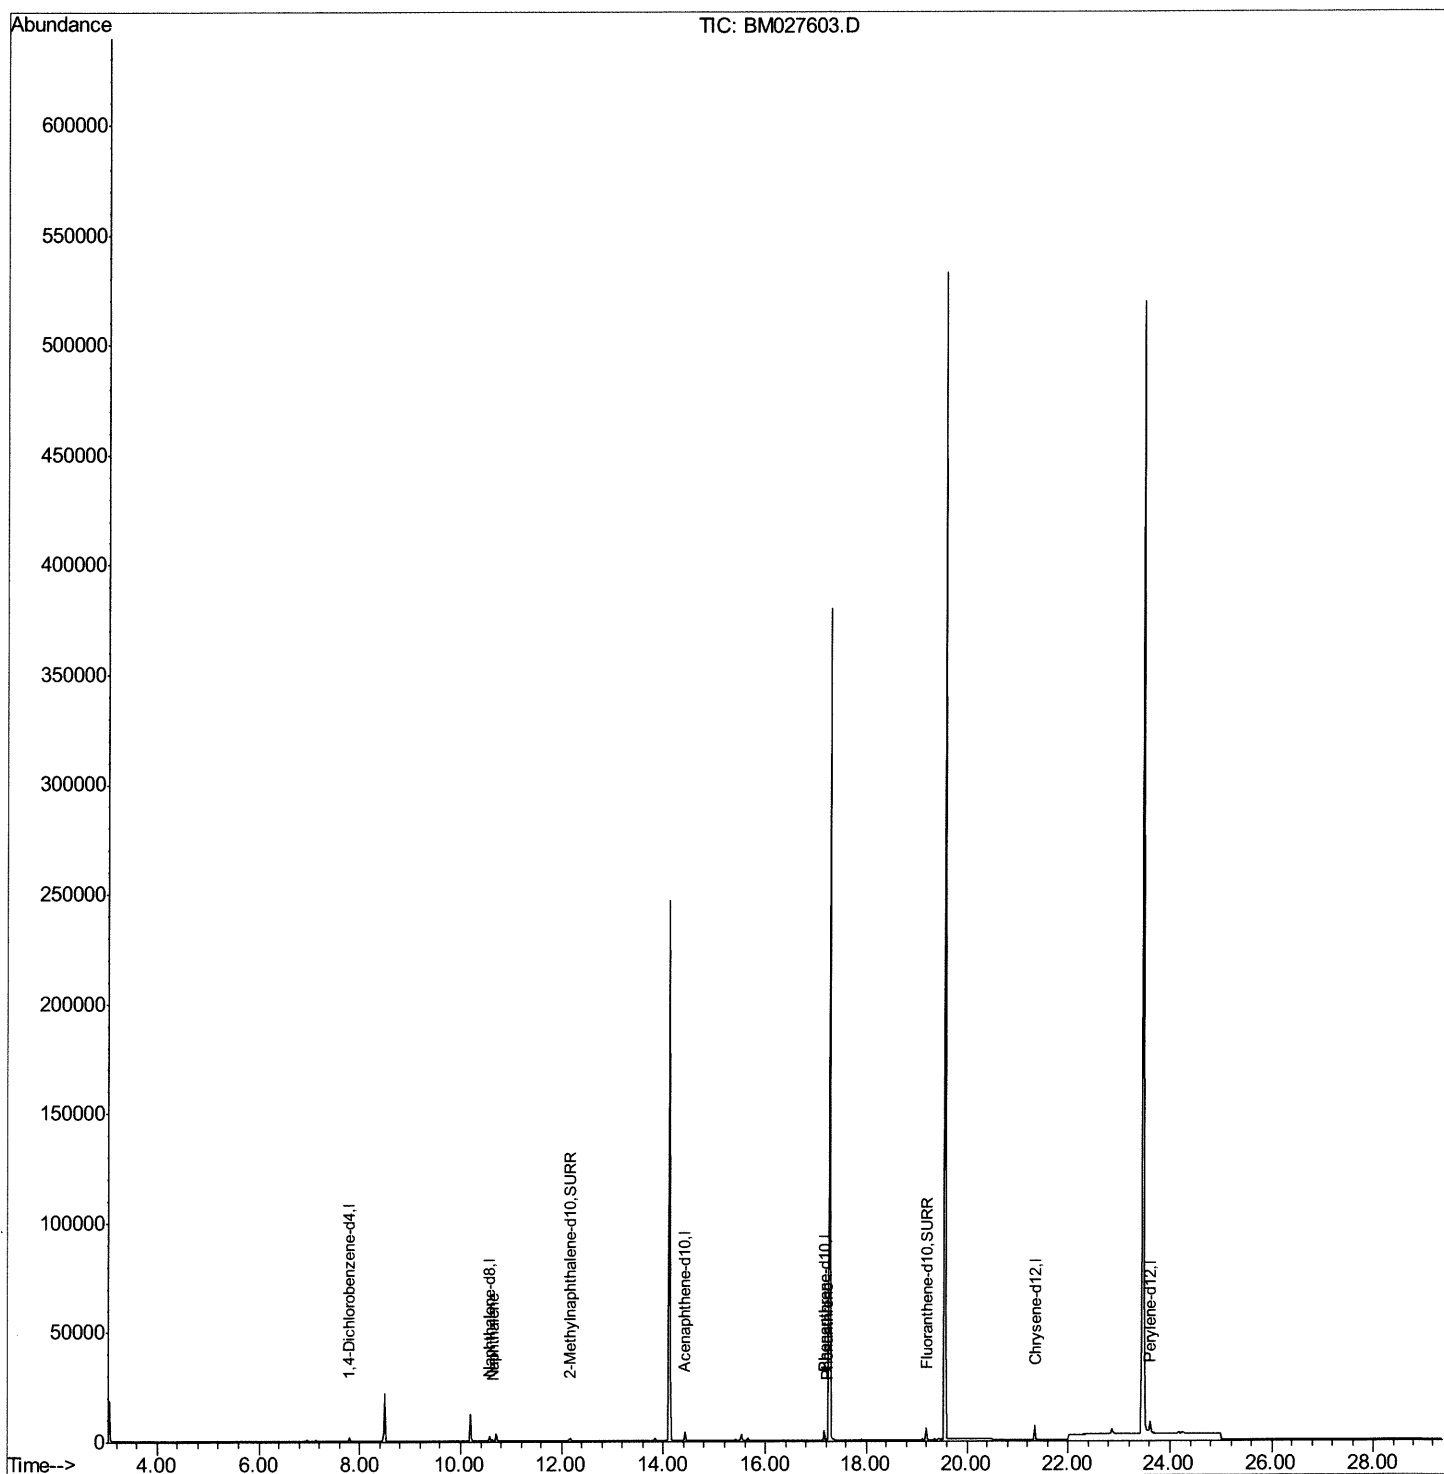

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100520\
 Data File : BM027603.D
 Acq On : 05 Oct 2020 13:04
 Operator : JU/CG
 Sample : L4185-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AR6

Manual Integrations
 APPROVED

mohammad
 10/6/2020 3:23:29 PM

Quant Time: Oct 05 13:36:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 05 10:43:07 2020
 Response via : Initial Calibration

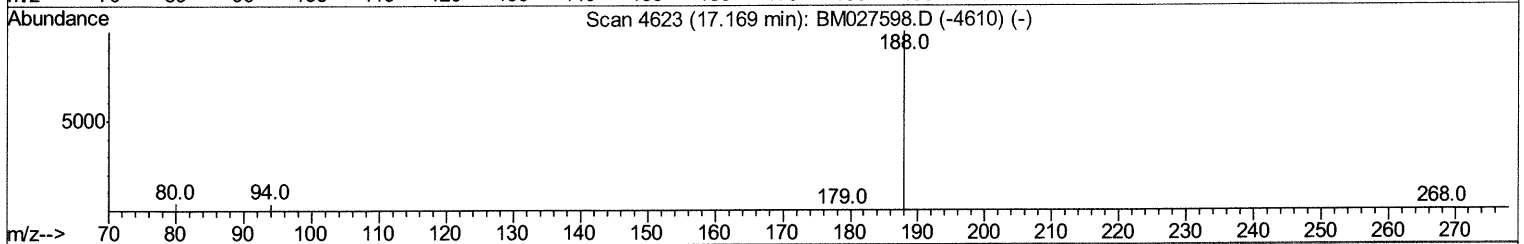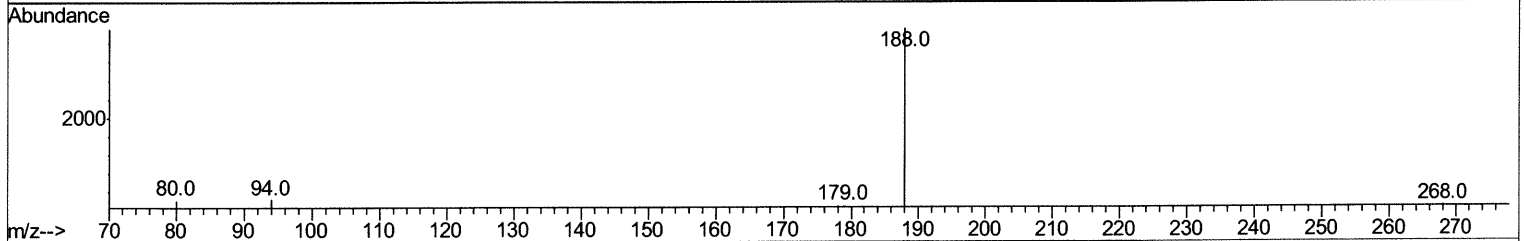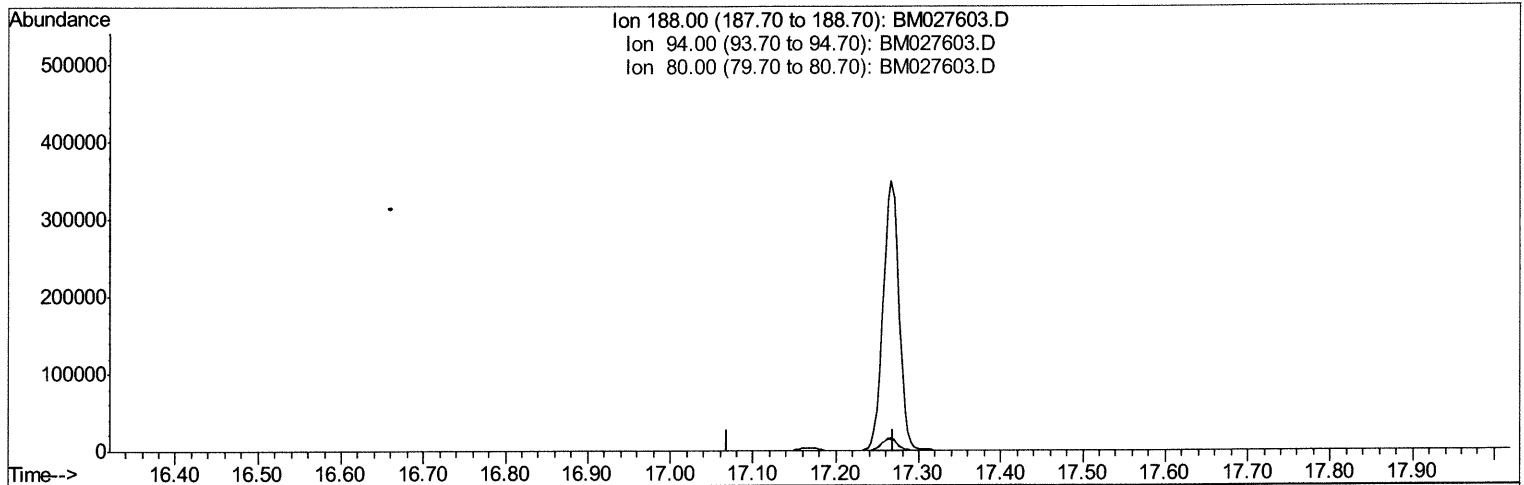

TIC: BM027603.D

(10) Phenanthrene-d10 (I)
 17.169min (-17.169) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	5.20	0.00#
80.00	6.20	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100520\
 Data File : BM027603.D
 Acq On : 05 Oct 2020 13:04
 Operator : JU/CG
 Sample : L4185-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AR6

Manual Integrations
 APPROVED

mohammad
 10/6/2020 3:23:29 PM

Quant Time: Oct 05 13:36:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 05 10:43:07 2020
 Response via : Initial Calibration

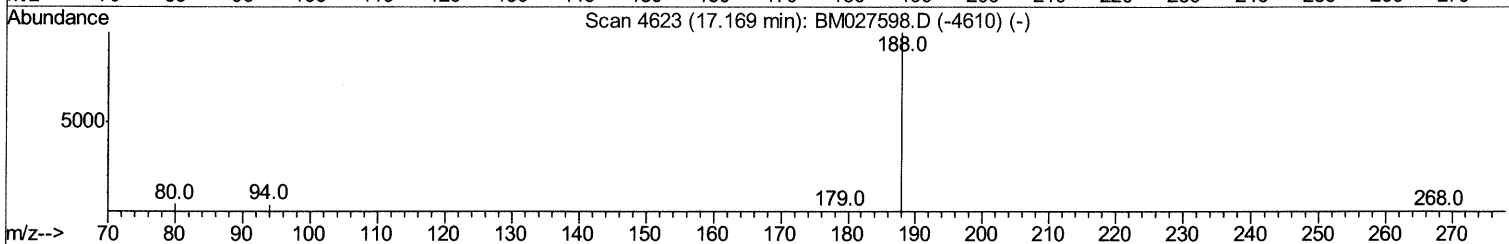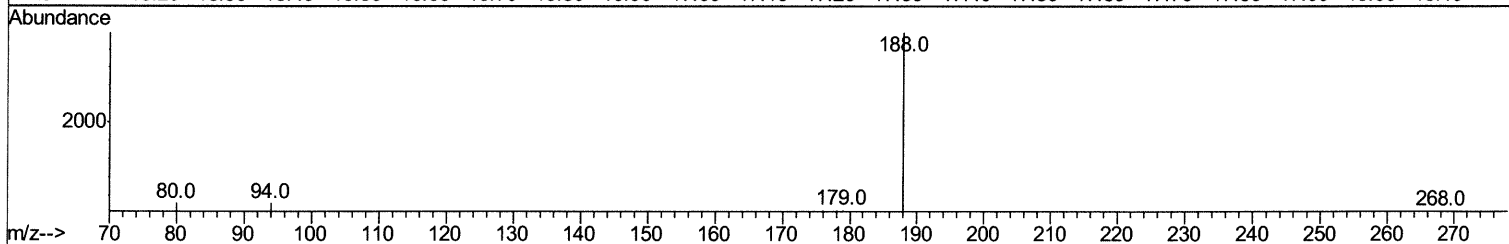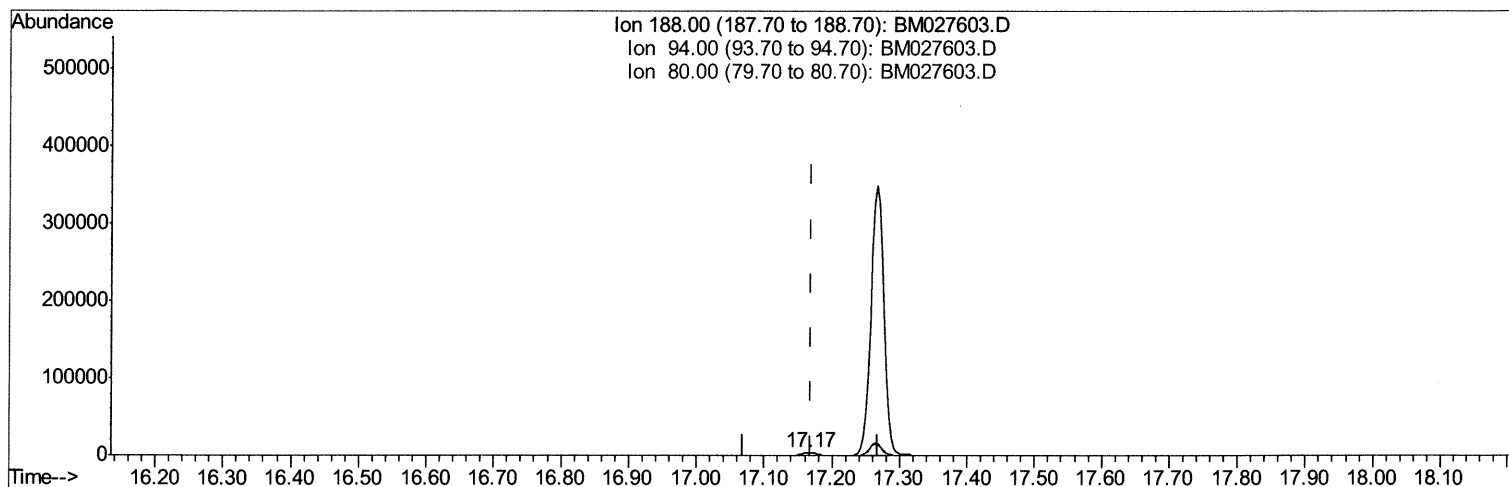

TIC: BM027603.D

(10) Phenanthrene-d10 (I)

17.166min (-0.003) 0.40ng/ul m 10/07/20 JU

response 5601

Ion	Exp%	Act%
188.00	100	100
94.00	5.20	5.86
80.00	6.20	5.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100520\
 Data File : BM027603.D
 Acq On : 05 Oct 2020 13:04
 Operator : JU/CG
 Sample : L4185-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AR6

Manual Integrations
 APPROVED

mohammad
 10/6/2020 3:23:29 PM

Quant Time: Oct 05 13:37:13 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 05 10:43:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	1020	0.40	ng/ul	0.00
2) Naphthalene-d8	10.58	136	2954	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.42	164	2217	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.17	188	5601m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.35	240	6233	0.40	ng/ul	0.00
20) Perylene-d12	23.61	264	6895	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.17	152	1554	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.19	212	6158	0.40	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.63	128	437	0.051	ng/ul#	71
12) Phenanthrene	17.21	178	355	0.021	ng/ul#	58

(#) = qualifier out of range (m) = manual integration (+) = signals summed

10/6/2020 J4