


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100520\
Data File : BM027606.D
Acq On : 05 Oct 2020 14:53
Operator : JU/CG
Sample : L4209-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLWS8

Manual Integrations
APPROVED

mohammad
10/6/2020 3:23:38 PM

Quant Time: Oct 05 15:39:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 10:43:07 2020
Response via : Initial Calibration

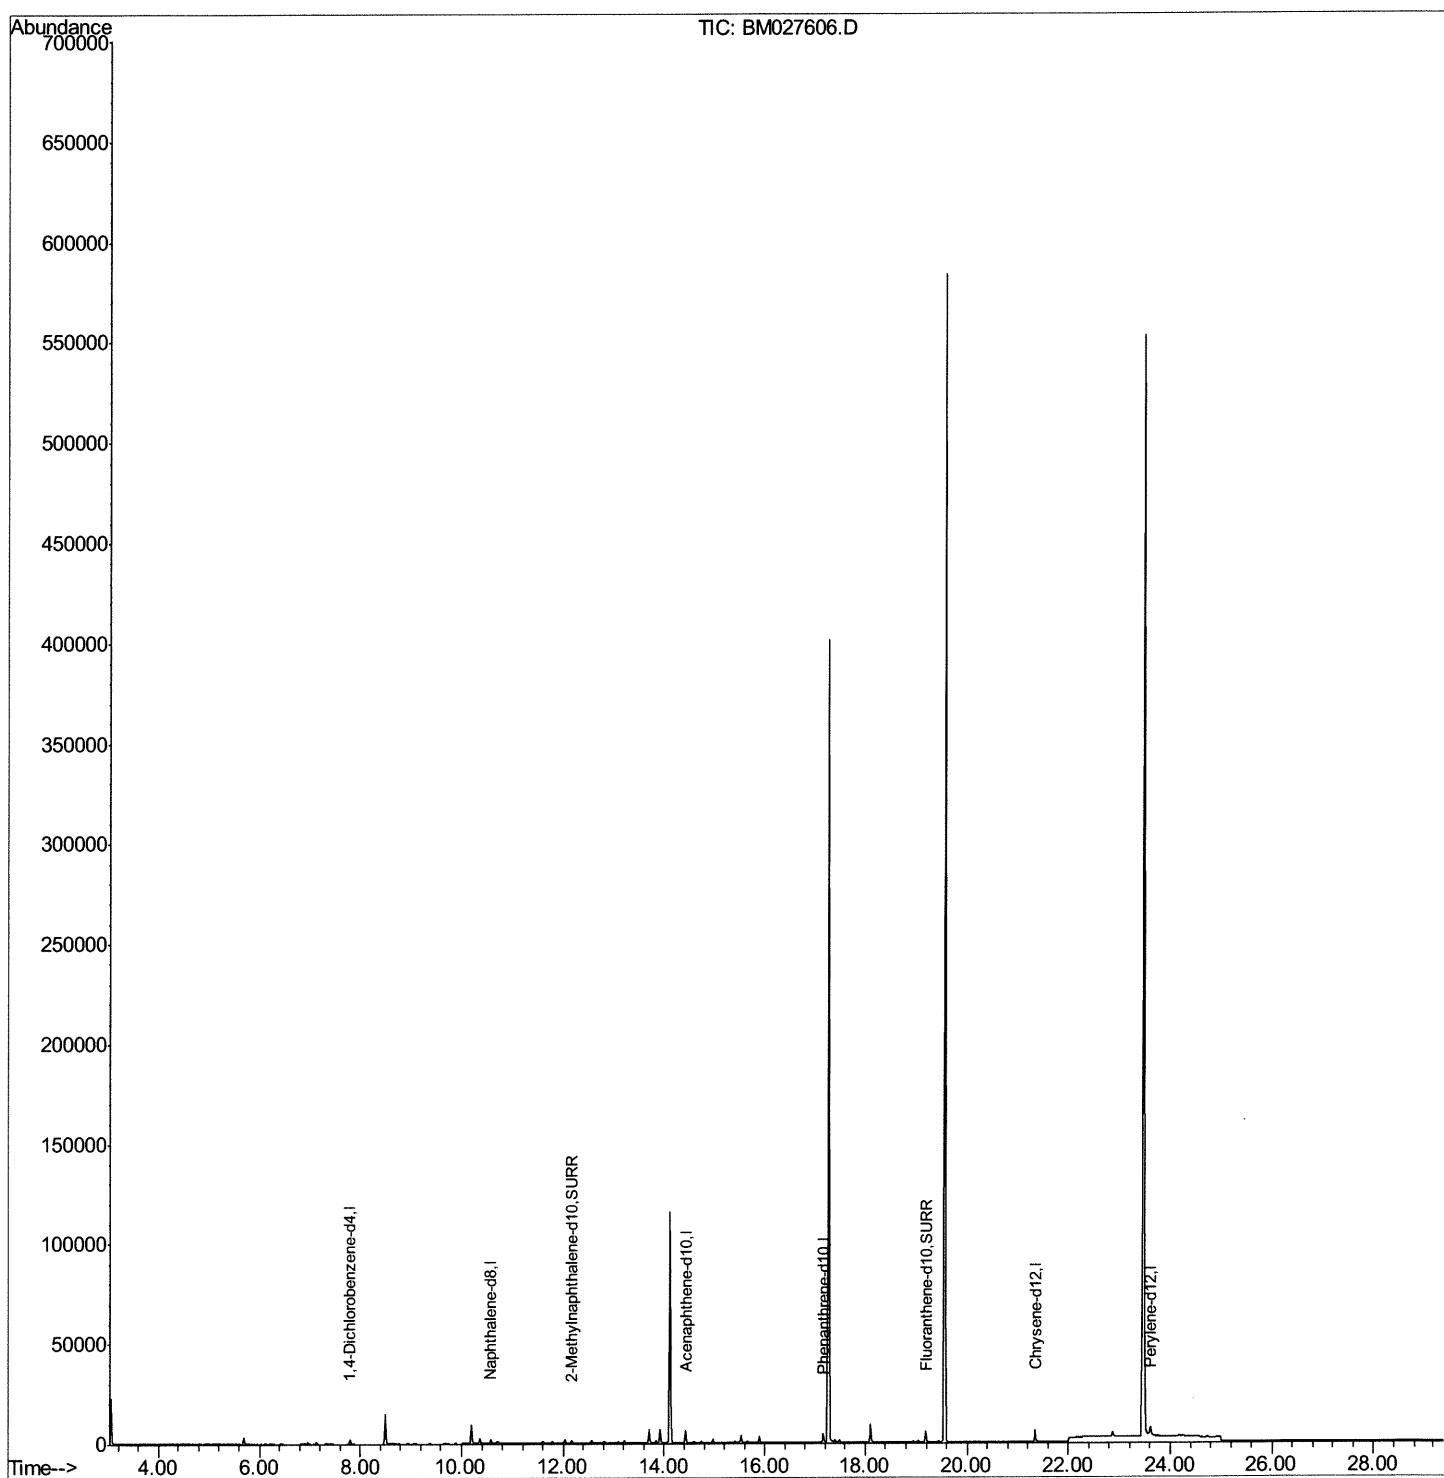

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100520\
Data File : BM027606.D
Acq On : 05 Oct 2020 14:53
Operator : JU/CG
Sample : L4209-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLWS8

Manual Integrations
APPROVED

mohammad
10/6/2020 3:23:38 PM

Quant Time: Oct 05 15:38:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 10:43:07 2020
Response via : Initial Calibration

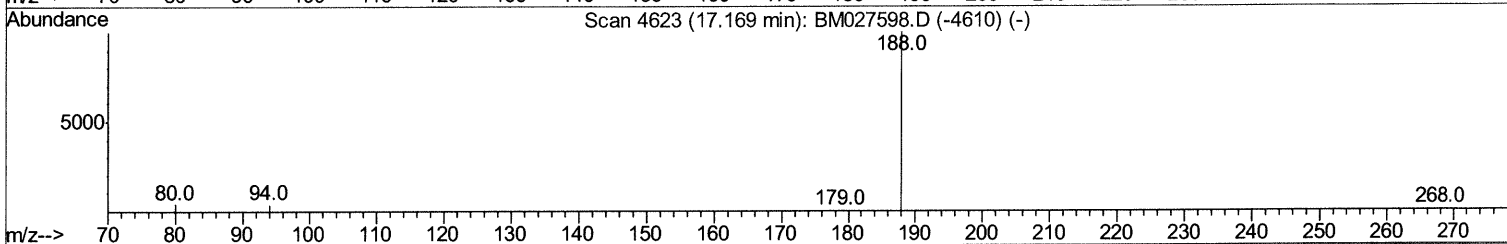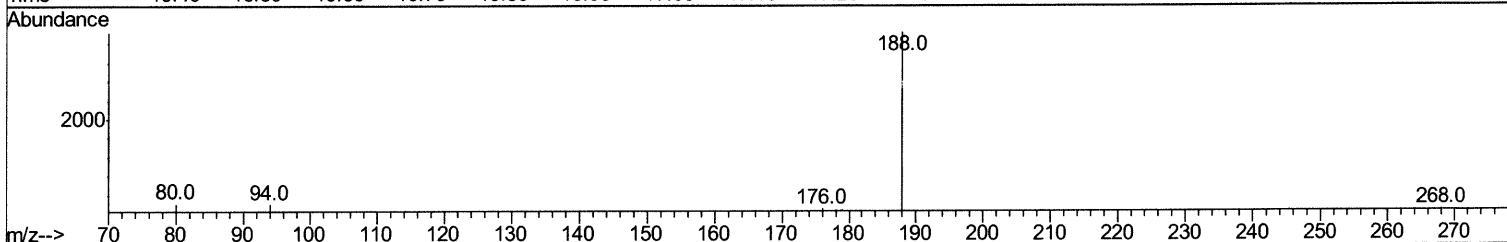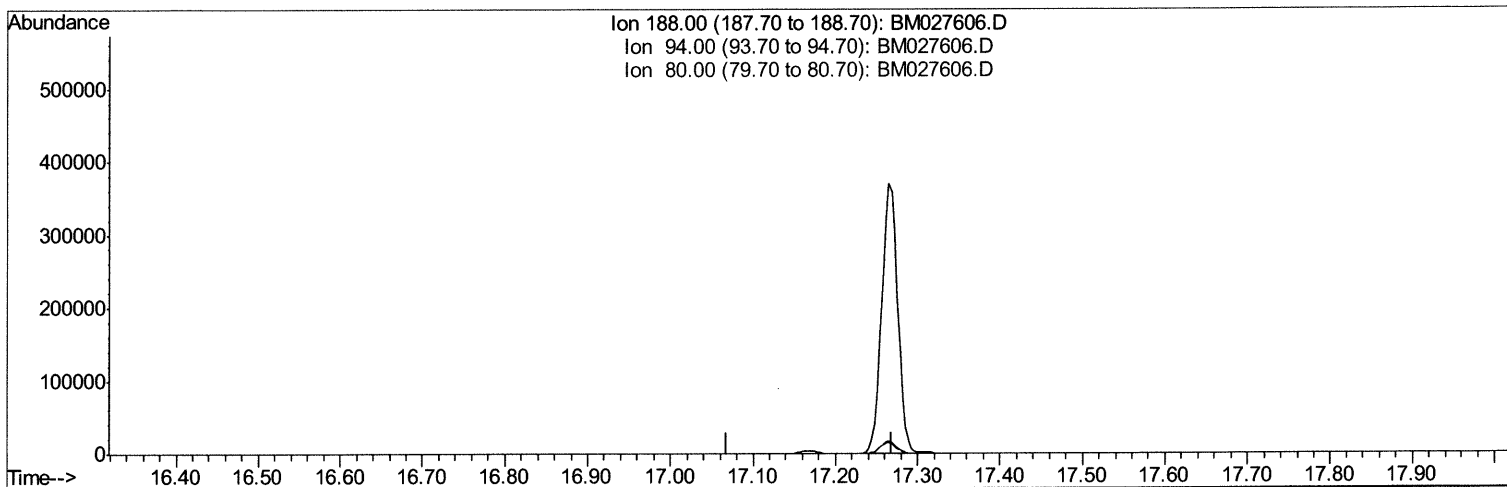

TIC: BM027606.D

(10) Phenanthrene-d10 (I)

17.169min (-17.169) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	5.20	0.00#
80.00	6.20	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100520\
Data File : BM027606.D
Acq On : 05 Oct 2020 14:53
Operator : JU/CG
Sample : L4209-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLWS8

Manual Integrations
APPROVED

mohammad
10/6/2020 3:23:38 PM

Quant Time: Oct 05 15:38:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 10:43:07 2020
Response via : Initial Calibration

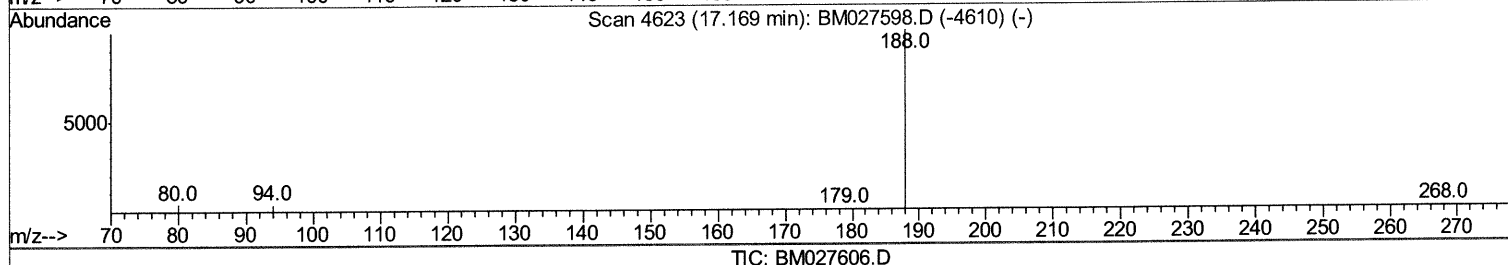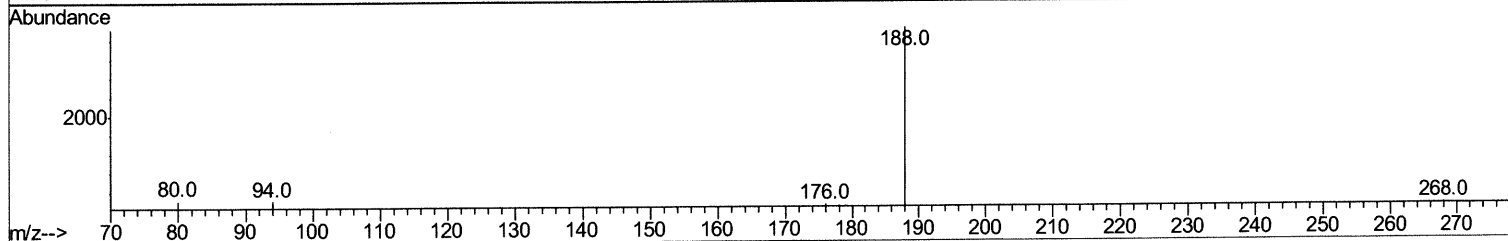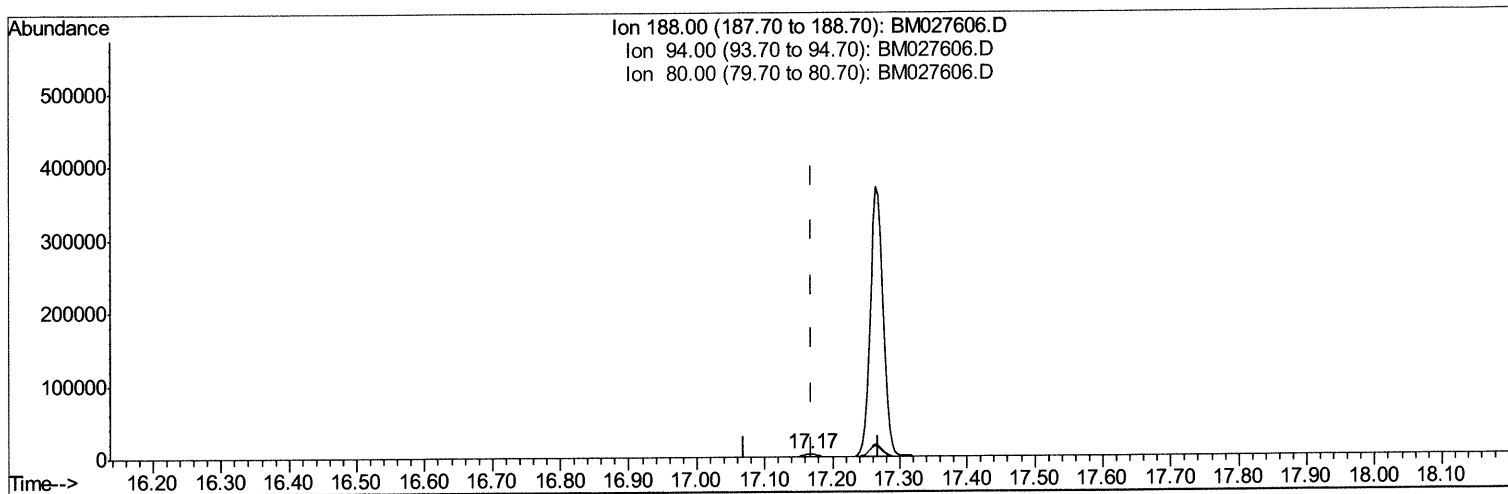

(10) Phenanthrene-d10 (I)

17.168min (-0.002) 0.40ng/ul m

10/07/2020

response 5473

Ion	Exp%	Act%
188.00	100	100
94.00	5.20	5.18
80.00	6.20	5.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100520\
Data File : BM027606.D
Acq On : 05 Oct 2020 14:53
Operator : JU/CG
Sample : L4209-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLWS8

Manual Integrations
APPROVED

mohammad
10/6/2020 3:23:38 PM

Quant Time: Oct 05 15:39:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 10:43:07 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	976	0.40	ng/ul	0.00
2) Naphthalene-d8	10.58	136	2868	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.43	164	3224	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.17	188	5473m>	0.40	ng/ul	> 0.00
16) Chrysene-d12	21.35	240	5801	0.40	ng/ul	0.00
20) Perylene-d12	23.61	264	6315	0.40	ng/ul	0.00

10/6/2020 JU

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.17	152	1636	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.19	212	6876	0.46	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed