

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100520\
Quantitation Report (QT Reviewed)


Data File : BM027622.D
Acq On : 06 Oct 2020 01:14
Operator : JU/CG
Sample : L4184-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AN7

Manual Integrations
APPROVED

mohammad
10/6/2020 3:24:20 PM

Quant Time: Oct 06 03:33:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 06 01:23:11 2020
Response via : Initial Calibration

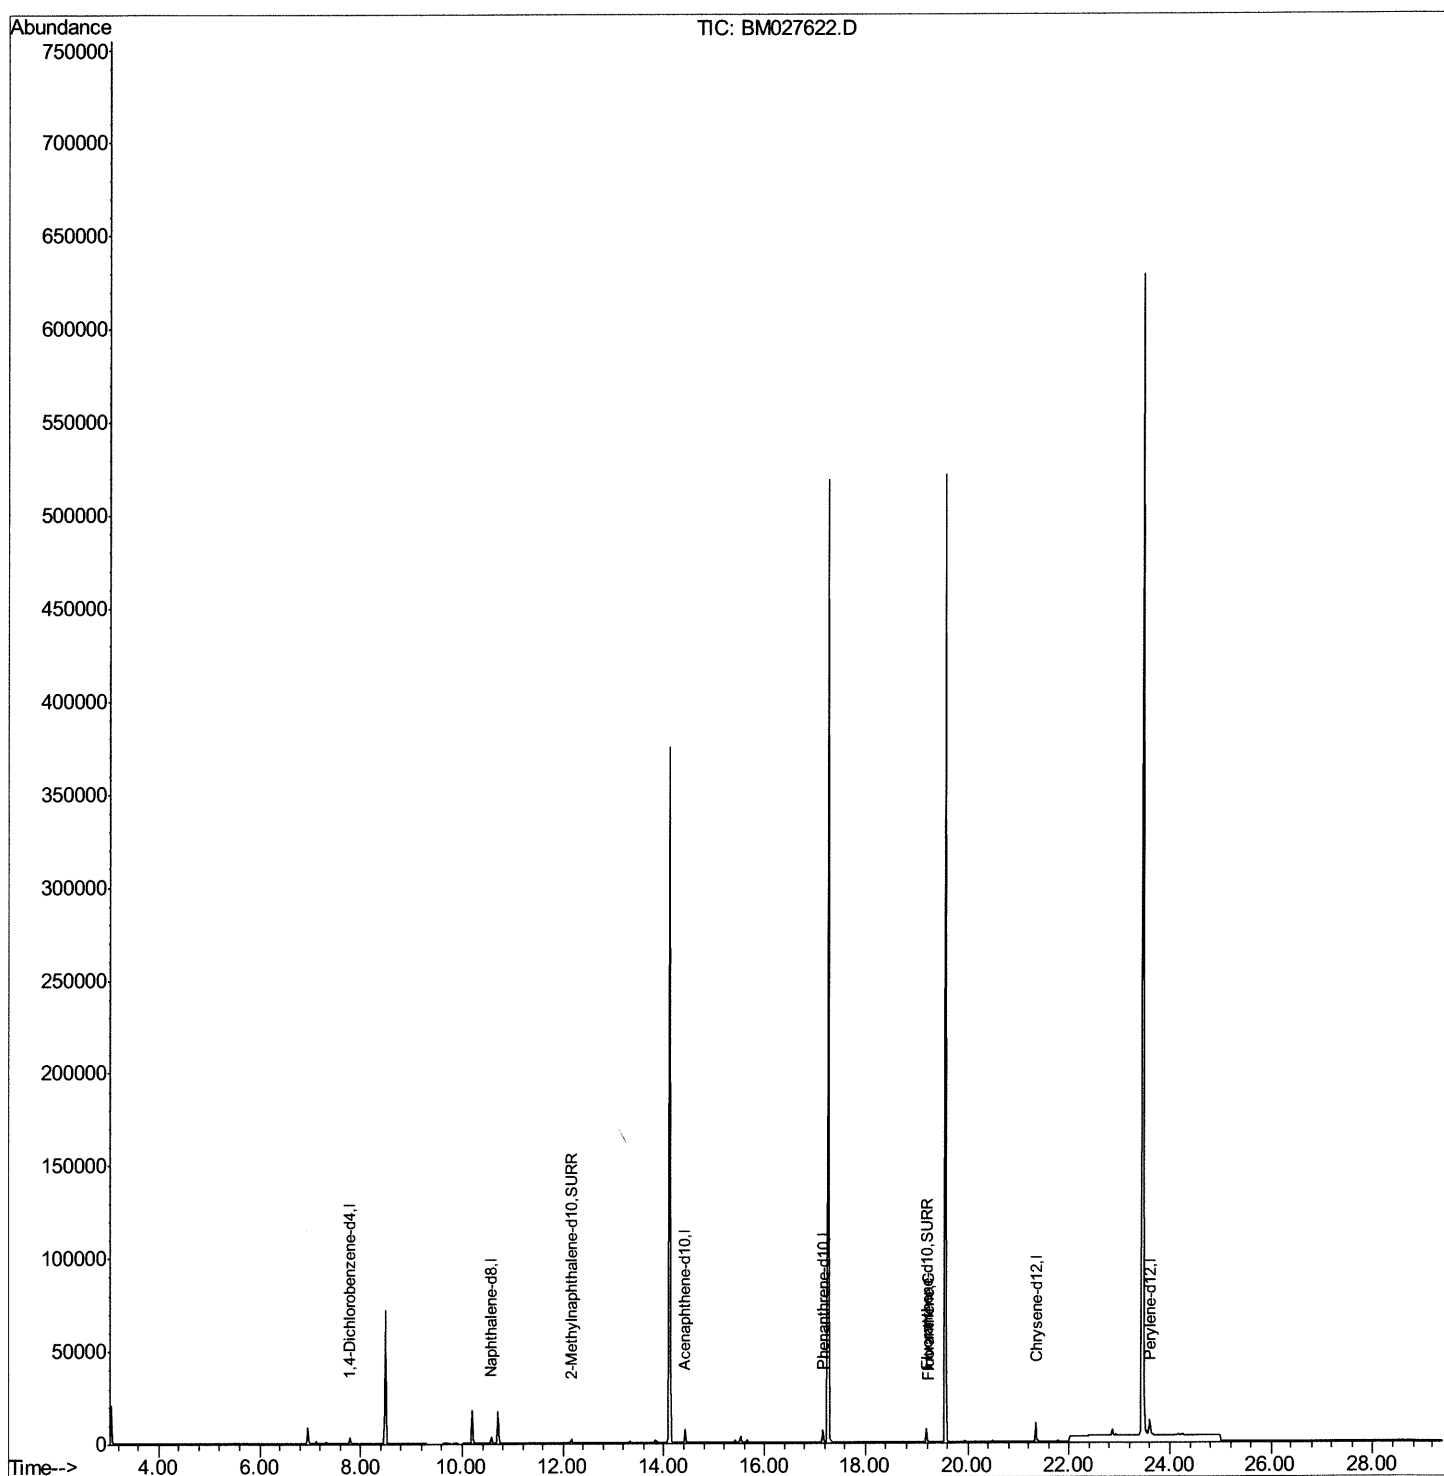

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100520\
Quantitation Report (Qedit)




Data File : BM027622.D
Acq On : 06 Oct 2020 01:14
Operator : JU/CG
Sample : L4184-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AN7

Manual Integrations
APPROVED

mohammad
10/6/2020 3:24:20 PM

Quant Time: Oct 06 03:31:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 06 01:23:11 2020
Response via : Initial Calibration

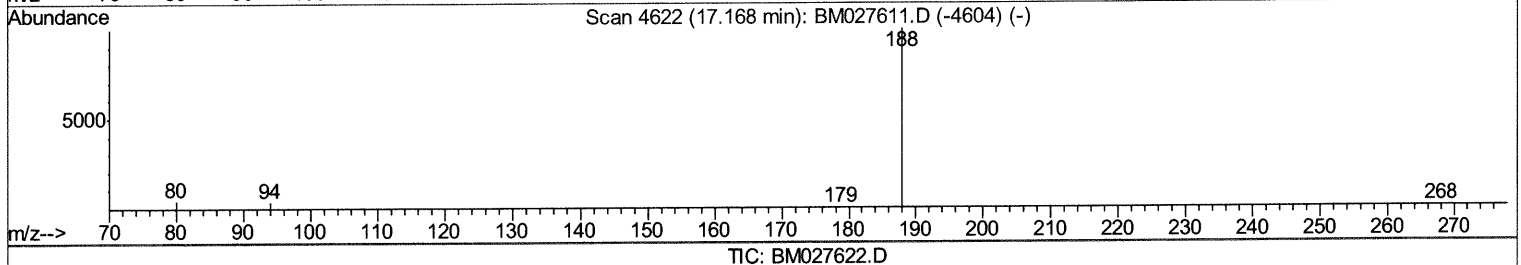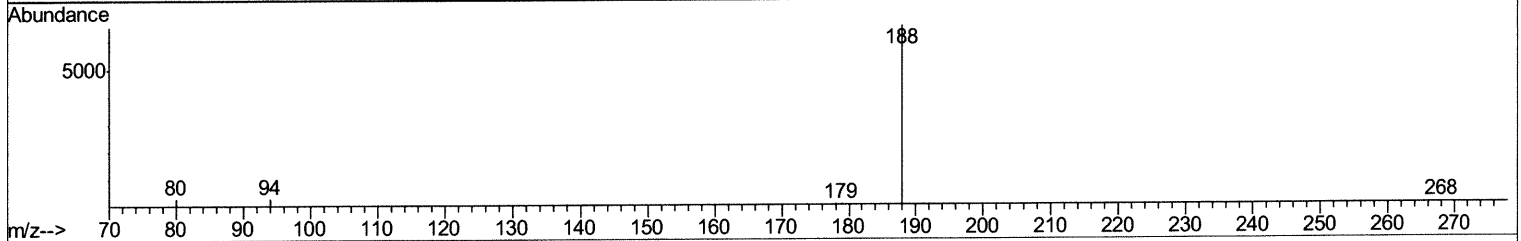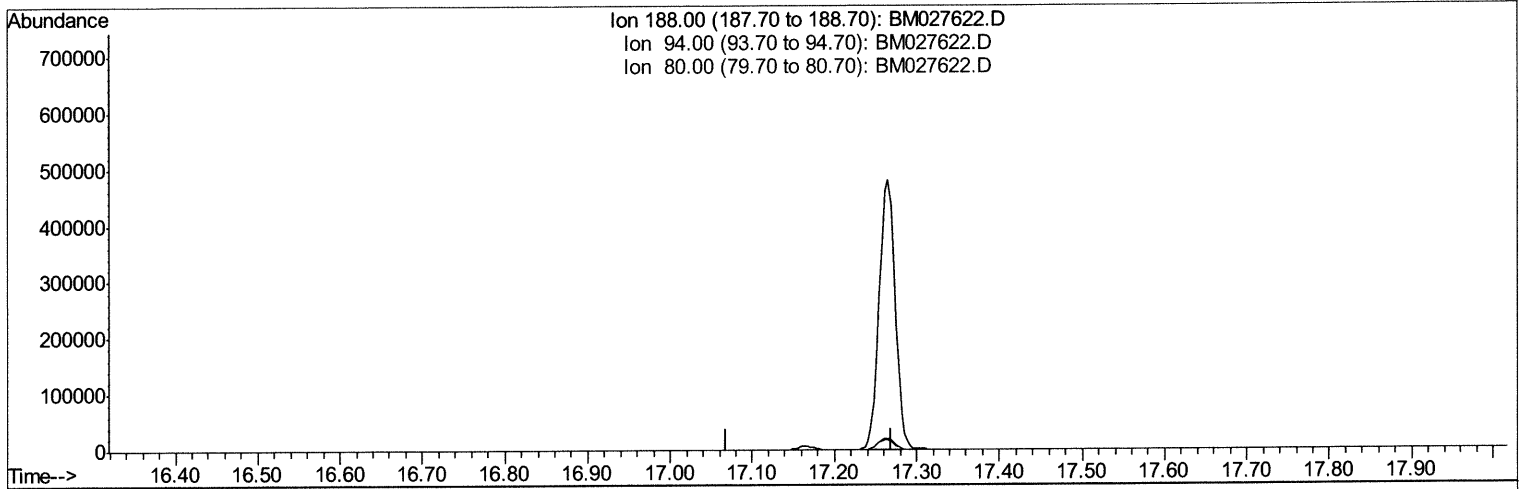

TIC: BM027622.D

(10) Phenanthrene-d10 (I)
17.169min (-17.169) 0.00ng/ul
response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	5.20	0.00#
80.00	6.20	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100520\
Quantitation Report (Qedit)




Data File : BM027622.D
Acq On : 06 Oct 2020 01:14
Operator : JU/CG
Sample : L4184-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AN7

Manual Integrations
APPROVED

mohammad
10/6/2020 3:24:20 PM

Quant Time: Oct 06 03:31:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 06 01:23:11 2020
Response via : Initial Calibration

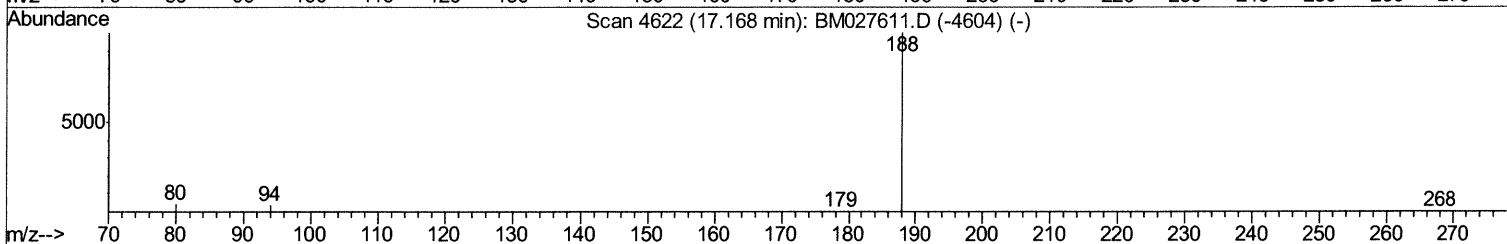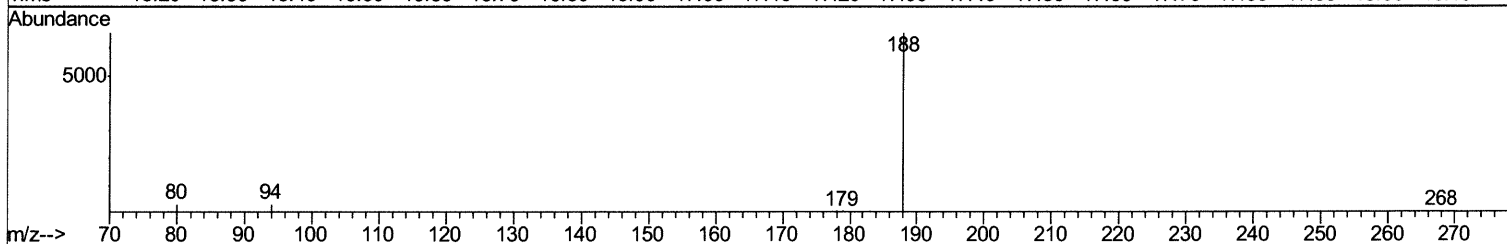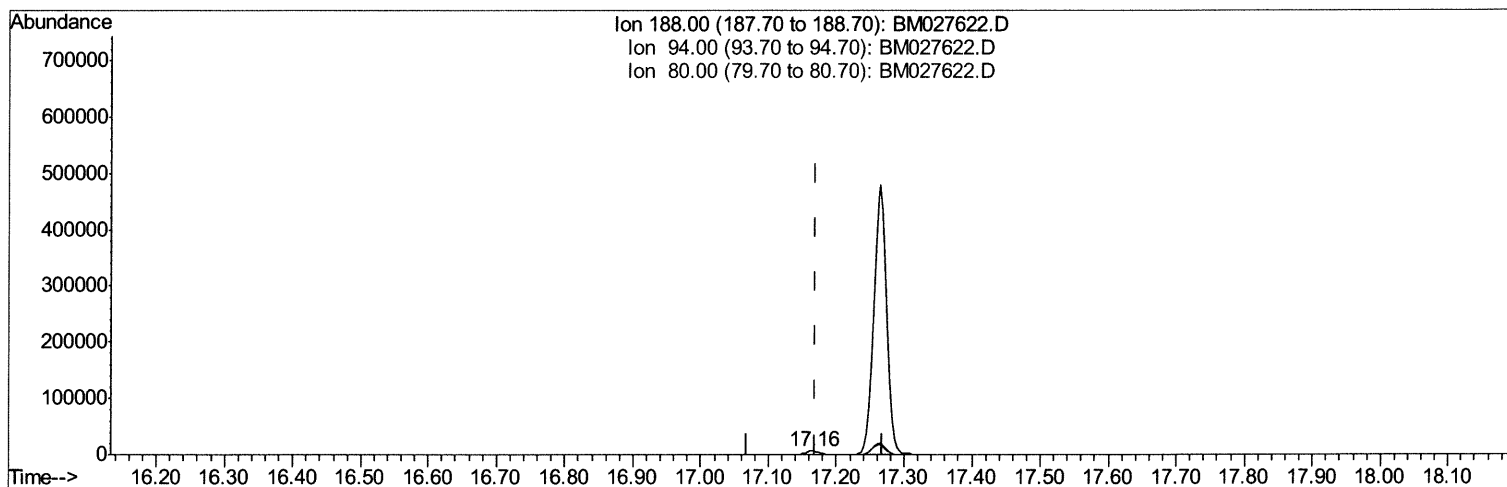

TIC: BM027622.D

(10) Phenanthrene-d10 (I)

17.164min (-0.005) 0.40ng/ul m 10/07/20 JU

response 9040

Ion	Exp%	Act%
188.00	100	100
94.00	5.20	4.81
80.00	6.20	4.92#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100520\
Quantitation Report (QT Reviewed)

Data File : BM027622.D
Acq On : 06 Oct 2020 01:14
Operator : JU/CG
Sample : L4184-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AN7

Manual Integrations
APPROVED

mohammad
10/6/2020 3:24:20 PM

Quant Time: Oct 06 03:33:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 06 01:23:11 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	1742	0.40	ng/ul	0.00
2) Naphthalene-d8	10.58	136	4971	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.42	164	3717	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.16	188	9040m>	0.40	ng/ul	> 0.00
16) Chrysene-d12	21.34	240	9943	0.40	ng/ul	0.00
20) Perylene-d12	23.60	264	10823	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.17	152	2755	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.19	212	8430	0.34	ng/ul	0.00
Target Compounds						
15) Fluoranthene	19.22	202	711	0.021	ng/ul	Qvalue 72

(#) = qualifier out of range (m) = manual integration (+) = signals summed

10/6/20 JU