

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100520\
Quantitation Report (QT Reviewed)


Data File : BM027624.D
Acq On : 06 Oct 2020 02:26
Operator : JU/CG
Sample : L4184-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK0

Manual Integrations
APPROVED

mohammad
10/6/2020 3:24:26 PM

Quant Time: Oct 06 03:39:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 06 01:23:11 2020
Response via : Initial Calibration

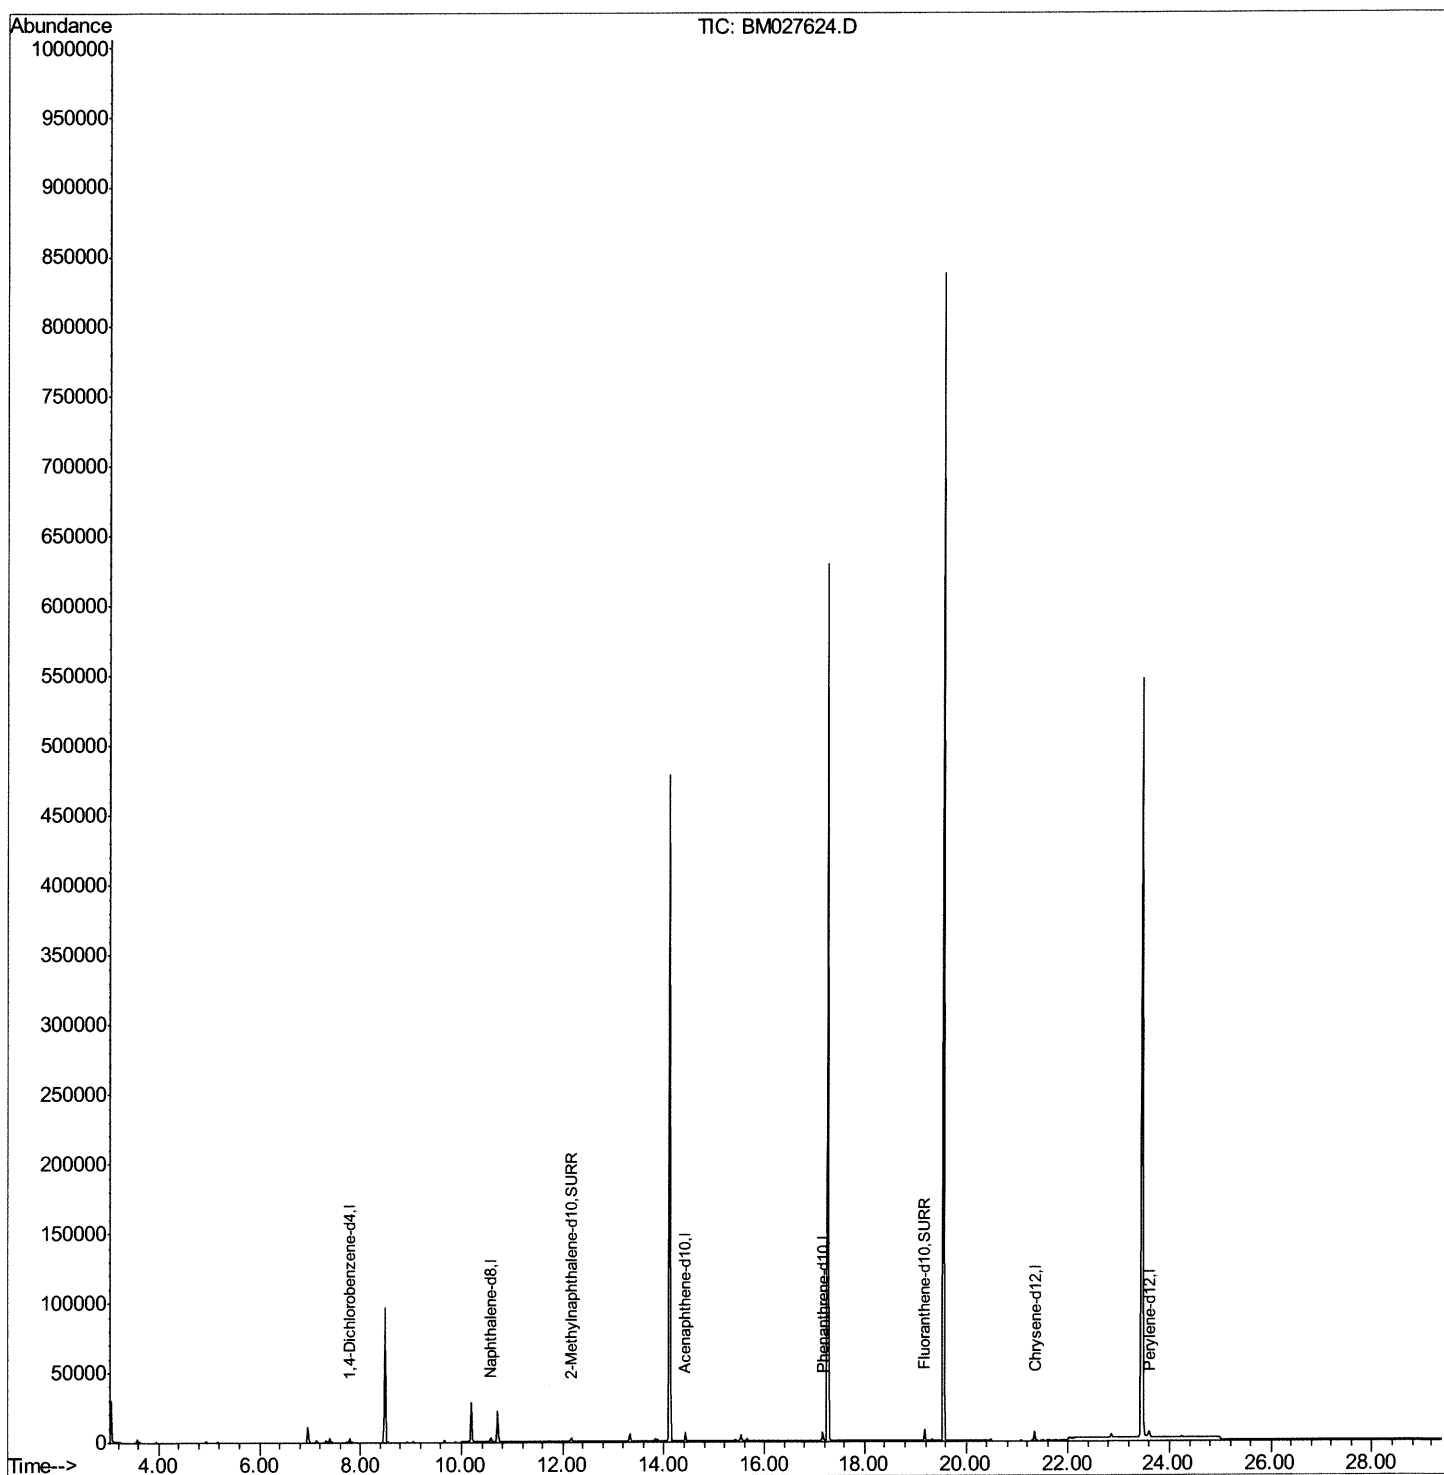

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100520\
Quantitation Report (Qedit)




Data File : BM027624.D
Acq On : 06 Oct 2020 02:26
Operator : JU/CG
Sample : L4184-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK0

Manual Integrations
APPROVED

mohammad
10/6/2020 3:24:26 PM

Quant Time: Oct 06 03:35:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 06 01:23:11 2020
Response via : Initial Calibration

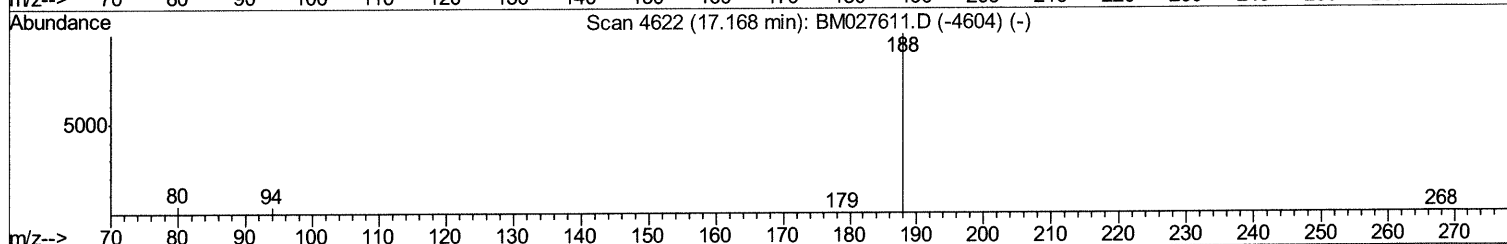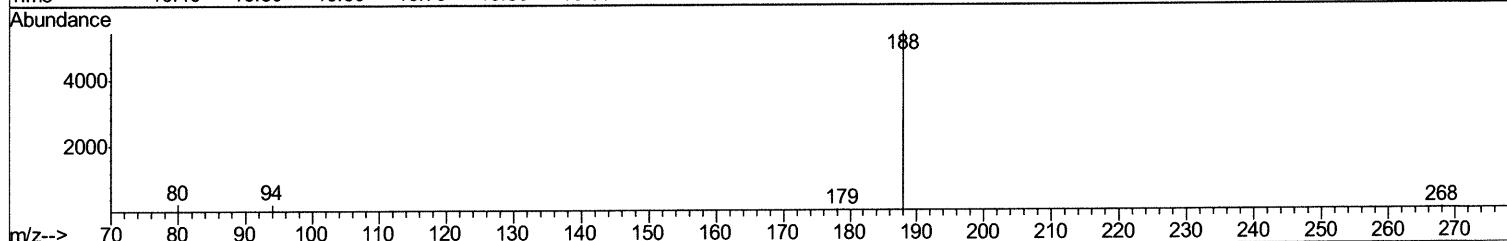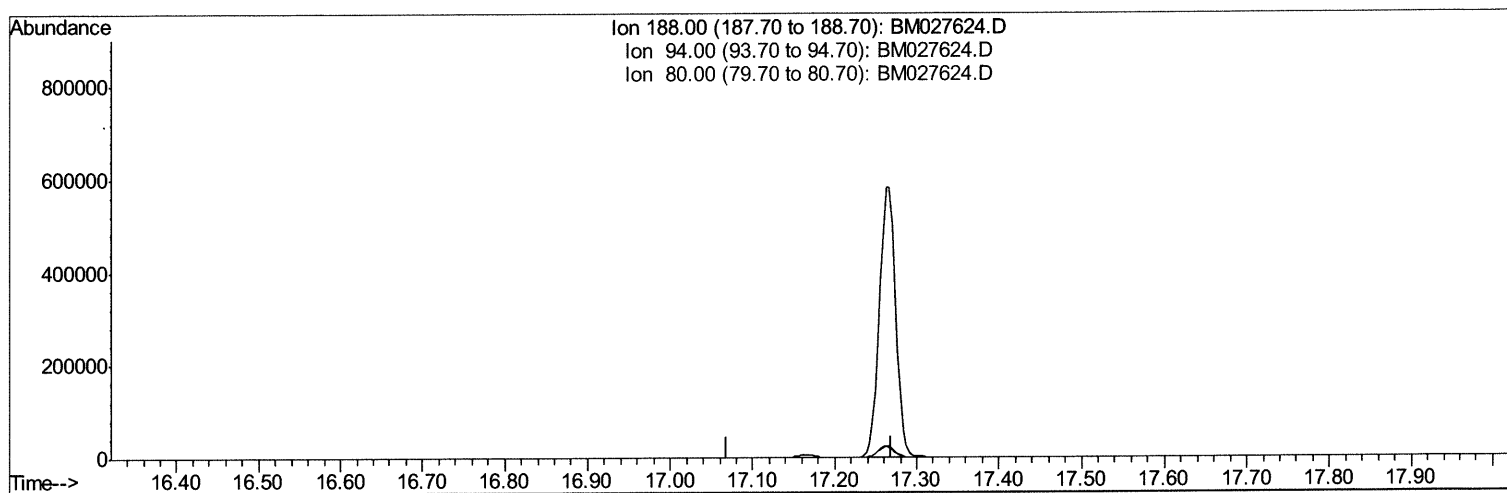

TIC: BM027624.D

(10) Phenanthrene-d10 (I)

17.169min (-17.169) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	5.20	0.00#
80.00	6.20	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100520\
Quantitation Report (Qedit)




Data File : BM027624.D
Acq On : 06 Oct 2020 02:26
Operator : JU/CG
Sample : L4184-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK0

Manual Integrations
APPROVED

mohammad
10/6/2020 3:24:26 PM

Quant Time: Oct 06 03:35:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 06 01:23:11 2020
Response via : Initial Calibration

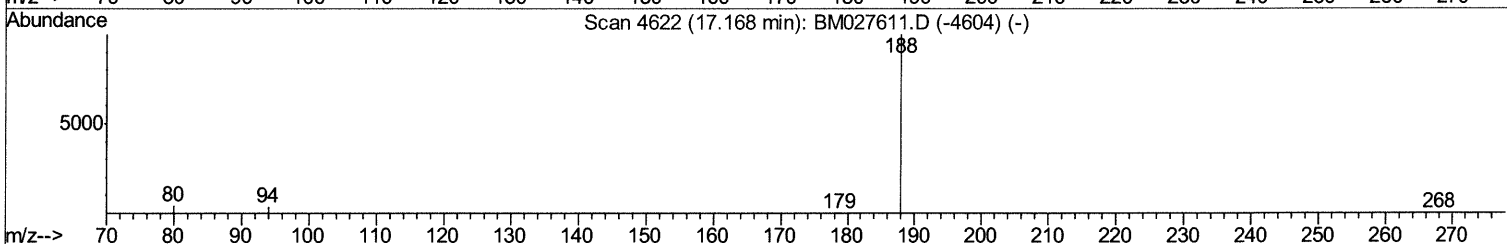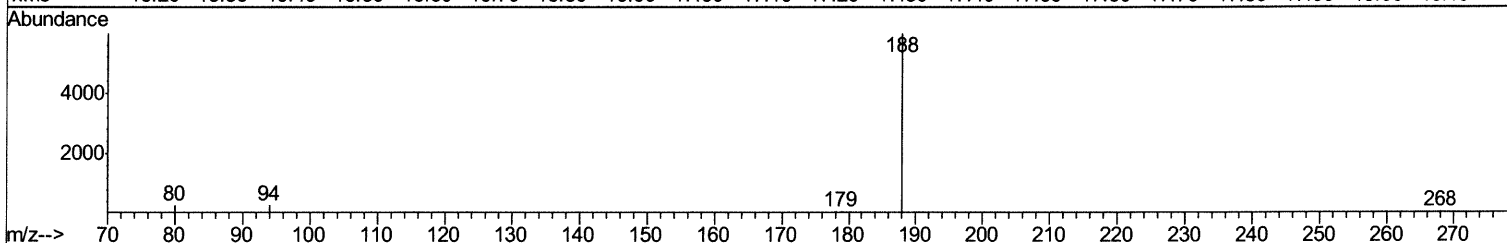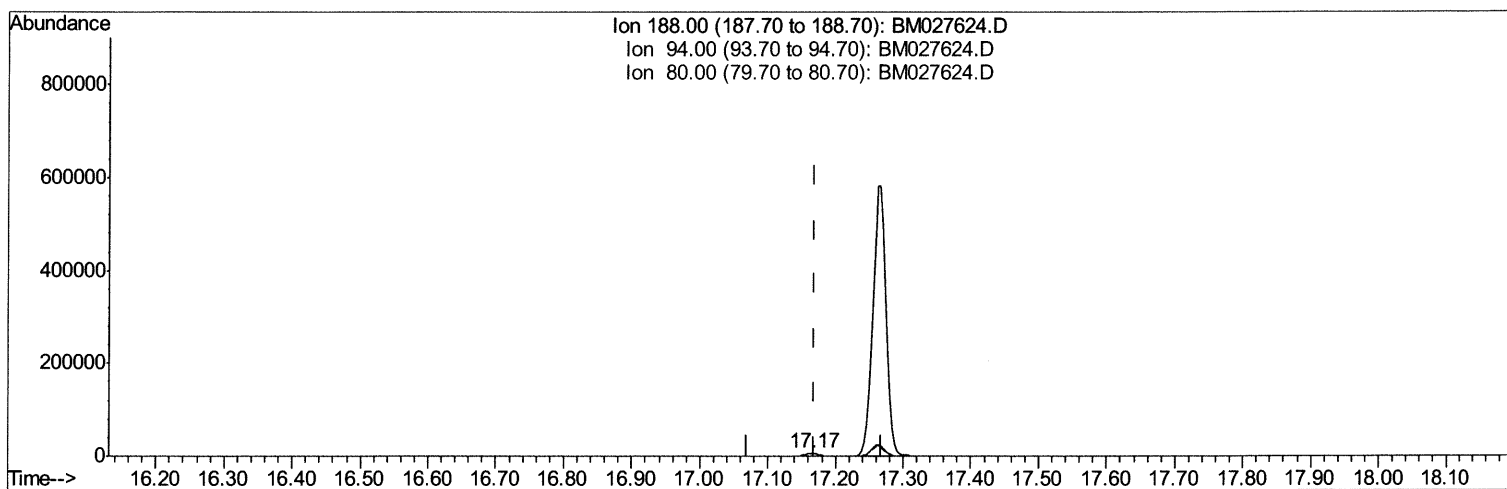

TIC: BM027624.D

(10) Phenanthrene-d10 (I)

17.166min (-0.004) 0.40ng/ul m 10/07/2020

response 7878

Ion	Exp%	Act%
188.00	100	100
94.00	5.20	4.61
80.00	6.20	4.84#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100520\
Quantitation Report (QT Reviewed)

Data File : BM027624.D
Acq On : 06 Oct 2020 02:26
Operator : JU/CG
Sample : L4184-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK0

Manual Integrations
APPROVED

mohammad
10/6/2020 3:24:26 PM

Quant Time: Oct 06 03:39:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 06 01:23:11 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	1528	0.40	ng/ul	0.00
2) Naphthalene-d8	10.58	136	4352	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.42	164	3324	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.17	188	7878m	0.40	ng/ul	> 0.00
16) Chrysene-d12	21.34	240	6459	0.40	ng/ul	0.00
20) Perylene-d12	23.60	264	6143	0.40	ng/ul	0.00

6/10/20 J4

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev (Min)
4) 2-Methylnaphthalene-d10	12.16	152	3487	0.44	ng/ul	0.00
14) Fluoranthene-d10	19.19	212	10484	0.49	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed