

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100520\
Quantitation Report (QT Reviewed)


Data File : BM027625.D
Acq On : 06 Oct 2020 03:02
Operator : JU/CG
Sample : L4184-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AM1

Manual Integrations
APPROVED

mohammad
10/6/2020 3:24:29 PM

Quant Time: Oct 06 03:41:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 06 01:23:11 2020
Response via : Initial Calibration

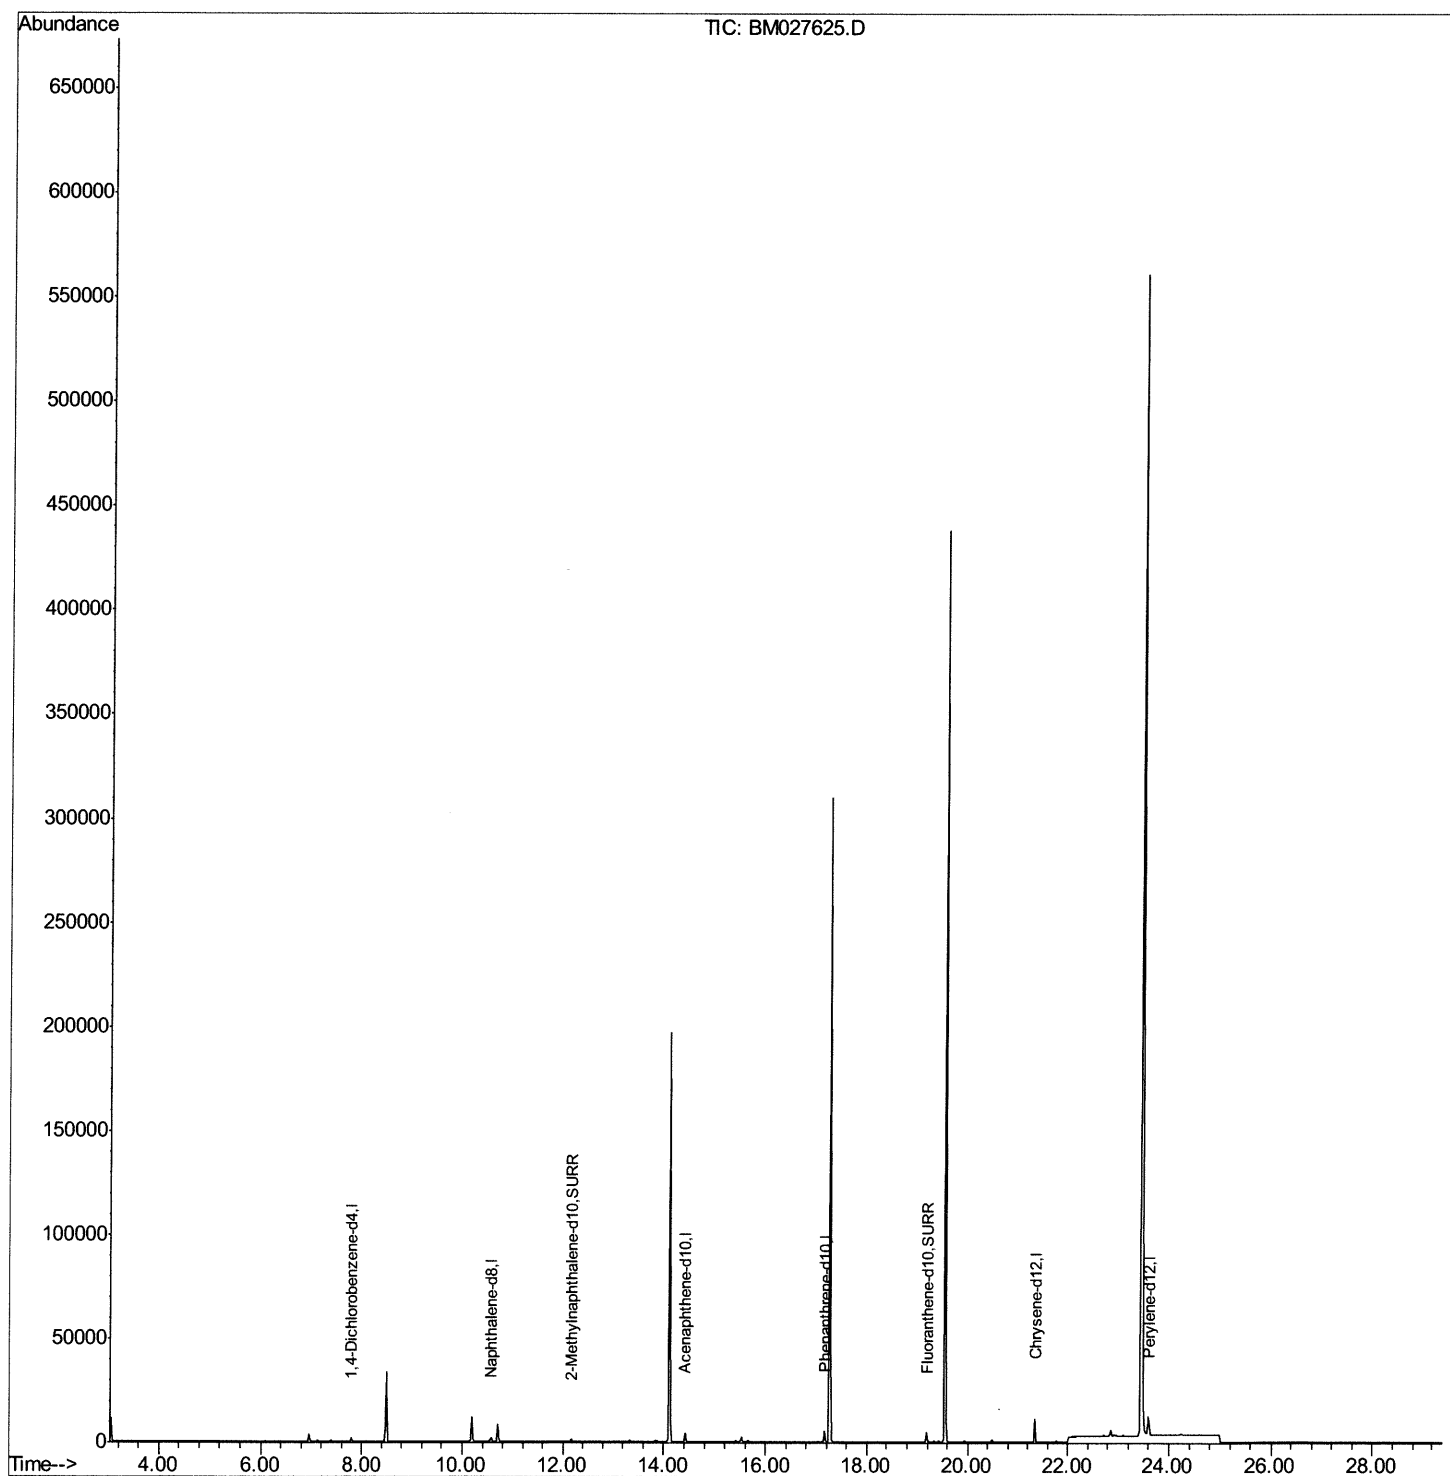

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100520\
Quantitation Report (Qedit)




Data File : BM027625.D
Acq On : 06 Oct 2020 03:02
Operator : JU/CG
Sample : L4184-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AM1

Manual Integrations
APPROVED

mohammad
10/6/2020 3:24:29 PM

Quant Time: Oct 06 03:40:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 06 01:23:11 2020
Response via : Initial Calibration

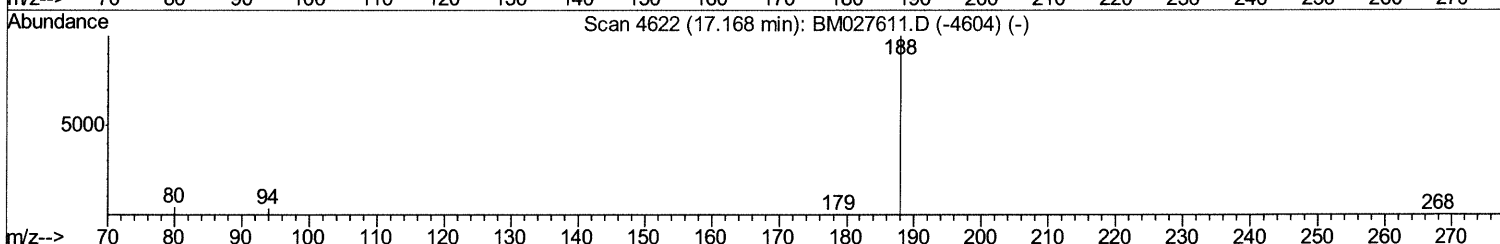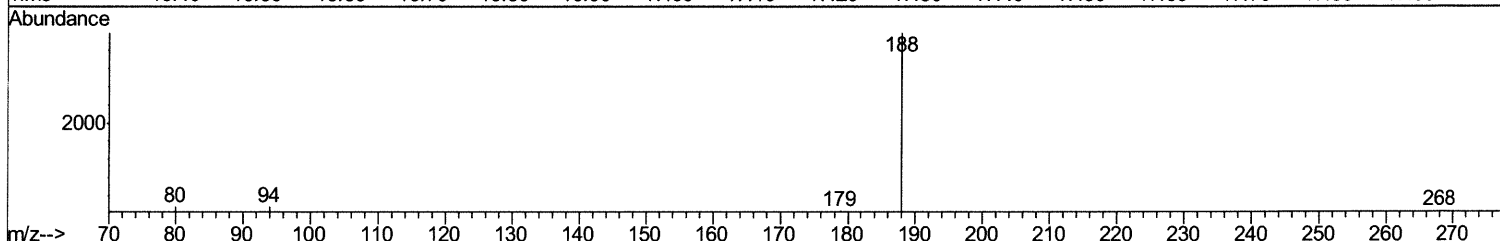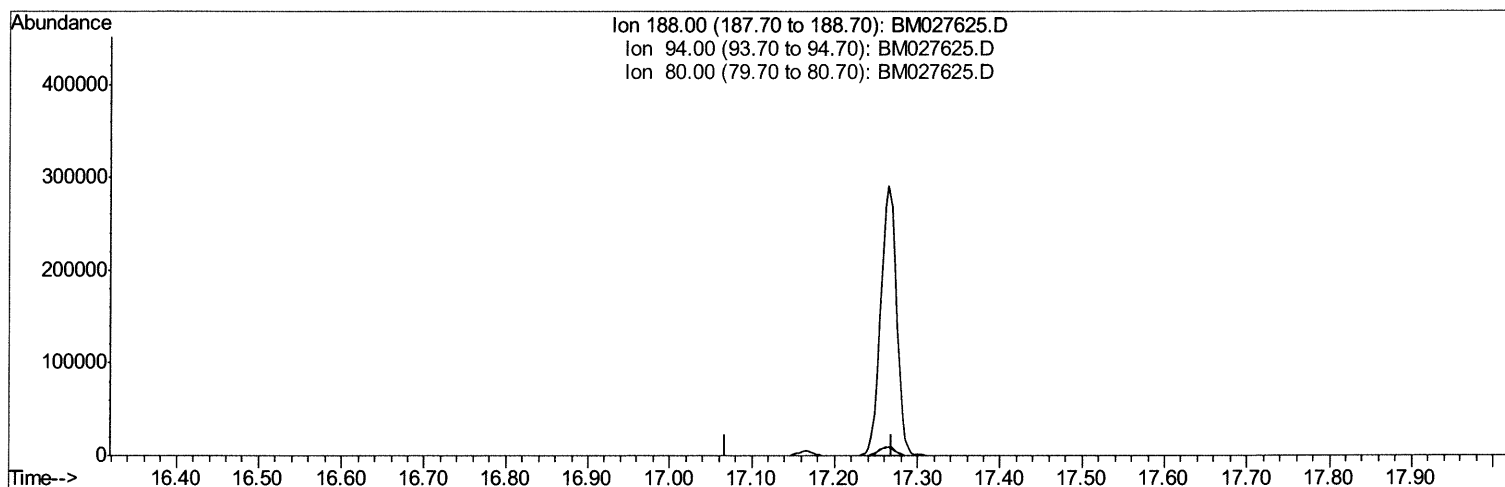

TIC: BM027625.D

(10) Phenanthrene-d10 (I)

17.169min (-17.169) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	5.20	0.00#
80.00	6.20	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100520\
Quantitation Report (Qedit)




Data File : BM027625.D
Acq On : 06 Oct 2020 03:02
Operator : JU/CG
Sample : L4184-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AM1

Manual Integrations
APPROVED

mohammad
10/6/2020 3:24:29 PM

Quant Time: Oct 06 03:40:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 06 01:23:11 2020
Response via : Initial Calibration

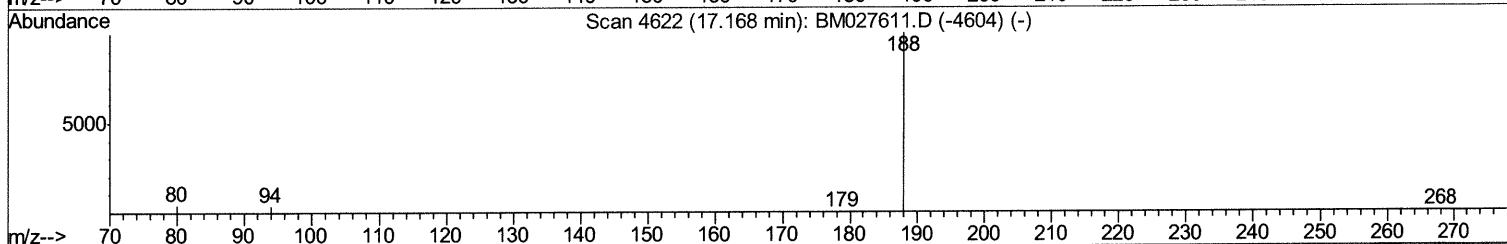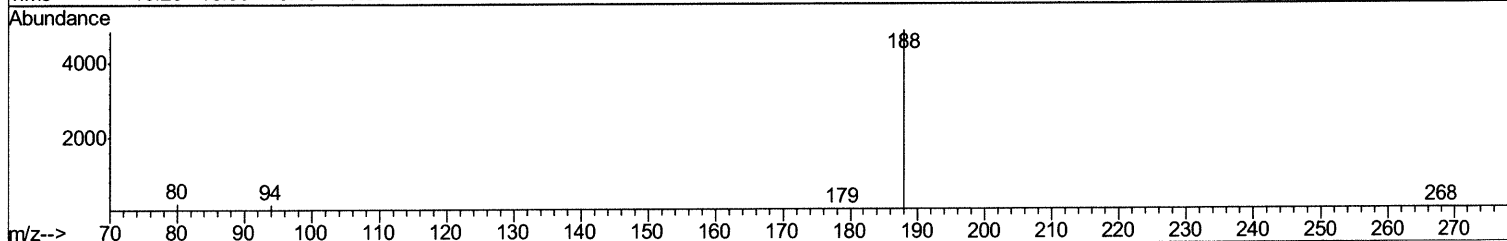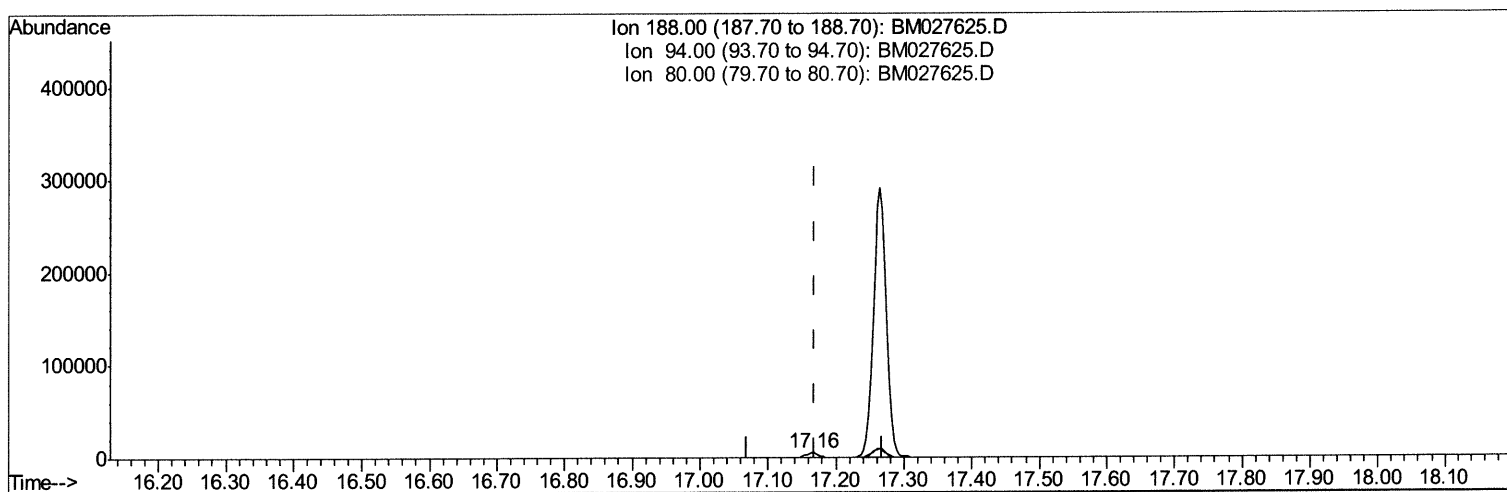

TIC: BM027625.D

(10) Phenanthrene-d10 (I)

17.164min (-0.005) 0.40ng/ul m 10/6/20 JU

response 6584

Ion	Exp%	Act%
188.00	100	100
94.00	5.20	3.94#
80.00	6.20	4.50#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM100520\
Quantitation Report (QT Reviewed)

Data File : BM027625.D
Acq On : 06 Oct 2020 03:02
Operator : JU/CG
Sample : L4184-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AM1

Manual Integrations
APPROVED

mohammad
10/6/2020 3:24:29 PM

Quant Time: Oct 06 03:41:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 06 01:23:11 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	1004	0.40	ng/ul	0.00
2) Naphthalene-d8	10.58	136	2817	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.42	164	2368	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.16	188	6584m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.34	240	10460	0.40	ng/ul	0.00
20) Perylene-d12	23.60	264	11581	0.40	ng/ul	0.00

10/6/2020 JU

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev (Min)
4) 2-Methylnaphthalene-d10	12.17	152	1340	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.19	212	5287	0.29	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed