

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100520\
 Data File : BM027622.D
 Acq On : 06 Oct 2020 01:14
 Operator : JU/CG
 Sample : L4184-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AN7

Manual Integrations
 APPROVED

mohammad
 10/6/2020 3:24:20 PM

Quant Time: Oct 06 03:30:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 06 01:23:11 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	1742	0.40	ng/ul	0.00
2) Naphthalene-d8	10.579	136	4971	0.40	ng/ul	# 0.00
6) Acenaphthene-d10	14.423	164	3717	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.164	188	9040m	0.40	ng/ul	0.00
16) Chrysene-d12	21.343	240	9943	0.40	ng/ul	0.00
20) Perylene-d12	23.600	264	10823	0.40	ng/ul	# 0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.167	152	2755	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.190	212	8430	0.34	ng/ul	0.00
Target Compounds						Qvalue
15) Fluoranthene	19.221	202	711	0.02	ng/ul	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100520\
Data File : BM027622.D
Acq On : 06 Oct 2020 01:14
Operator : JU/CG
Sample : L4184-10
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AN7

Manual Integrations
APPROVED


mohammad
10/6/2020 3:24:20 PM

Quant Time: Oct 06 03:30:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 06 01:23:11 2020
Response via : Initial Calibration


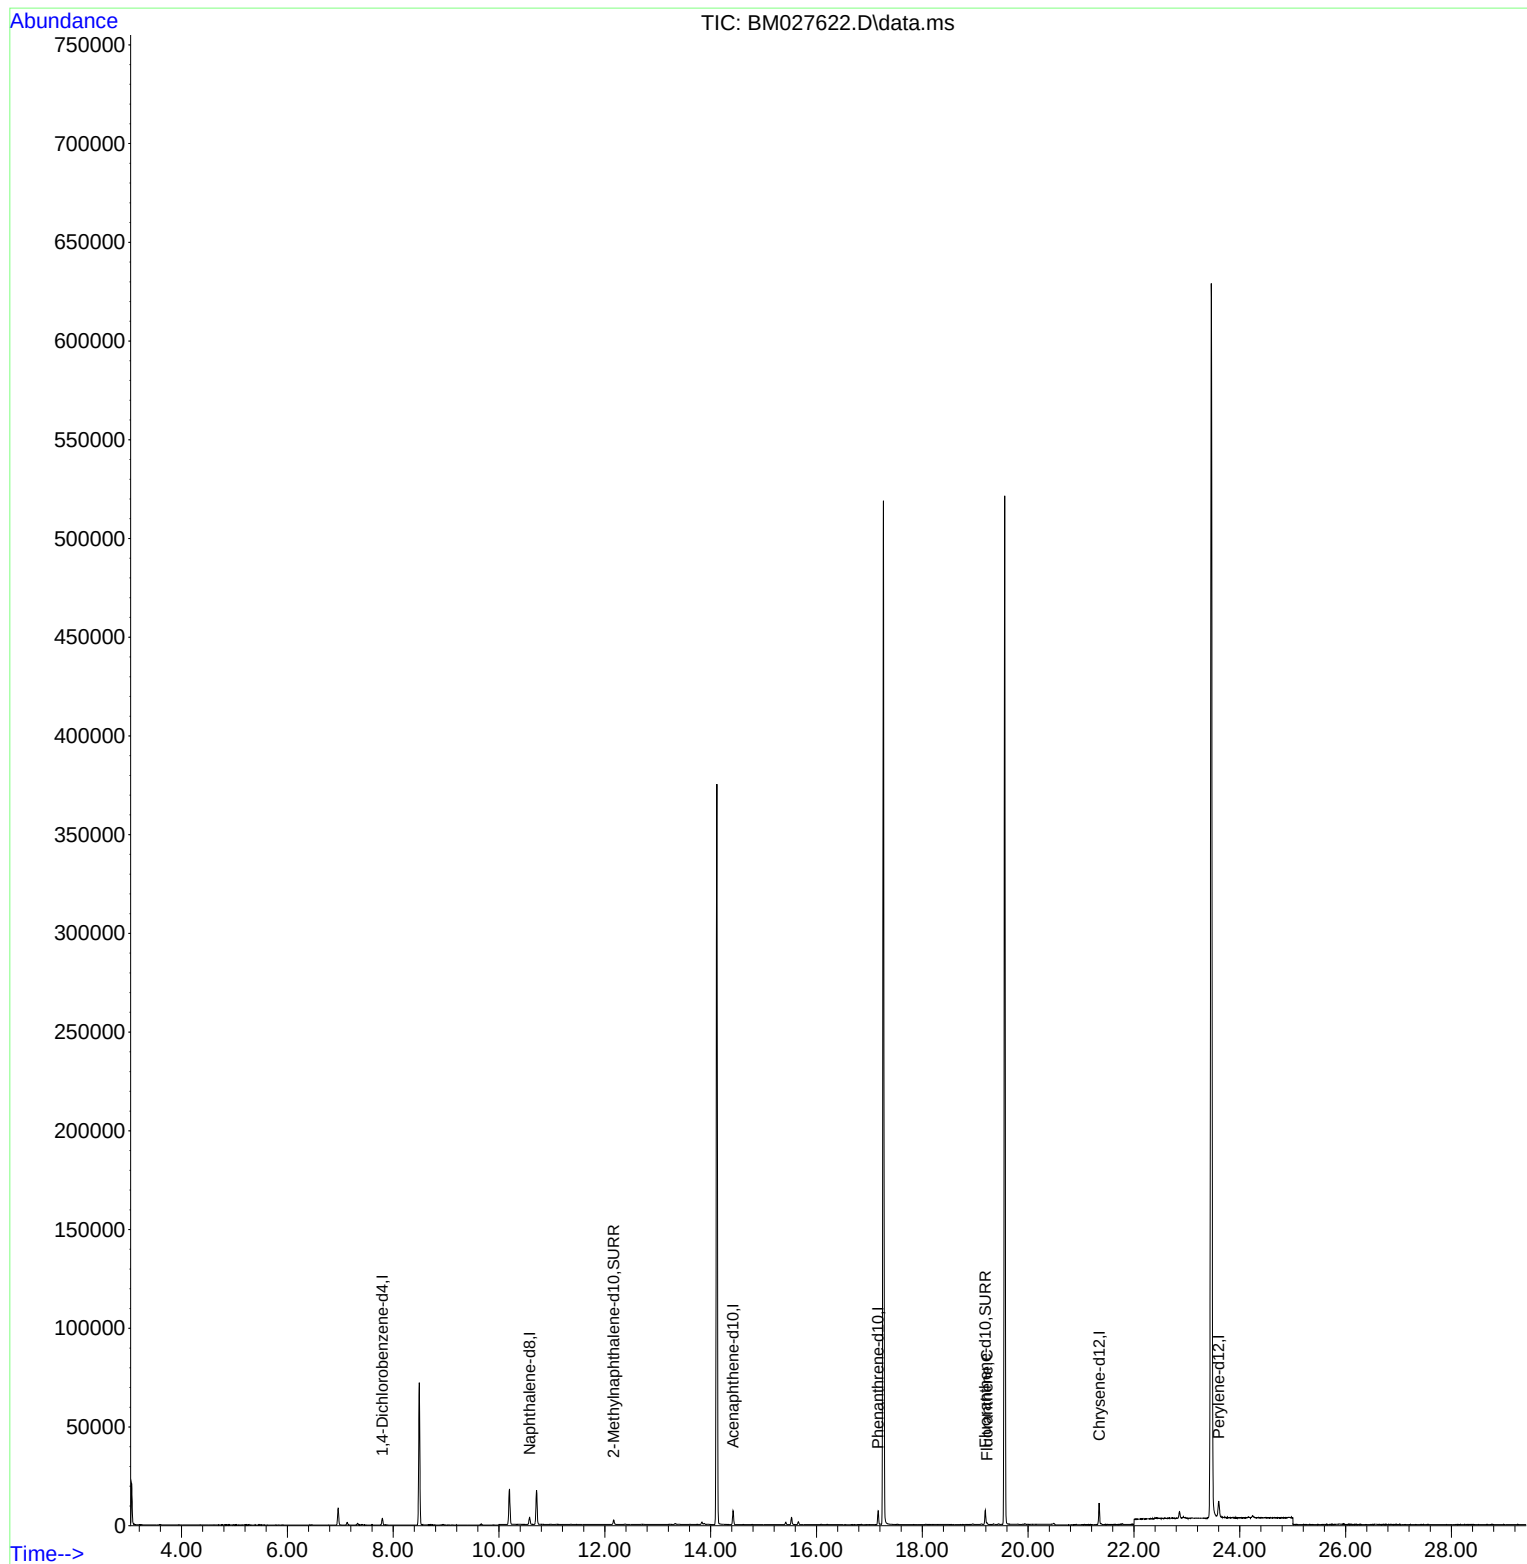


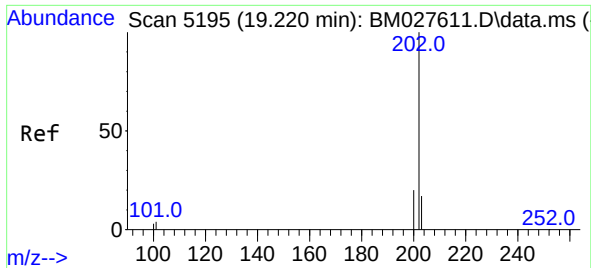

#15
 Fluoranthene
 Concen: 0.02 ng/ul
 RT: 19.221 min Scan# 5195
 Delta R.T. -0.002 min
 Lab File: BM027622.D
 Acq: 06 Oct 2020 01:14

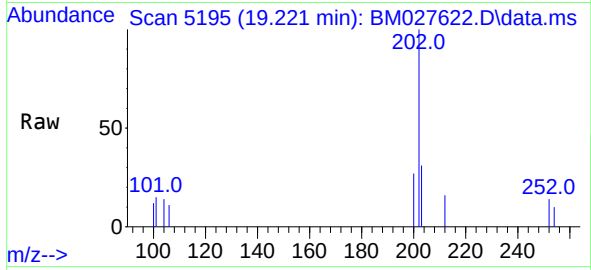

Tgt Ion:	202	Resp:	711
Ion	Ratio	Lower	Upper
202	100		
101	15.2	0.0	24.9
100	12.0	0.0	24.1

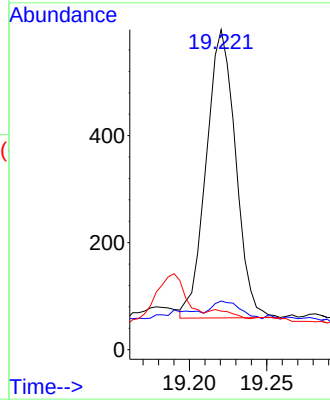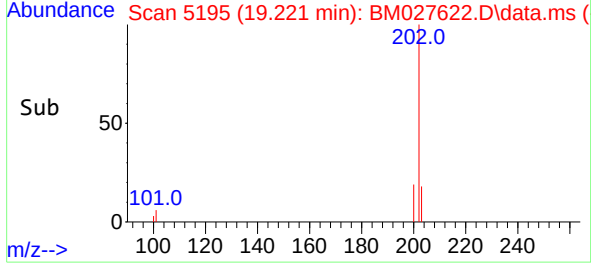

Instrument :
 BNA_M
 ClientSampleId :
 C0AN7

Manual Integrations
 APPROVED

mohammad
 10/6/2020 3:24:20 PM