


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100520\
 Data File : BM027597.D
 Acq On : 05 Oct 2020 08:47
 Operator : JU/CG
 Sample : DFTPP86
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP86

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 05 10:43:07 2020

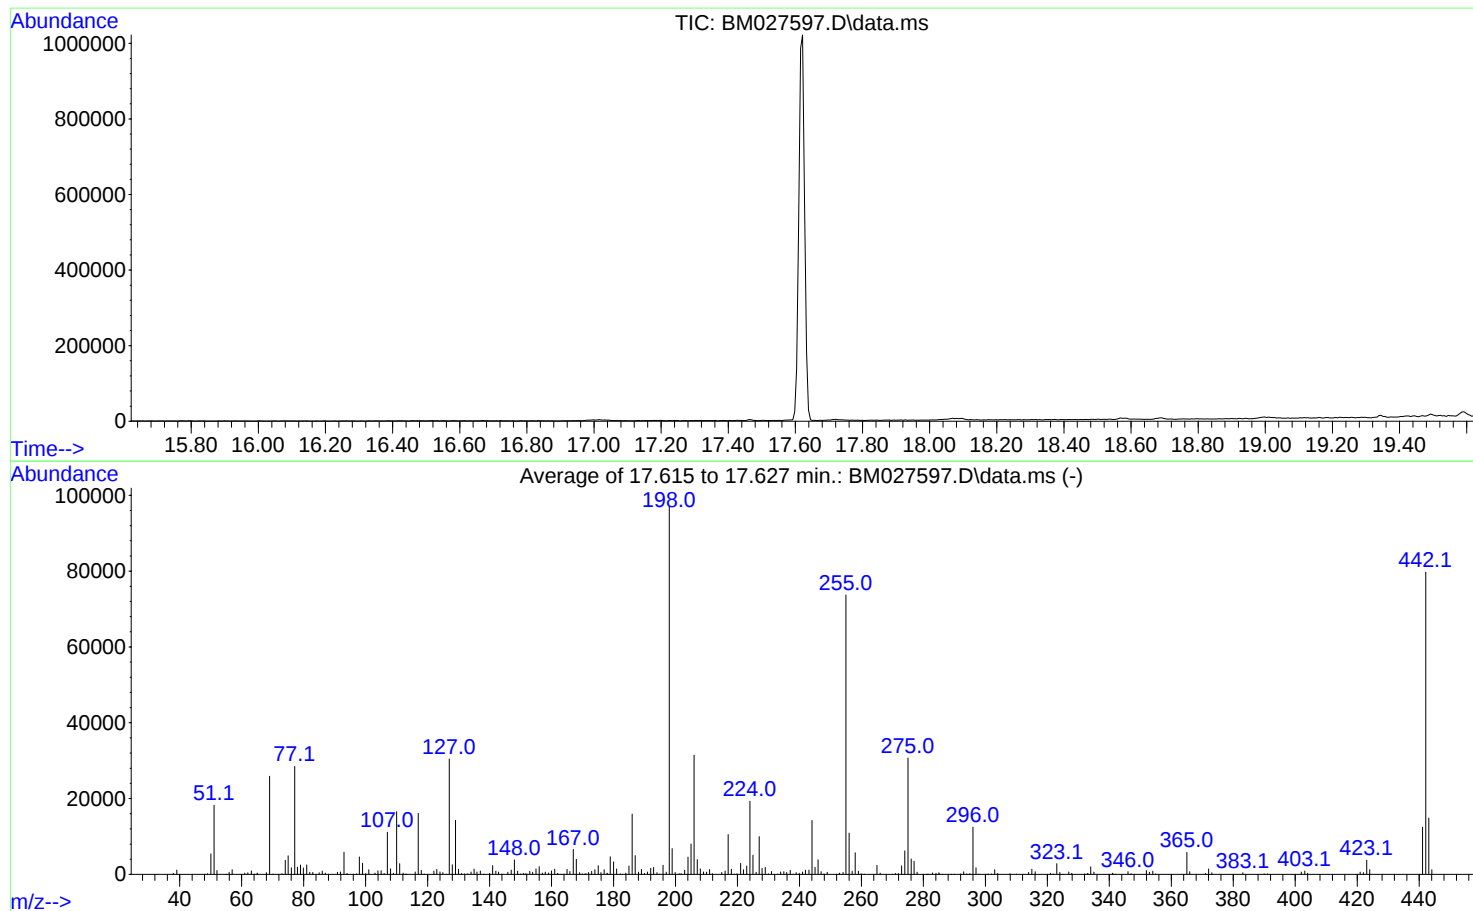

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.8	18249	PASS
68	69	0.00	2	1.8	477	PASS
69	198	0.00	100	26.6	25863	PASS
70	69	0.00	2	0.3	74	PASS
127	198	10	80	31.4	30456	PASS
197	198	0.00	2	0.6	587	PASS
198	198	100	100	100.0	97053	PASS
199	198	5	9	7.0	6808	PASS
275	198	10	60	31.6	30685	PASS
365	198	1	100	6.0	5789	PASS
441	198	0.01	100	12.8	12460	PASS
442	198	50	100	82.2	79731	PASS
443	442	15	24	18.7	14878	PASS

m/z	Abundance
73.00	363.0
147.10	225.0
193.00	228.0
207.00	1122.0
208.00	187.0
281.10	364.0
282.00	172.0
354.90	165.0

Instrument :
BNA_M
ClientSampleId :
DFTPP86

m/z	Abundance
37.90	464.0
39.00	1542.0
49.00	267.0
50.00	7408.0
51.10	24224.0
52.00	1484.0
56.00	729.0
57.00	1535.0
61.00	502.0
62.00	603.0
63.10	1230.0
64.00	194.0
65.00	526.0
68.10	629.0
69.00	33984.0
70.10	222.0
73.00	682.0
74.00	4869.0
75.00	6438.0
76.00	2073.0
77.10	36176.0
78.00	2498.0
79.00	3344.0
79.90	2377.0
81.00	2783.0
81.90	611.0
83.00	776.0
85.00	540.0
86.00	1072.0
86.90	309.0
90.90	765.0
91.90	809.0
93.00	7058.0
94.00	403.0
97.10	171.0
98.00	6073.0
99.00	3945.0
100.00	307.0
101.00	1173.0
103.10	517.0
103.90	1199.0
105.00	1112.0
106.00	517.0
107.00	14015.0
108.10	1982.0
109.00	443.0
110.00	20544.0
111.00	3648.0
112.20	526.0
113.10	188.0
116.10	823.0
117.00	19616.0
117.90	1164.0
122.00	1101.0
122.90	1739.0
124.10	824.0
124.90	452.0
127.00	37752.0
128.00	2808.0
129.00	17696.0
130.00	1426.0
130.90	247.0
131.90	178.0
133.00	165.0
134.00	576.0
135.00	1575.0
136.00	737.0
137.00	1144.0
138.10	182.0
140.00	451.0
141.00	2618.0
142.00	1031.0
142.90	660.0
144.00	251.0
145.90	780.0
147.00	1525.0
148.00	4829.0
149.10	840.0
149.90	269.0
150.90	449.0
151.70	172.0
152.90	902.0
153.90	606.0
155.00	2186.0
156.00	2531.0
157.10	382.0
157.90	698.0
159.00	443.0
160.00	1194.0
161.00	1625.0
161.90	474.0
165.00	1604.0

Instrument :
BNA_M
ClientSampleId :
DFTPP86

165.90	846.0
167.00	7633.0
168.00	4737.0
169.00	529.0
169.90	229.0
171.10	348.0
171.90	534.0
173.00	758.0
174.00	1641.0
175.10	2558.0
175.90	411.0
177.00	1282.0
177.90	688.0
178.90	5648.0
180.00	3710.0
181.00	1945.0
182.20	174.0
182.90	179.0
184.00	400.0
185.00	2889.0
186.00	18576.0
187.10	6047.0
188.10	846.0
189.00	1187.0
190.10	254.0
191.00	692.0
192.00	1855.0
192.90	2179.0
194.00	388.0
195.00	161.0
196.00	2624.0
197.00	599.0
198.00	112760.0
198.90	8049.0
199.90	568.0
201.50	332.0
203.00	1436.0
204.10	4949.0
205.00	9680.0
206.00	37352.0
207.00	5658.0
208.00	1892.0
209.00	683.0
210.00	640.0
211.10	1381.0
211.90	282.0
215.00	491.0
216.00	989.0
217.00	12397.0
218.00	1326.0
218.90	214.0
219.80	164.0
221.00	3677.0
222.00	1444.0
223.00	2531.0
224.00	21704.0
225.00	6095.0
226.10	767.0
227.00	10711.0
227.90	1803.0
228.90	1751.0
230.00	290.0
231.00	885.0
233.00	296.0
233.90	812.0
235.00	954.0
235.90	639.0
237.00	1179.0
239.00	508.0
239.90	237.0
240.90	649.0
242.00	1048.0
243.10	1480.0
244.00	15598.0
245.10	2368.0
246.00	4172.0
247.10	771.0
247.90	236.0
249.00	636.0
252.90	421.0
254.10	639.0
255.00	81832.0
256.00	12063.0
257.00	1233.0
258.00	6246.0
259.00	1067.0
260.00	217.0
260.90	209.0
265.00	2484.0
266.10	306.0
271.00	210.0
271.90	218.0
273.00	2407.0
274.00	6326.0
275.00	32584.0
276.10	4693.0

Instrument :
BNA_M
ClientSampleId :
DFTPP86

277.00	3660.0
277.90	765.0
281.20	326.0
281.80	163.0
282.90	312.0
284.10	275.0
285.00	675.0
286.10	153.0
290.00	183.0
291.90	299.0
293.00	662.0
293.90	217.0
294.90	178.0
296.00	13330.0
297.00	2021.0
300.90	153.0
302.10	180.0
303.00	1115.0
303.80	203.0
307.90	172.0
310.10	228.0
313.90	423.0
315.00	1255.0
316.10	692.0
321.00	272.0
323.10	2714.0
324.00	568.0
326.90	666.0
327.80	286.0
332.90	295.0
334.00	2022.0
335.00	714.0
341.00	415.0
342.00	174.0
346.00	612.0
347.00	199.0
352.00	957.0
353.00	599.0
354.00	912.0
354.90	180.0
365.00	5632.0
366.00	908.0
370.90	225.0
372.10	1345.0
373.00	458.0
383.20	378.0
389.90	234.0
391.10	156.0
401.90	415.0
403.10	670.0
404.00	312.0
421.10	620.0
422.00	514.0
423.10	3401.0
424.10	1287.0
441.10	10703.0
442.10	72272.0
443.10	14363.0
444.00	1516.0

Instrument :
BNA_M
ClientSampleId :
DFTPP86

m/z	Abundance
38.10	248.0
39.10	1394.0
49.00	244.0
50.10	5950.0
51.10	20624.0
52.00	1011.0
55.00	173.0
55.90	540.0
56.90	1471.0
61.00	365.0
62.00	401.0
63.10	1068.0
65.00	520.0
68.00	537.0
69.00	29976.0
73.00	545.0
74.10	3795.0
75.00	5352.0
76.10	1988.0
77.10	33288.0
78.00	2155.0
79.00	2920.0
79.90	1824.0
81.00	3385.0
82.00	675.0
82.90	572.0
85.10	543.0
86.00	968.0
87.00	380.0
88.00	174.0
90.90	586.0
91.90	764.0
93.00	6707.0
94.00	339.0
96.00	192.0
97.00	157.0
98.00	5045.0
99.00	3543.0
100.10	320.0
101.00	1656.0
103.00	478.0
104.00	970.0
105.00	1125.0
106.00	248.0
107.00	12841.0
108.00	1549.0
109.00	308.0
110.00	19448.0
111.00	3167.0
112.00	480.0
113.00	219.0
116.00	615.0
117.00	19408.0
118.00	1143.0
118.90	247.0
122.00	945.0
123.00	1460.0
123.90	629.0
125.00	633.0
127.00	34568.0
128.00	3179.0
129.00	16648.0
130.00	1768.0
130.80	296.0
132.00	209.0
133.00	153.0
134.00	835.0
135.00	1726.0
135.90	775.0
137.00	985.0
140.00	302.0
141.00	2698.0
142.10	1021.0
143.00	713.0
146.00	600.0
147.00	1901.0
148.00	4189.0
149.00	833.0
150.10	156.0
150.90	304.0
151.70	357.0
152.10	280.0
153.00	1007.0
153.90	555.0
155.00	1284.0
156.00	2220.0
157.00	351.0
158.00	769.0
159.10	454.0
160.00	1032.0
161.00	1519.0
162.10	361.0

Instrument :
BNA_M
ClientSampleId :
DFTPP86

163.10	159.0
164.00	228.0
165.00	1429.0
166.00	811.0
167.00	7562.0
168.00	4841.0
169.10	603.0
169.90	223.0
170.80	227.0
172.00	785.0
172.90	1105.0
174.00	1192.0
175.00	2454.0
176.00	749.0
176.90	1317.0
178.10	515.0
179.00	5426.0
180.00	3835.0
181.00	1465.0
182.20	162.0
184.00	441.0
185.00	2442.0
186.00	18384.0
187.00	5726.0
188.00	618.0
189.00	1773.0
189.90	329.0
190.90	855.0
192.00	2177.0
193.00	2620.0
194.00	705.0
194.90	155.0
195.90	2905.0
197.00	890.0
198.00	114416.0
198.90	7788.0
199.90	651.0
200.90	217.0
201.30	214.0
201.90	318.0
202.90	1246.0
204.00	5583.0
205.00	9878.0
206.00	36120.0
207.10	5805.0
208.00	1599.0
209.10	861.0
210.00	652.0
210.90	1536.0
212.00	237.0
214.90	501.0
216.00	1138.0
217.00	12760.0
218.00	1829.0
219.90	184.0
221.00	3253.0
221.90	1479.0
223.00	2698.0
224.00	22920.0
225.00	5914.0
226.00	631.0
227.00	12061.0
228.00	1635.0
229.00	2522.0
229.90	219.0
231.00	983.0
233.90	636.0
234.90	790.0
236.00	528.0
237.00	1091.0
237.90	176.0
238.90	645.0
239.90	413.0
241.00	716.0
241.90	1418.0
243.00	1224.0
244.10	16736.0
245.00	2125.0
246.00	4479.0
246.90	864.0
247.90	184.0
249.00	561.0
252.90	540.0
254.00	404.0
255.00	88792.0
256.00	13144.0
257.00	827.0
258.00	6757.0
259.00	1029.0
259.80	245.0
265.00	3003.0
265.90	450.0
271.00	296.0
272.00	223.0
272.90	2567.0
274.00	7882.0

Instrument :
BNA_M
ClientSampleId :
DFTPP86

275.00	36976.0
276.00	4501.0
277.00	4044.0
278.00	730.0
281.00	466.0
282.10	151.0
283.00	556.0
284.00	458.0
285.00	590.0
288.90	194.0
292.10	153.0
293.00	822.0
294.00	179.0
295.10	269.0
296.00	14110.0
296.90	2035.0
300.90	243.0
303.00	1376.0
304.00	424.0
314.00	638.0
315.00	1617.0
316.00	1027.0
321.10	393.0
321.90	264.0
323.00	3258.0
324.10	653.0
325.00	162.0
326.90	755.0
327.90	483.0
332.10	329.0
333.10	551.0
334.00	2401.0
335.00	614.0
341.20	332.0
346.00	795.0
347.00	183.0
352.00	1187.0
352.90	662.0
354.00	1037.0
355.00	391.0
365.00	6903.0
366.00	613.0
371.00	263.0
372.00	1693.0
373.10	446.0
383.00	619.0
390.00	194.0
391.00	226.0
402.00	858.0
403.00	1163.0
404.00	304.0
420.90	711.0
421.90	502.0
423.00	4477.0
424.00	1376.0
441.10	16110.0
442.10	96200.0
443.10	17760.0
444.10	1418.0

Instrument :
BNA_M
ClientSampleId :
DFTPP86

m/z	Abundance
38.00	286.0
39.00	505.0
50.10	2851.0
51.10	9898.0
52.00	503.0
56.00	373.0
56.90	713.0
60.90	155.0
61.90	223.0
63.10	473.0
65.20	269.0
67.90	264.0
69.00	13628.0
72.90	395.0
74.00	2443.0
75.00	2859.0
76.00	1169.0
77.10	16044.0
78.00	1068.0
79.00	1130.0
80.00	925.0
81.00	1307.0
81.90	321.0
83.00	239.0
84.90	247.0
86.00	565.0
87.10	285.0
90.90	304.0
92.00	390.0
93.00	3853.0
94.20	155.0
98.00	2643.0
99.00	1392.0
101.00	890.0
102.80	191.0
104.00	610.0
105.00	683.0
107.00	6454.0
108.00	873.0
109.10	177.0
110.00	9669.0
111.00	1638.0
115.90	423.0
117.00	9239.0
117.90	870.0
122.10	687.0
123.00	762.0
123.90	404.0
124.90	368.0
126.10	173.0
127.00	19048.0
128.00	1569.0
129.00	8450.0
130.10	850.0
131.00	151.0
133.00	166.0
134.00	451.0
134.90	854.0
135.90	356.0
137.00	519.0
140.90	1677.0
141.90	447.0
142.80	350.0
145.80	279.0
147.00	702.0
148.00	2370.0
149.00	839.0
151.10	194.0
152.90	539.0
154.00	370.0
154.90	869.0
156.00	1331.0
157.00	229.0
158.00	274.0
159.10	292.0
159.90	611.0
160.90	881.0
162.00	229.0
164.90	860.0
165.90	587.0
167.00	4532.0
167.90	2363.0
169.00	231.0
171.10	272.0
171.90	260.0
173.00	561.0
174.00	870.0
175.00	1800.0
175.90	188.0
177.00	1090.0
177.90	312.0
179.00	2852.0

Instrument :
BNA_M
ClientSampleId :
DFTPP86

180.00	2308.0
181.00	860.0
183.80	238.0
185.10	1327.0
186.00	10742.0
186.90	3007.0
188.20	353.0
189.00	979.0
189.90	181.0
190.90	406.0
191.90	846.0
193.00	1292.0
194.00	287.0
196.00	1674.0
197.00	273.0
198.00	63984.0
199.00	4588.0
200.00	317.0
201.80	230.0
202.90	629.0
204.00	3158.0
205.00	4514.0
206.00	20928.0
207.00	3507.0
208.00	1352.0
209.00	416.0
210.00	510.0
211.00	886.0
211.80	179.0
214.90	517.0
216.00	522.0
217.00	6372.0
218.00	867.0
221.00	1820.0
221.90	777.0
223.00	1365.0
224.00	13249.0
225.00	3139.0
226.00	294.0
227.00	7172.0
228.00	1314.0
228.90	1293.0
231.10	456.0
233.90	462.0
234.90	478.0
235.80	385.0
237.00	922.0
238.90	257.0
240.00	206.0
241.10	384.0
242.00	837.0
243.10	785.0
244.10	10316.0
245.00	1098.0
246.00	2920.0
247.00	589.0
248.90	456.0
252.00	153.0
253.10	300.0
254.00	440.0
255.00	50456.0
256.00	7469.0
256.90	480.0
258.00	4075.0
258.90	500.0
265.00	1612.0
266.10	255.0
270.00	173.0
270.90	210.0
271.90	226.0
273.00	1777.0
274.00	4457.0
275.00	22496.0
276.00	3017.0
277.00	2691.0
277.90	326.0
281.00	360.0
282.90	319.0
284.10	224.0
285.20	400.0
293.00	552.0
294.90	172.0
296.00	9980.0
297.00	1154.0
297.90	153.0
301.90	199.0
303.00	1153.0
304.00	249.0
307.90	283.0
314.00	402.0
315.00	1242.0
316.00	499.0
321.00	278.0
323.10	2533.0
324.10	323.0
327.00	448.0

Instrument :
BNA_M
ClientSampleId :
DFTPP86

328.10	157.0
332.90	343.0
334.00	1586.0
335.00	489.0
341.00	448.0
346.00	757.0
347.00	220.0
351.90	933.0
352.90	415.0
353.90	607.0
355.10	267.0
365.00	4831.0
365.90	617.0
371.10	278.0
372.00	1303.0
373.00	353.0
383.10	299.0
402.00	558.0
403.10	778.0
404.00	300.0
420.90	498.0
422.00	422.0
423.10	3378.0
424.10	1071.0
441.10	10566.0
442.10	70720.0
443.10	12510.0
444.10	742.0

Instrument :
BNA_M
ClientSampleId :
DFTPP86