
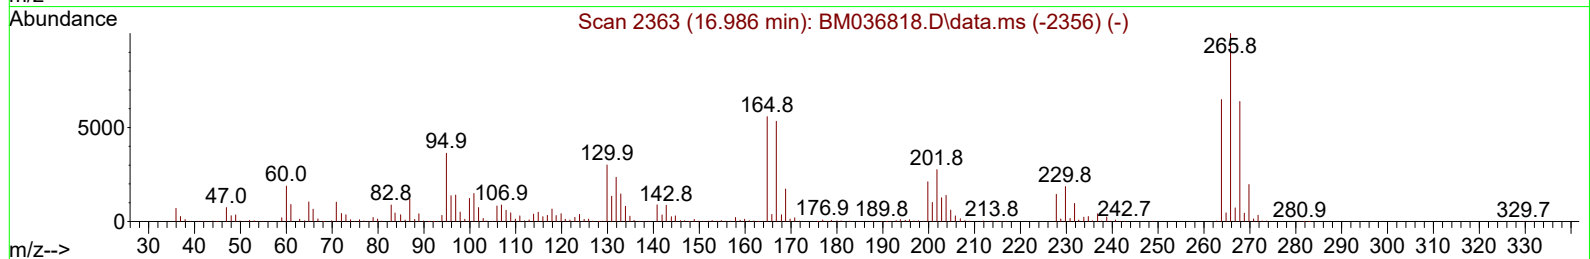
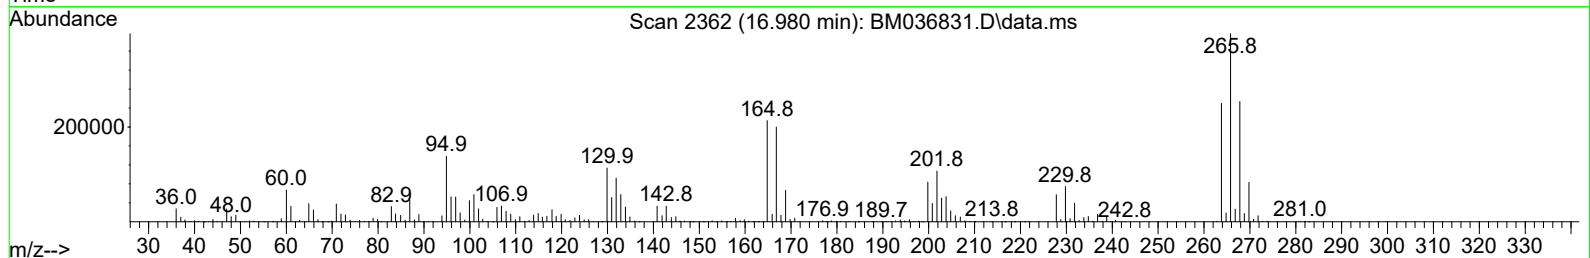


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100522\
Data File : BM036831.D
Acq On : 05 Oct 2022 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 04:45:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 03:17:03 2022
Response via : Initial Calibration

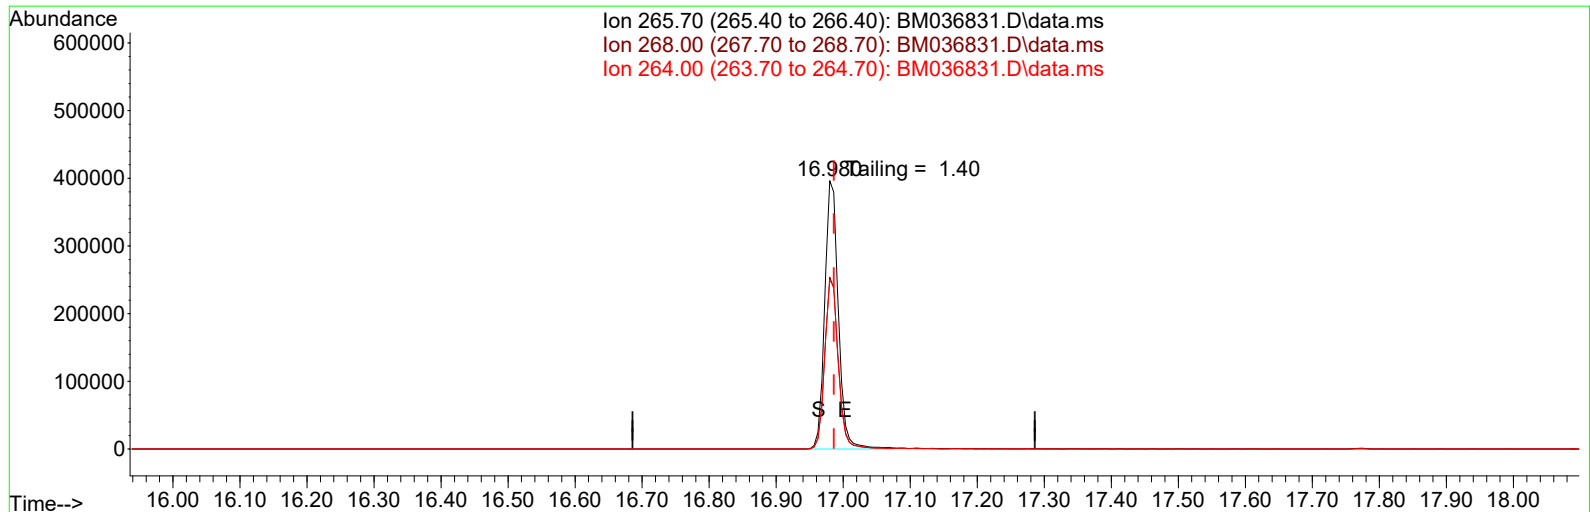

TIC: BM036831.D\data.ms

(70) Pentachlorophenol (C)




16.980min (-0.006) 1638510.00 ng

response 564785

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.03
264.00	64.90	63.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100522\
Data File : BM036831.D
Acq On : 05 Oct 2022 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 04:45:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 03:17:03 2022
Response via : Initial Calibration

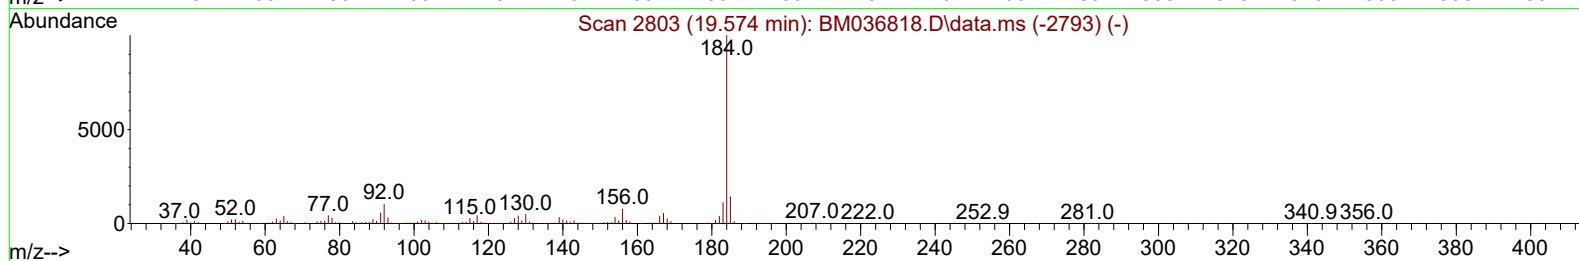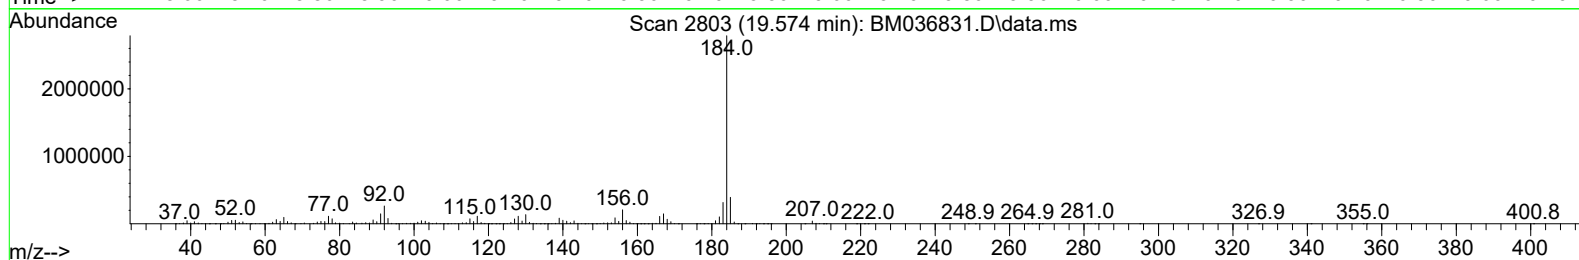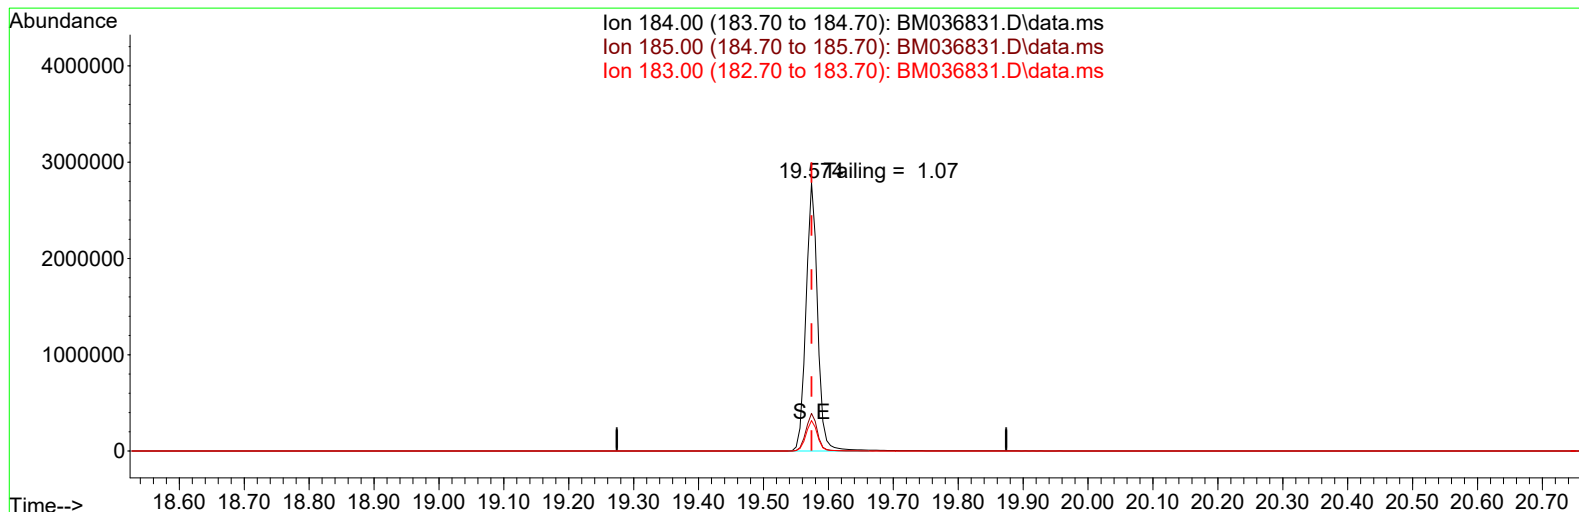

TIC: BM036831.D\data.ms

(77) Benzidine**19.574min (-0.000) 462945.62 ng****response 3496663**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.01
183.00	11.10	11.35
0.00	0.00	0.00