
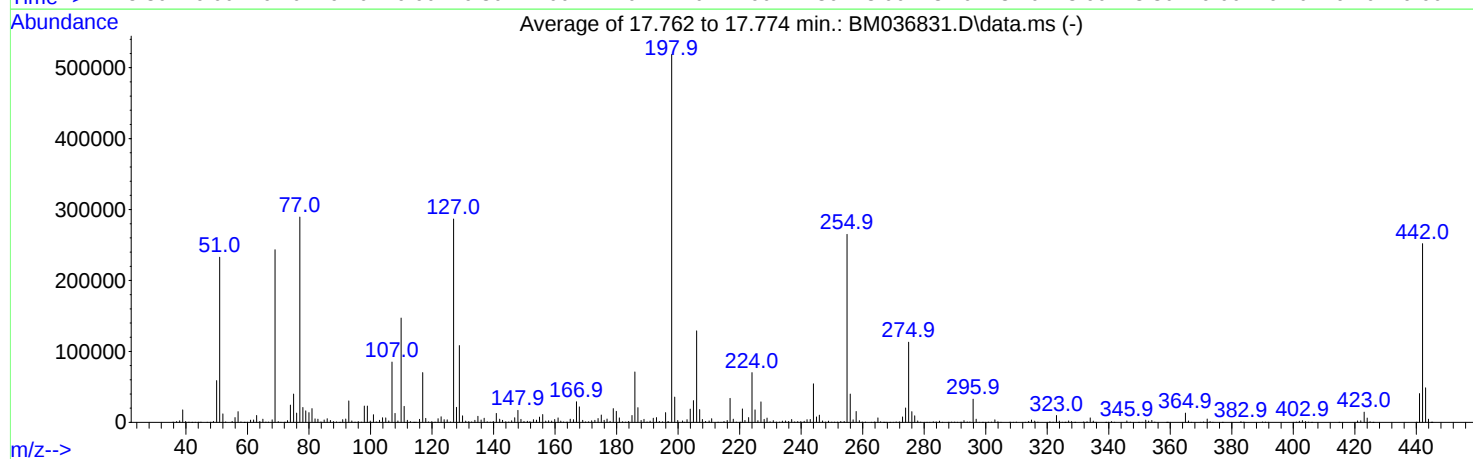


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100522\
 Data File : BM036831.D
 Acq On : 05 Oct 2022 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 04 03:17:03 2022

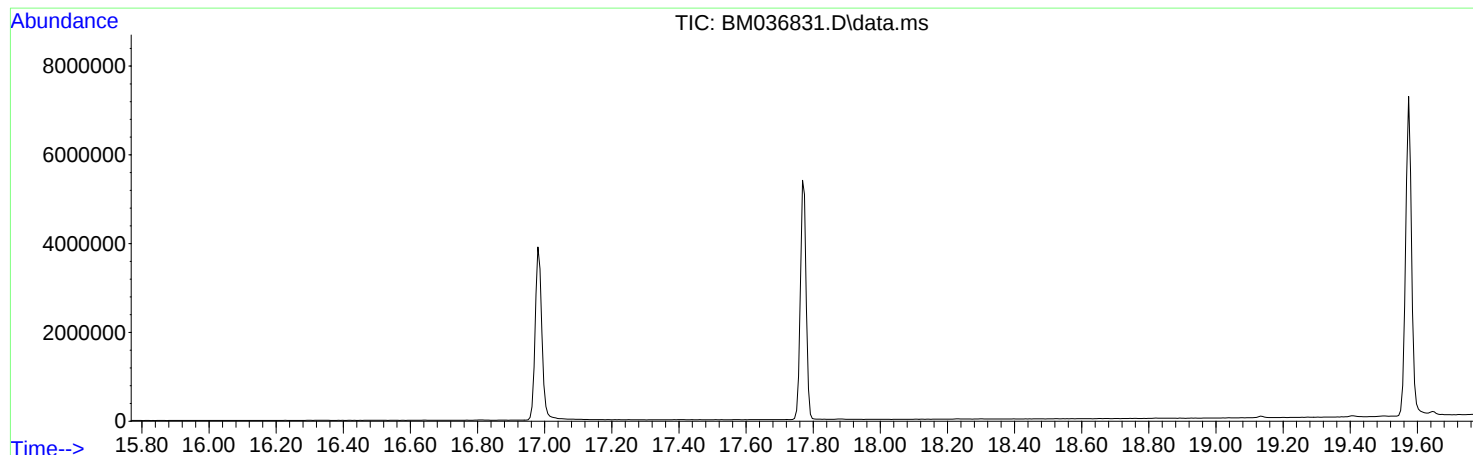




AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	232849	PASS
68	69	0.00	2	1.5	3612	PASS
69	198	0.00	100	46.9	243392	PASS
70	69	0.00	2	0.5	1201	PASS
127	198	10	80	55.3	286699	PASS
197	198	0.00	2	0.2	1238	PASS
198	198	100	100	100.0	518571	PASS
199	198	5	9	6.9	35723	PASS
275	198	10	60	21.8	113043	PASS
365	198	1	100	2.5	13036	PASS
441	198	0.01	100	7.9	40717	PASS
442	442	50	100	100.0	251976	PASS
443	442	15	24	19.3	48664	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100522\
Data File : BM036831.D
Acq On : 05 Oct 2022 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 06 04:45:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 03:17:03 2022
Response via : Initial Calibration

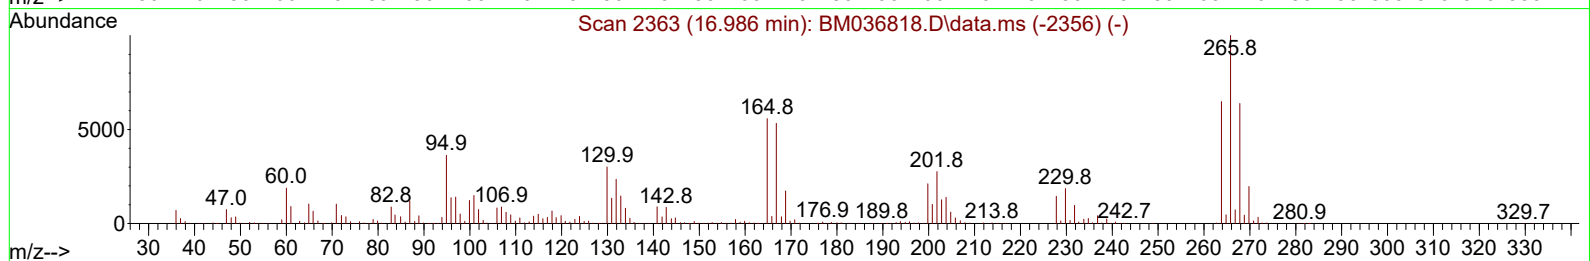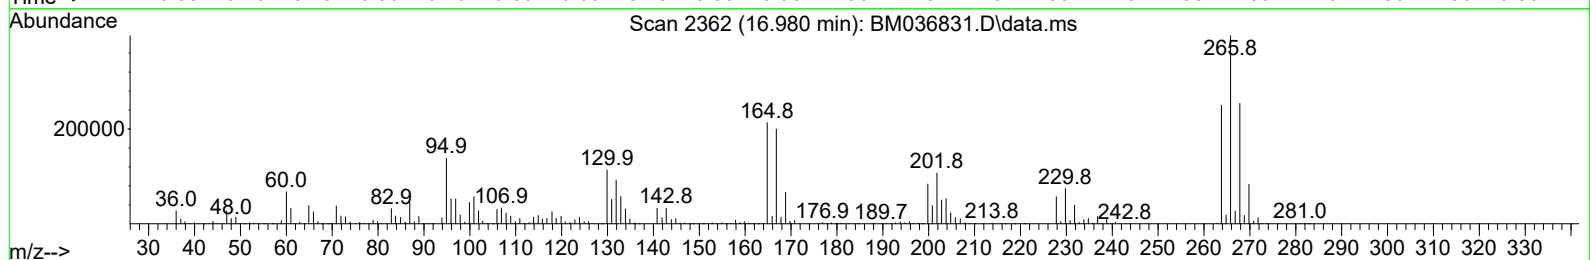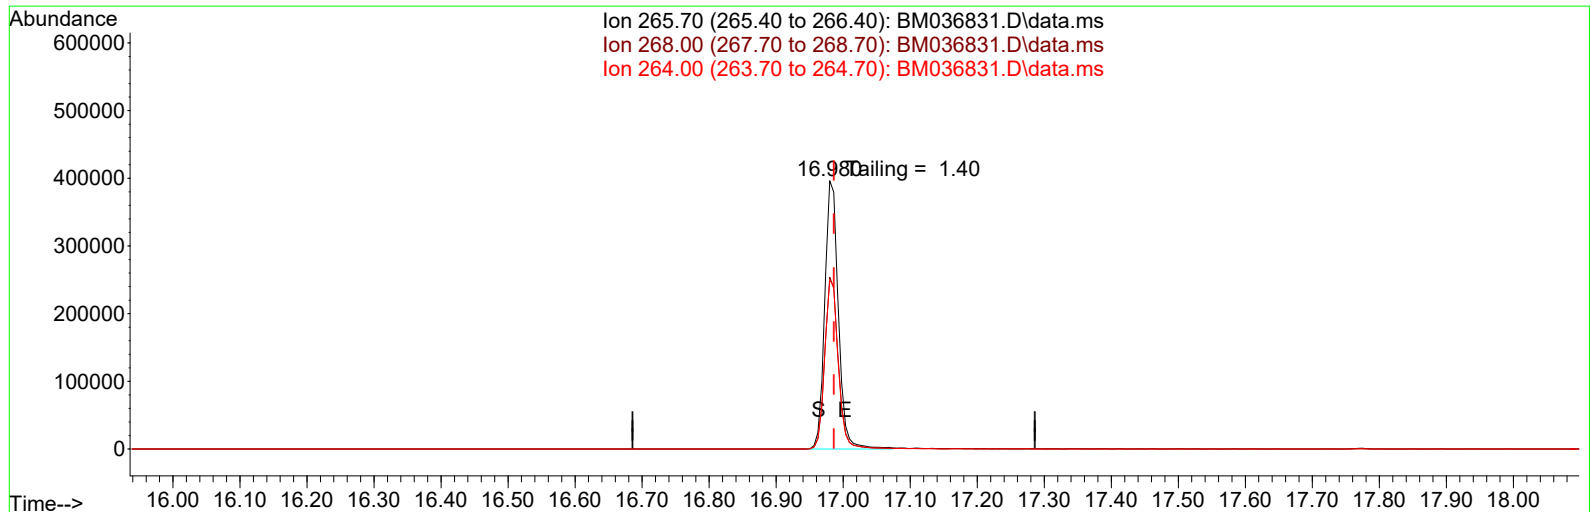

TIC: BM036831.D\data.ms

(70) Pentachlorophenol (C)

16.980min (-0.006) 1638510.00 ng




response 564785

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.03
264.00	64.90	63.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100522\
Data File : BM036831.D
Acq On : 05 Oct 2022 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 06 04:45:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 04 03:17:03 2022
Response via : Initial Calibration

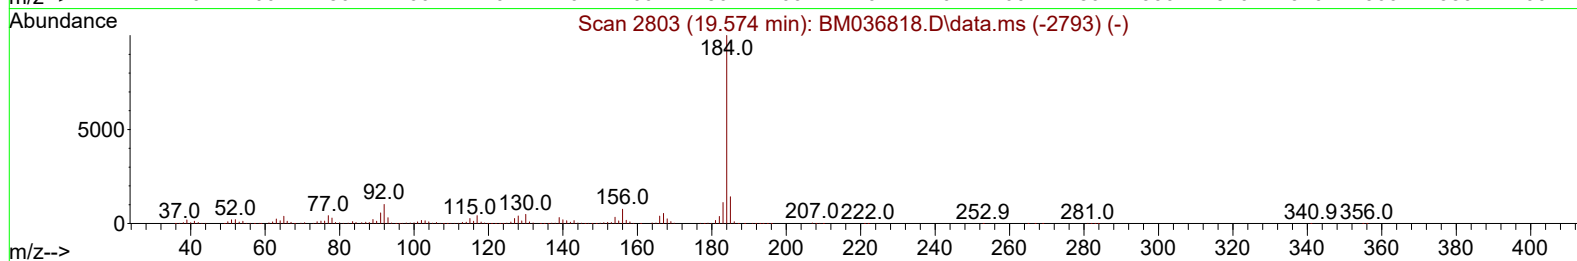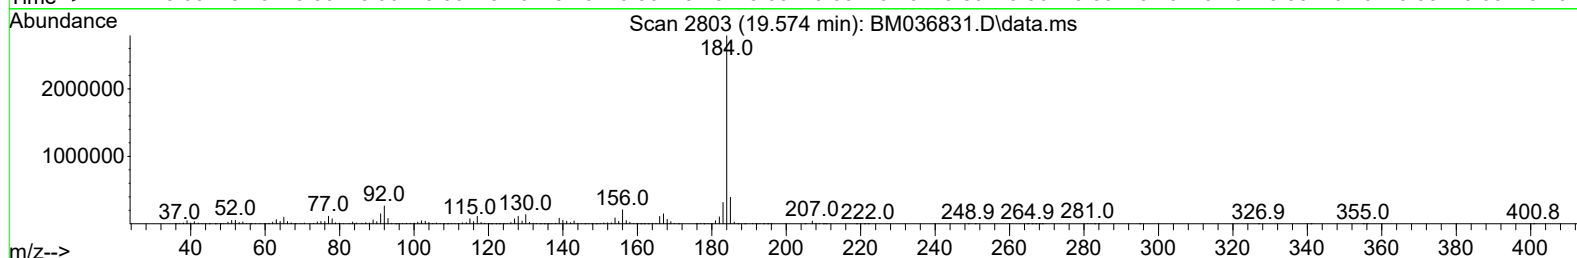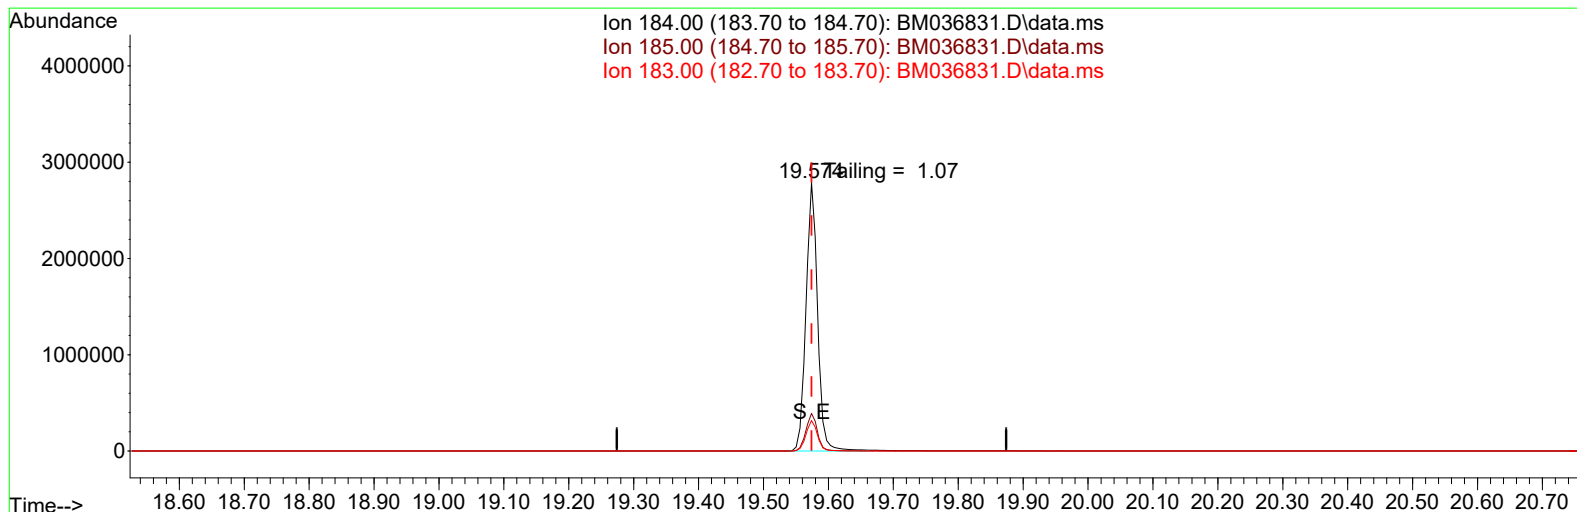

TIC: BM036831.D\data.ms

(77) Benzidine

19.574min (-0.000) 462945.62 ng

response 3496663

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.01
183.00	11.10	11.35
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/5/2022	BNA_M	<u>BM036831.D</u>
Compound Name	Response	Retention Time
DDT	1624179	20.803
DDD	11882	20.362
DDE	921	19.856
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12803	1636982	0.78

Instrument :
BNA_M
ClientSampleId :
DFTPP