

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100621\
 Data File : BM032344.D
 Acq On : 06 Oct 2021 16:30
 Operator : CG/JU
 Sample : M4003-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00T2

Quant Time: Oct 06 17:00:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 06 10:06:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.619	152	265553	20.000	ng/u1	0.00
20) Naphthalene-d8	10.407	136	1125924	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.266	164	733566	20.000	ng/u1	0.00
64) Phenanthrene-d10	16.995	188	1525203	20.000	ng/u1	0.00
79) Chrysene-d12	21.159	240	1496827	20.000	ng/u1	0.00
88) Perylene-d12	23.306	264	1487824	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.961	96	32191	4.860	ng/uL	0.00
4) Pyridine-d5	3.390	84	89893	4.804	ng/u1	0.00
7) Phenol-d5	6.801	99	182267	8.072	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.943	67	406778	31.374	ng/u1	0.00
11) 2-Chlorophenol-d4	7.154	132	454080	26.337	ng/u1	0.00
15) 4-Methylphenol-d8	8.343	113	326511	17.902	ng/u1	0.00
21) Nitrobenzene-d5	8.772	128	265719	33.449	ng/u1	0.00
24) 2-Nitrophenol-d4	9.495	143	275276	32.147	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.037	165	503495	29.537	ng/u1	0.00
31) 4-Chloroaniline-d4	10.542	131	573154	22.796	ng/u1	0.00
46) Dimethylphthalate-d6	13.672	166	1810790	35.669	ng/u1	0.00
49) Acenaphthylene-d8	13.954	160	2073899	33.627	ng/u1	0.00
54) 4-Nitrophenol-d4	14.466	143	62705	6.289	ng/u1	0.00
60) Fluorene-d10	15.254	176	1535809	35.671	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.372	200	238267	27.411	ng/u1	0.00
73) Anthracene-d10	17.089	188	2434280	36.666	ng/u1	0.00
81) Pyrene-d10	19.377	212	2771698	36.808	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.171	264	2602597	34.931	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.825	94	41985	1.835	ng/u1	95
16) Acetophenone	8.431	105	34242	1.282	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100621\
Data File : BM032344.D
Acq On : 06 Oct 2021 16:30
Operator : CG/JU
Sample : M4003-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00T2

Quant Time: Oct 06 17:00:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 06 10:06:22 2021
Response via : Initial Calibration




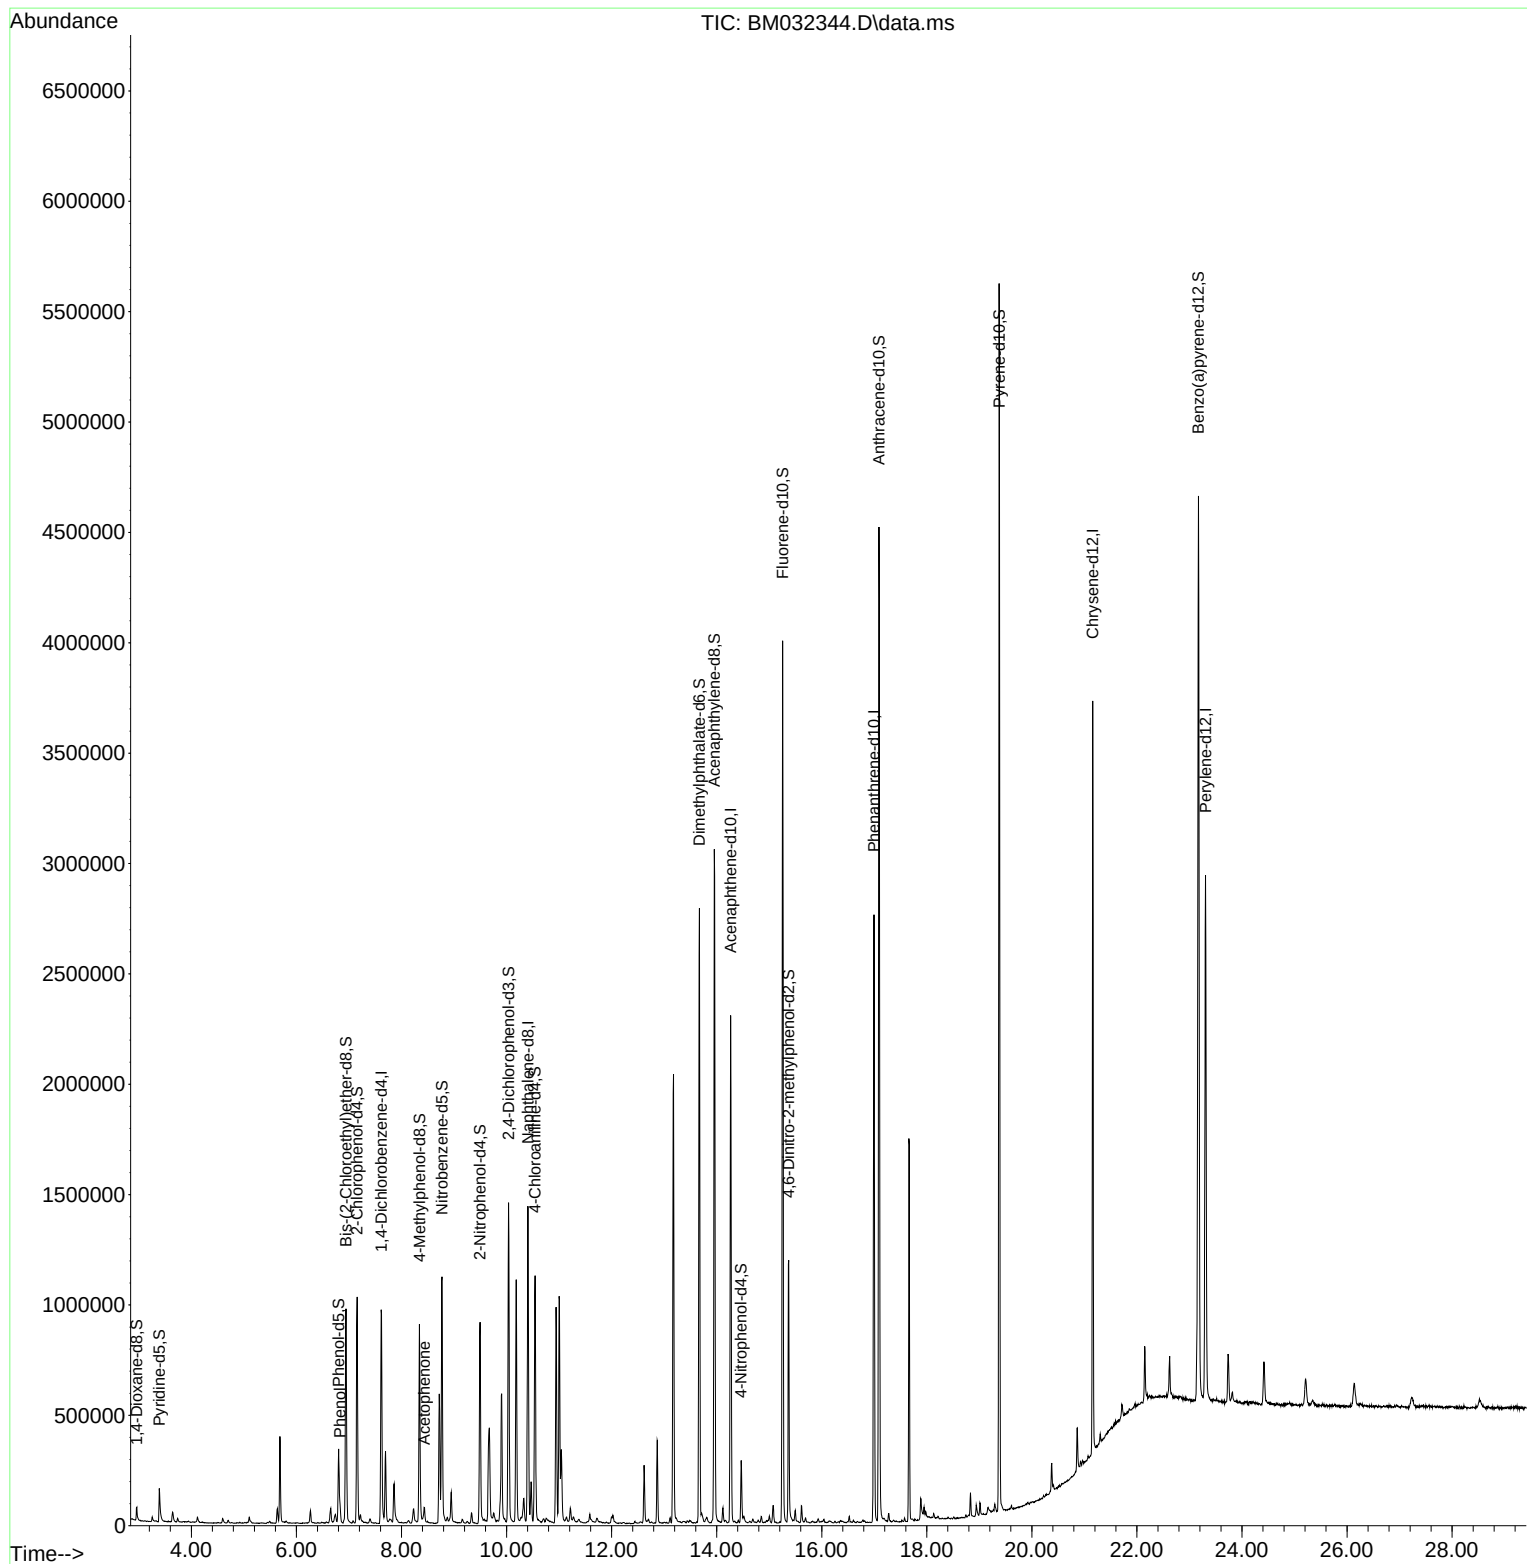


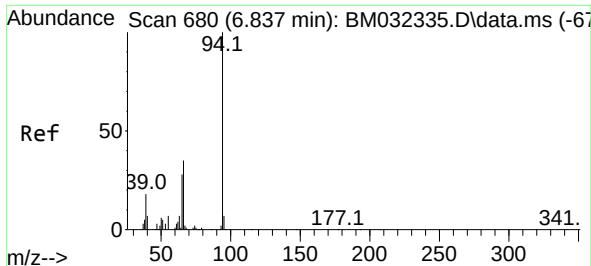

#8
Phenol
Concen: 1.835 ng/ul
RT: 6.825 min Scan# 678
Delta R.T. -0.012 min
Lab File: BM032344.D
Acq: 06 Oct 2021 16:30

Instrument :
BNA_M
ClientSampled :
C00T2

Tgt Ion: 94 Resp: 41985
Ion Ratio Lower Upper
94 100
65 27.5 22.3 33.5
66 41.5 29.5 44.3

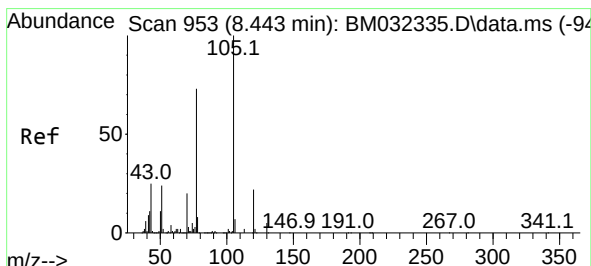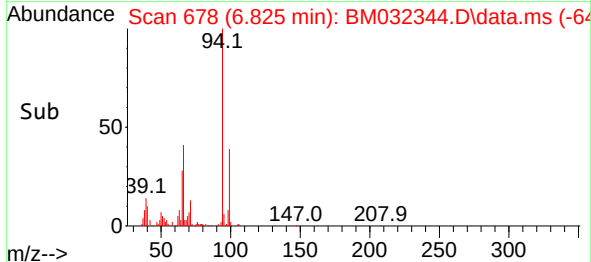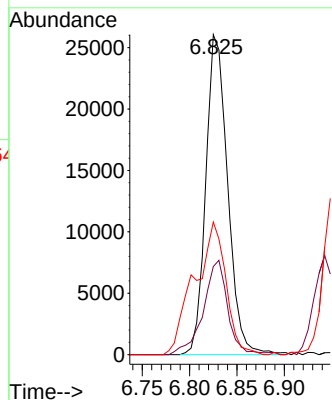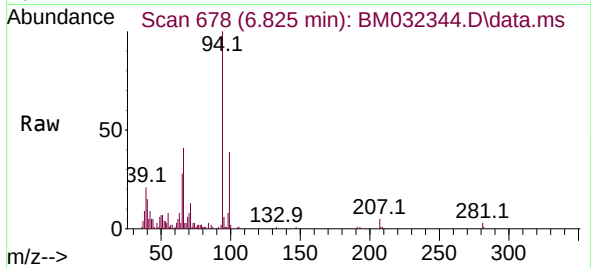

#16
Acetophenone
Concen: 1.282 ng/ul
RT: 8.431 min Scan# 951
Delta R.T. -0.012 min
Lab File: BM032344.D
Acq: 06 Oct 2021 16:30

Tgt Ion: 105 Resp: 34242
Ion Ratio Lower Upper
105 100
77 77.6 60.9 91.3
51 26.2 20.5 30.7

