

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100621\
 Data File : BM032336.D
 Acq On : 06 Oct 2021 09:25
 Operator : CG/JU
 Sample : PB139298BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK298

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Title : SVOA CALIBRATION

Signal : TIC: BM032336.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.960	17	21	33	rVB	60949	87511	1.56%	0.152%
2	3.384	90	93	111	rBV	720960	1155006	20.54%	2.009%
3	3.743	149	154	161	rVB	11620	18814	0.33%	0.033%
4	6.807	669	675	687	rBV	904200	1348976	23.99%	2.346%
5	6.948	693	699	707	rBV	718844	1095628	19.49%	1.906%
6	7.160	728	735	753	rBV	917904	1399831	24.90%	2.435%
7	7.625	806	814	831	rBV	771075	1229796	21.87%	2.139%
8	8.348	930	937	949	rBV	1105240	1708705	30.39%	2.972%
9	8.778	1001	1010	1020	rBV	813545	1292372	22.99%	2.248%
10	8.931	1033	1036	1042	rVB6	3912	7000	0.12%	0.012%
11	9.501	1125	1133	1148	rBV	655132	1039676	18.49%	1.808%
12	10.042	1215	1225	1240	rBV	1081101	1712536	30.46%	2.979%
13	10.413	1280	1288	1301	rBV	1122442	1832270	32.59%	3.187%
14	10.542	1301	1310	1329	rVV	1092222	1836794	32.67%	3.195%
15	11.730	1506	1512	1521	rVB4	7037	16519	0.29%	0.029%
16	12.001	1553	1558	1566	rBV2	15737	26178	0.47%	0.046%
17	13.672	1836	1842	1849	rBV	2127469	2811051	49.99%	4.890%
18	13.960	1884	1891	1900	rBV	2295025	3192911	56.79%	5.554%
19	14.271	1936	1944	1954	rBV	1794538	2562723	45.58%	4.458%
20	14.471	1971	1978	1996	rBV	953647	1317819	23.44%	2.292%
21	15.260	2105	2112	2125	rBV	2966278	4171831	74.20%	7.257%
22	15.371	2125	2131	2142	rBV	874398	1132751	20.15%	1.970%
23	15.495	2148	2152	2160	rVB2	23454	34196	0.61%	0.059%
24	15.924	2221	2225	2233	rVB7	4532	8662	0.15%	0.015%
25	16.036	2241	2244	2249	rVB6	4013	6700	0.12%	0.012%
26	16.789	2366	2372	2375	rBV3	6718	11554	0.21%	0.020%
27	16.995	2401	2407	2417	rBV	2314777	3163486	56.26%	5.503%
28	17.095	2417	2424	2442	rVV	3469388	4713507	83.83%	8.199%
29	18.942	2735	2738	2743	rBV3	27360	34690	0.62%	0.060%
30	19.012	2746	2750	2755	rVV	36182	49607	0.88%	0.086%
31	19.377	2806	2812	2826	rBV	4233411	5622665	100.00%	9.780%
32	21.159	3110	3115	3124	rBV	2845888	3590114	63.85%	6.245%
33	23.171	3450	3457	3465	rVB	3239078	5615059	99.86%	9.767%
34	23.300	3474	3479	3492	rVB2	2069020	3643551	64.80%	6.338%

Sum of corrected areas: 57490489

Instrument :

BNA_M

ClientSampleId :




SBLK298

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100621\
Data File : BM032336.D
Acq On : 06 Oct 2021 09:25
Operator : CG/JU
Sample : PB139298BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK298

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

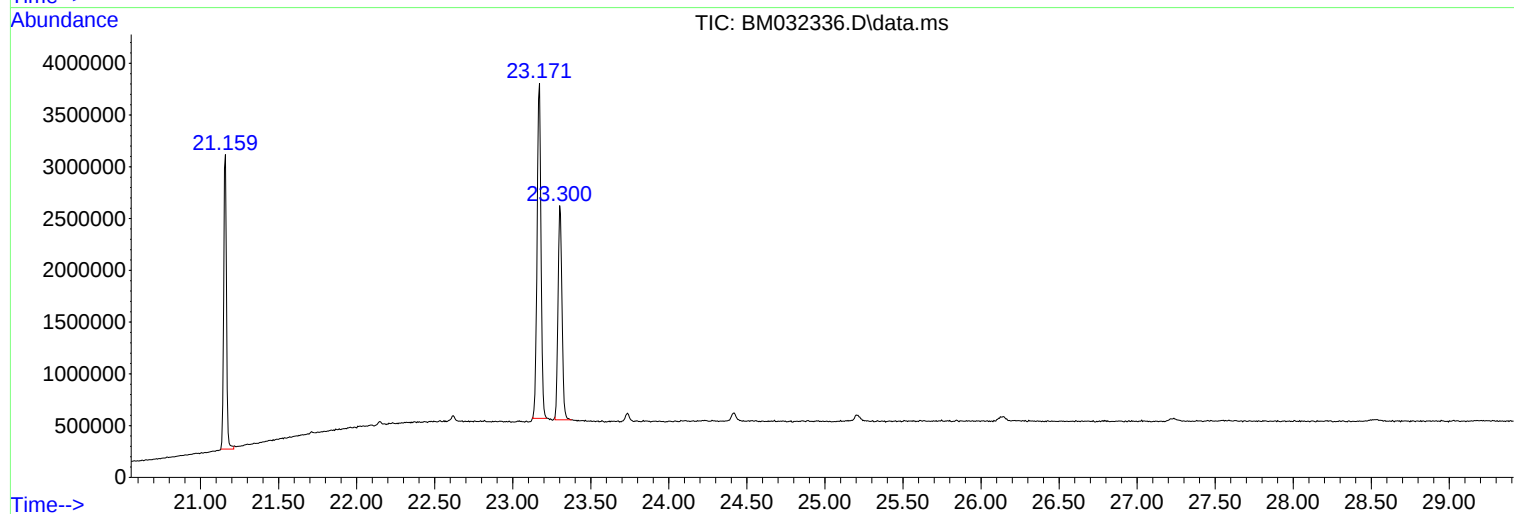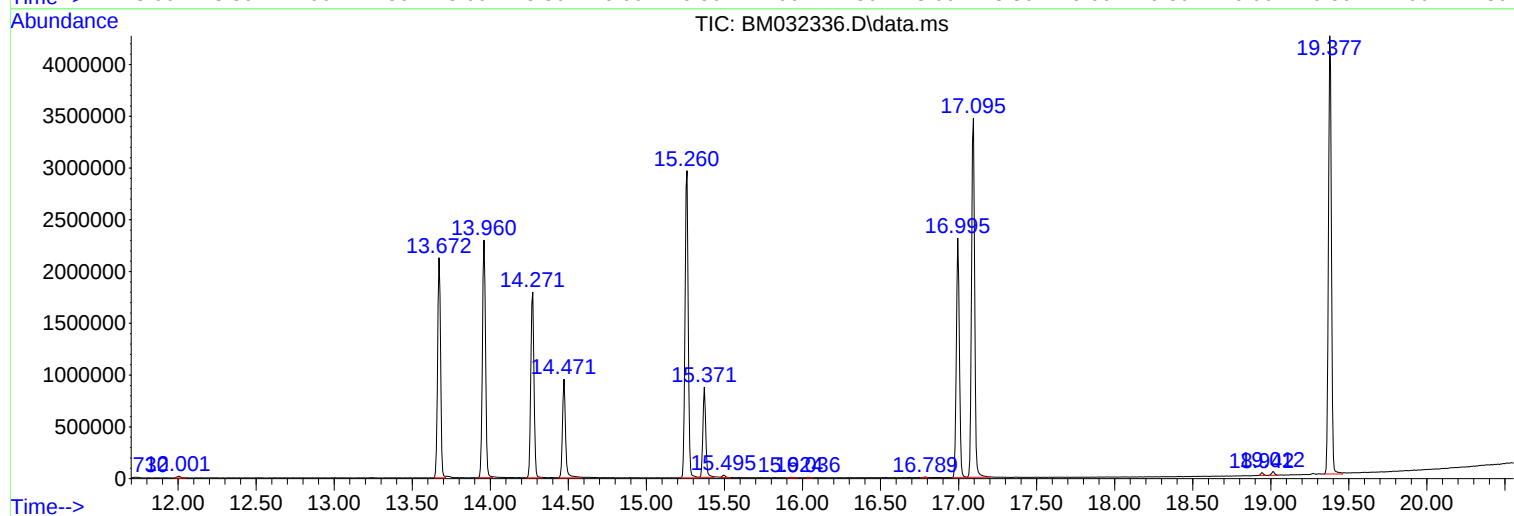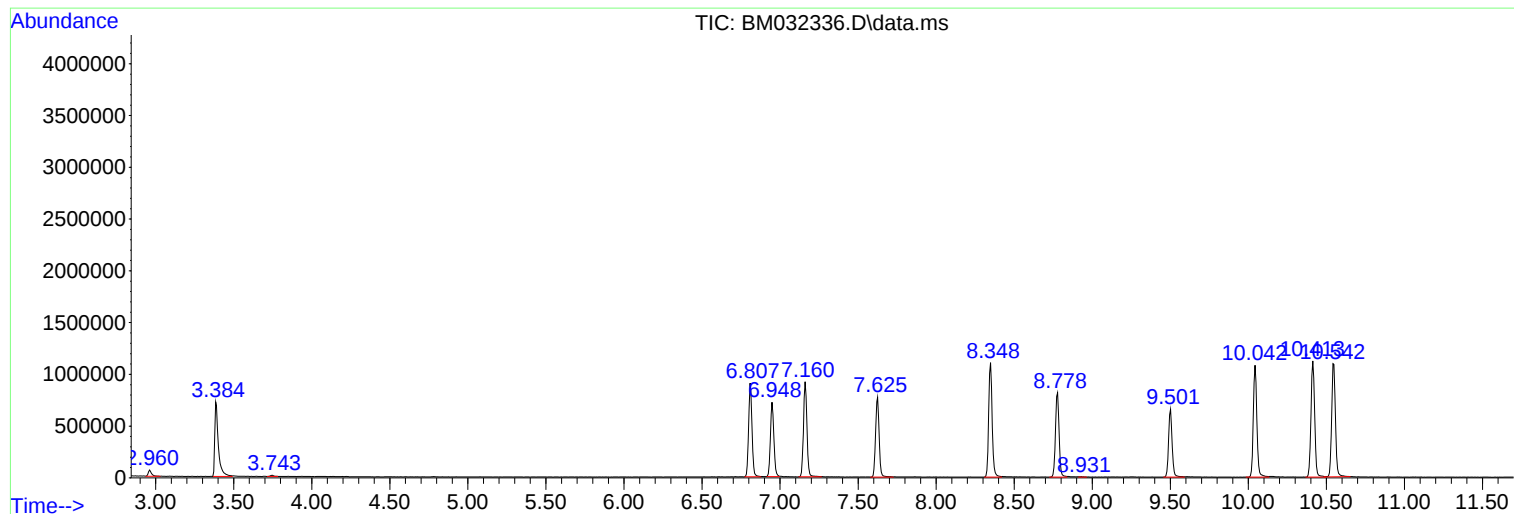

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100621\
Data File : BM032336.D
Acq On : 06 Oct 2021 09:25
Operator : CG/JU
Sample : PB139298BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK298

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100621\
Data File : BM032336.D
Acq On : 06 Oct 2021 09:25
Operator : CG/JU
Sample : PB139298BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK298

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
